


Data Path : Z:\HPCHEM1\BNA E\Data\BE050218\
 Data File : BE096288.D
 Acq On : 2 May 2018 9:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 30 14:27:29 2018

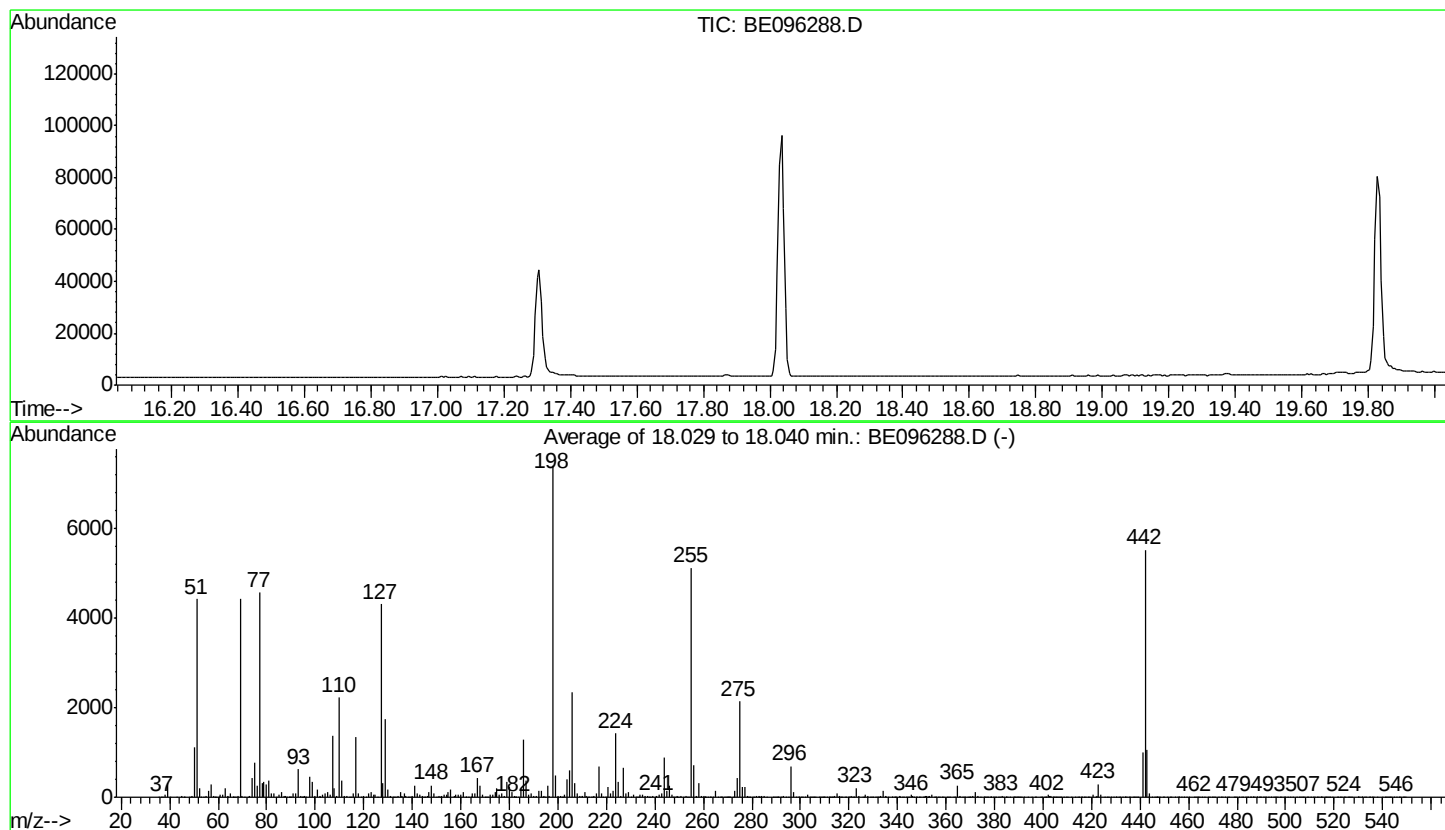

AutoFind: Scans 2628, 2629, 2630; Background Corrected with Scan 2620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.7	4419	PASS
68	69	0.00	2	0.4	17	PASS
69	198	0.00	100	59.7	4422	PASS
70	69	0.00	2	0.9	38	PASS
127	198	10	80	58.3	4313	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	7402	PASS
199	198	5	9	6.5	480	PASS
275	198	10	60	28.9	2137	PASS
365	198	1	100	3.7	272	PASS
441	443	0.01	100	94.8	1001	PASS
442	198	50	100	74.6	5523	PASS
443	442	15	24	19.1	1056	PASS