


Data Path : Z:\HPCHEM1\BNA E\Data\BE050218\
 Data File : BE096305.D
 Acq On : 2 May 2018 21:59
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 30 14:27:29 2018

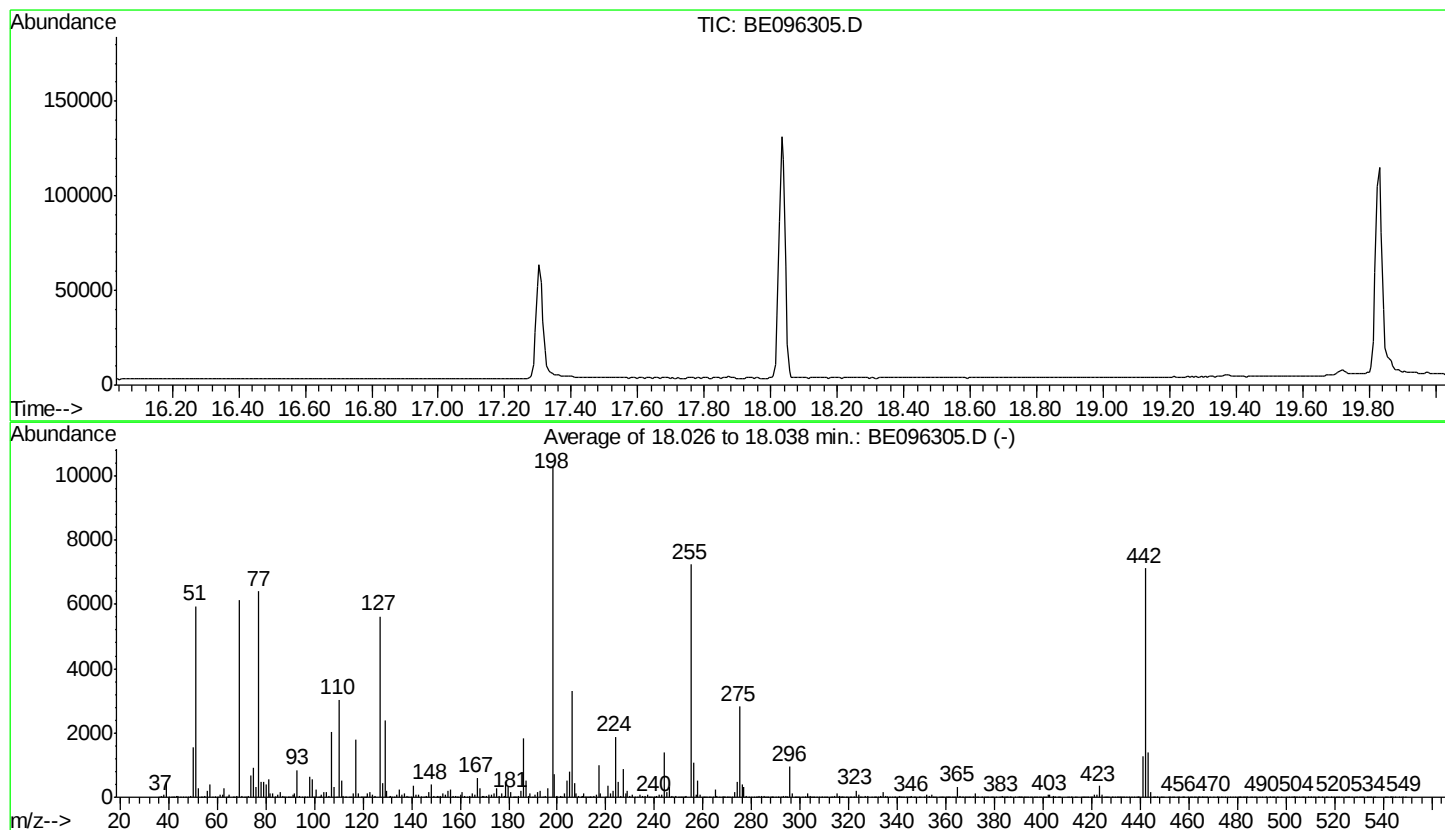

AutoFind: Scans 2627, 2628, 2629; Background Corrected with Scan 2618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.6	5941	PASS
68	69	0.00	2	0.7	41	PASS
69	198	0.00	100	59.3	6120	PASS
70	69	0.00	2	0.5	31	PASS
127	198	10	80	54.5	5623	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10312	PASS
199	198	5	9	6.8	698	PASS
275	198	10	60	27.2	2809	PASS
365	198	1	100	3.2	335	PASS
441	443	0.01	100	90.5	1270	PASS
442	198	50	100	68.9	7110	PASS
443	442	15	24	19.7	1404	PASS