


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE050219\
Data File : BE099491.D
Acq On : 2 May 2019 13:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042919.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 29 18:36:43 2019

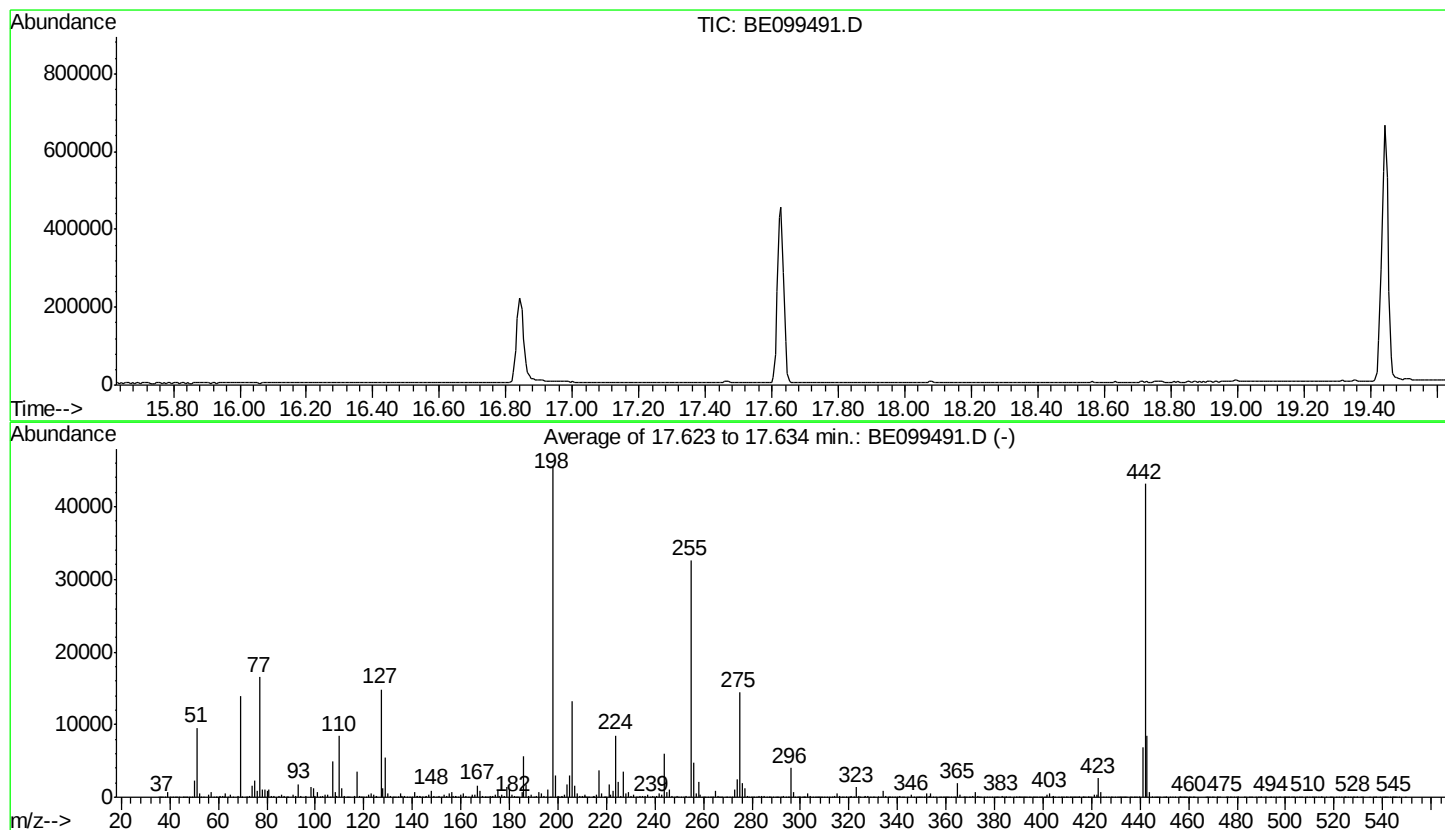

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2550

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.9	9546	PASS
68	69	0.00	2	1.5	204	PASS
69	198	0.00	100	30.5	13947	PASS
70	69	0.00	2	0.4	54	PASS
127	198	10	80	32.5	14841	PASS
197	198	0.00	2	0.2	72	PASS
198	198	100	100	100.0	45657	PASS
199	198	5	9	6.6	2999	PASS
275	198	10	60	31.5	14379	PASS
365	198	1	100	4.2	1899	PASS
441	198	0.01	100	15.2	6935	PASS
442	198	50	100	94.6	43171	PASS
443	442	15	24	19.5	8435	PASS