


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE050219\
 Data File : BE099510.D
 Acq On : 3 May 2019 1:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 29 18:36:43 2019

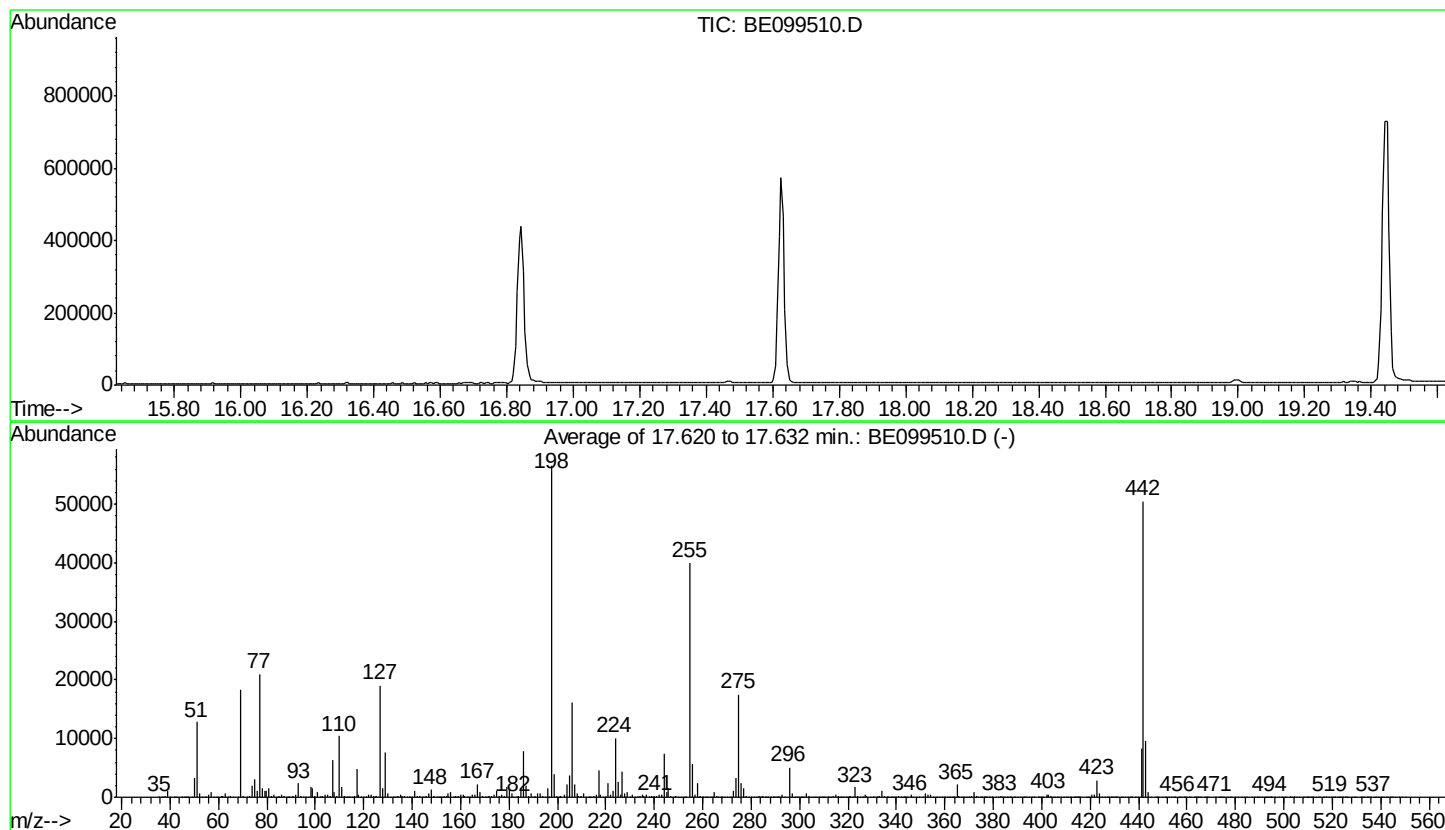

AutoFind: Scans 2558, 2559, 2560; Background Corrected with Scan 2550

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.7	12846	PASS
68	69	0.00	2	0.6	105	PASS
69	198	0.00	100	32.5	18400	PASS
70	69	0.00	2	0.9	161	PASS
127	198	10	80	33.7	19039	PASS
197	198	0.00	2	0.2	101	PASS
198	198	100	100	100.0	56579	PASS
199	198	5	9	7.1	4044	PASS
275	198	10	60	31.0	17515	PASS
365	198	1	100	3.8	2129	PASS
441	198	0.01	100	14.5	8204	PASS
442	198	50	100	89.2	50480	PASS
443	442	15	24	19.2	9699	PASS