
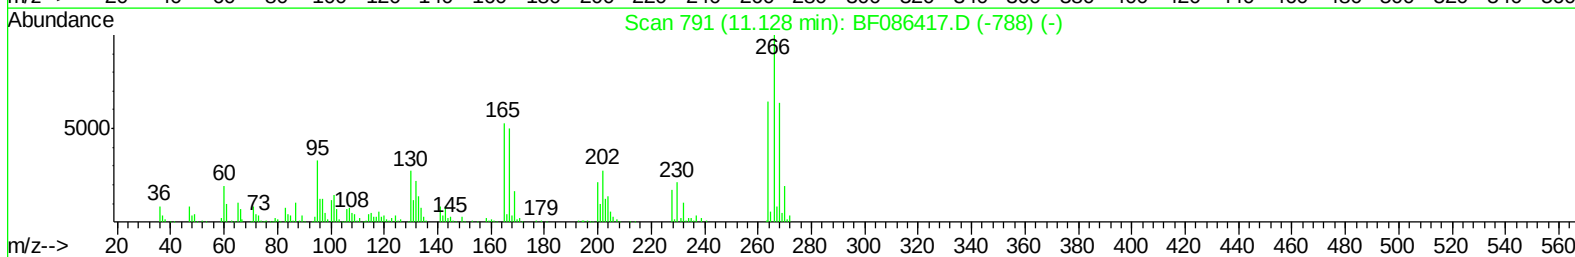
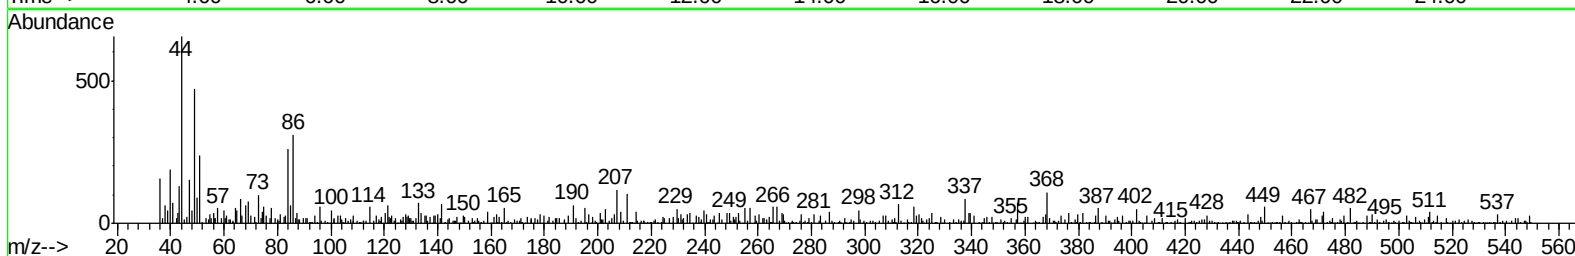


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE050316\
Data File : BE091740.D
Acq On : 3 May 2016 12:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 01:54:06 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

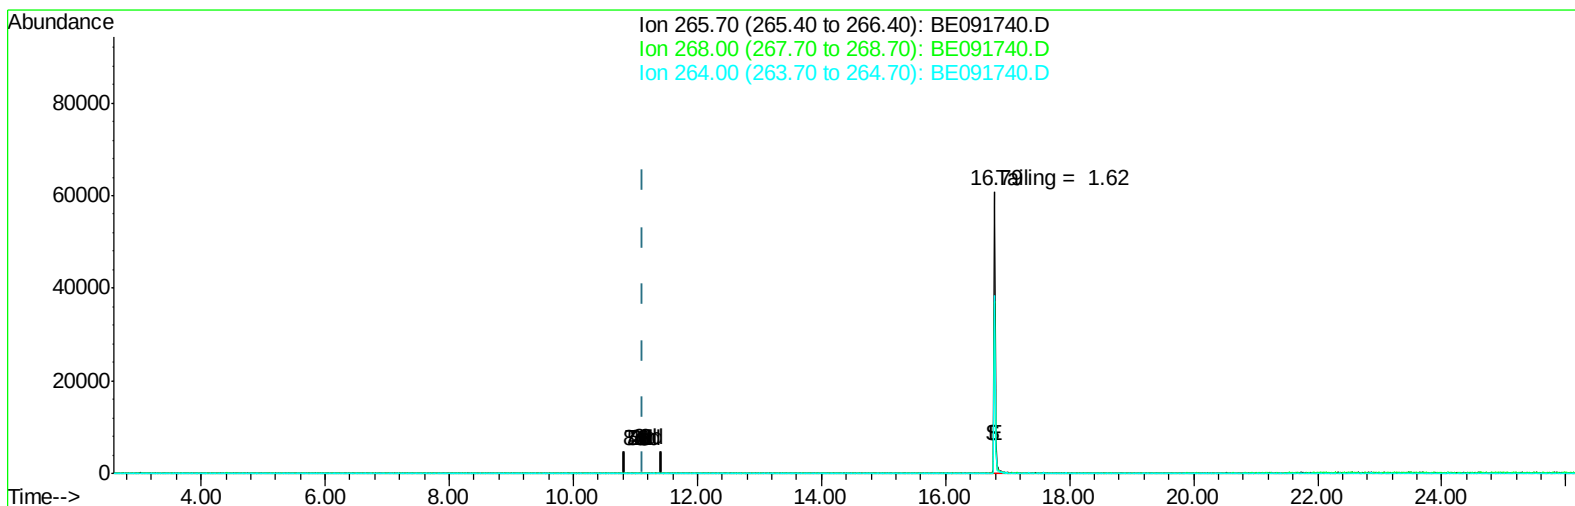

TIC: BE091740.D

(69) Pentachlorophenol (C)




11.130min (+0.003) 302.90ng

response 40

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	14.04#
264.00	66.10	38.60#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE050316\
Data File : BE091740.D
Acq On : 3 May 2016 12:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 01:54:06 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

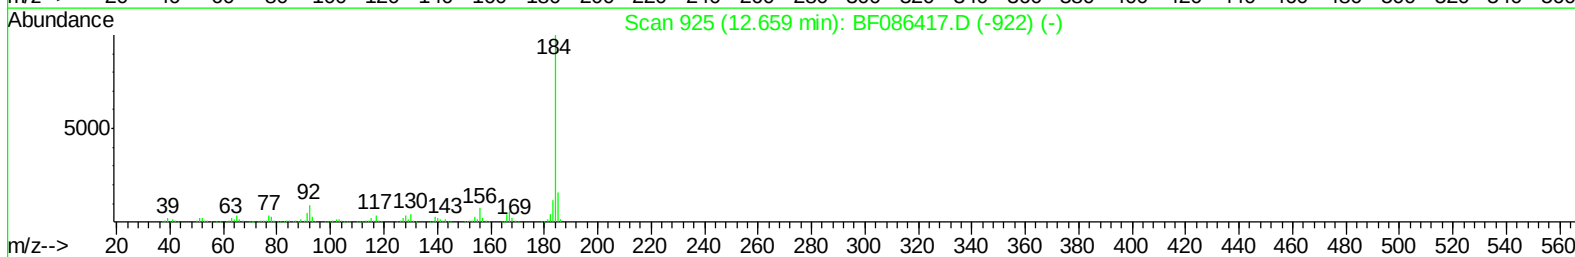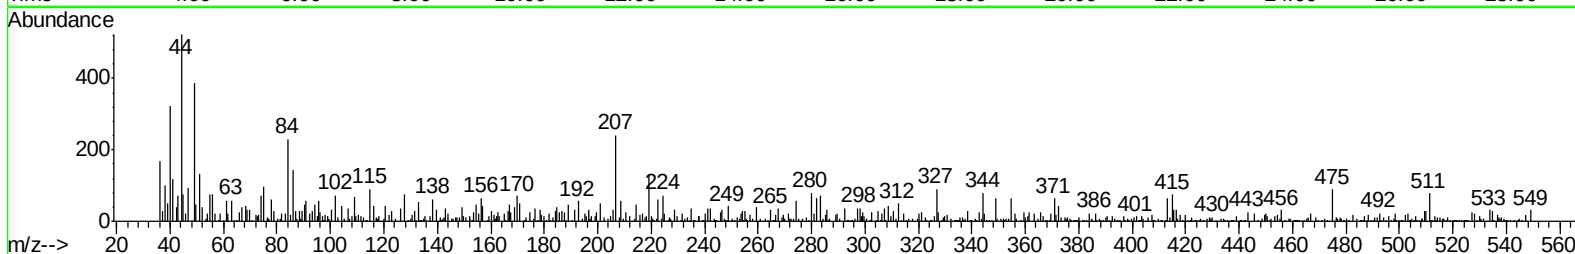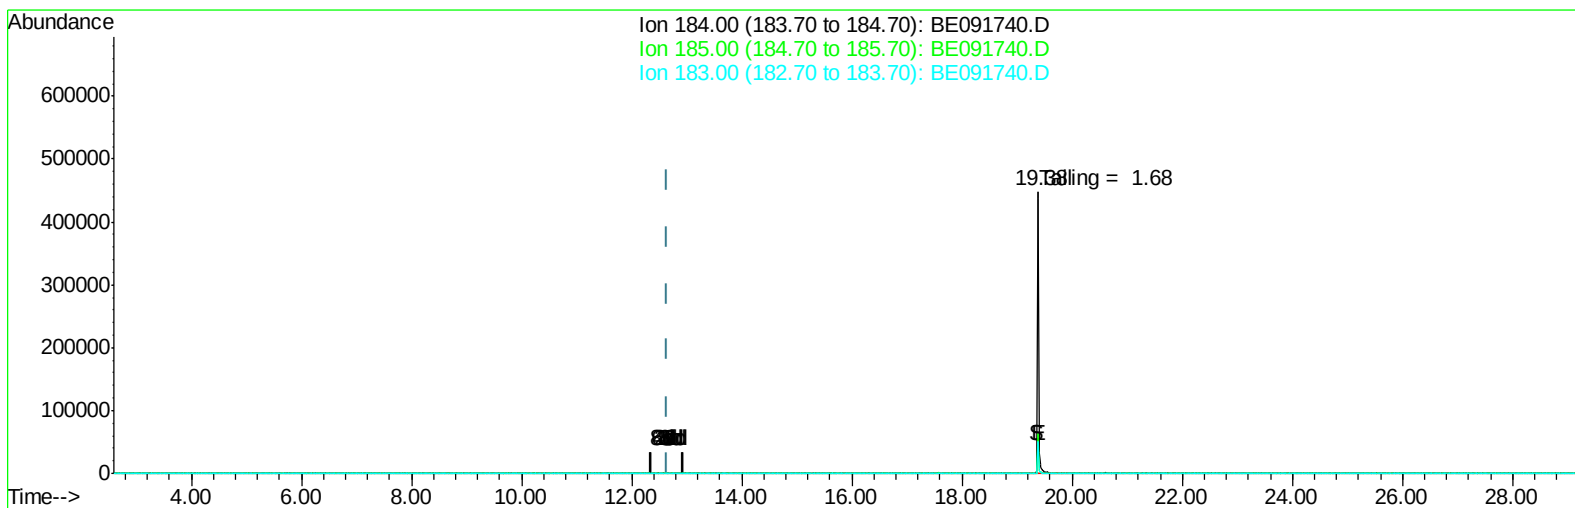

TIC: BE091740.D

(76) Benzidine

12.670min (+0.010) 77.98ng

response 67

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	36.62#
183.00	12.20	14.08
0.00	0.00	0.00