


Data Path : Z:\HPCHEM1\BNA E\Data\BE050316\
 Data File : BE091740.D
 Acq On : 3 May 2016 12:20
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 26 16:09:46 2016

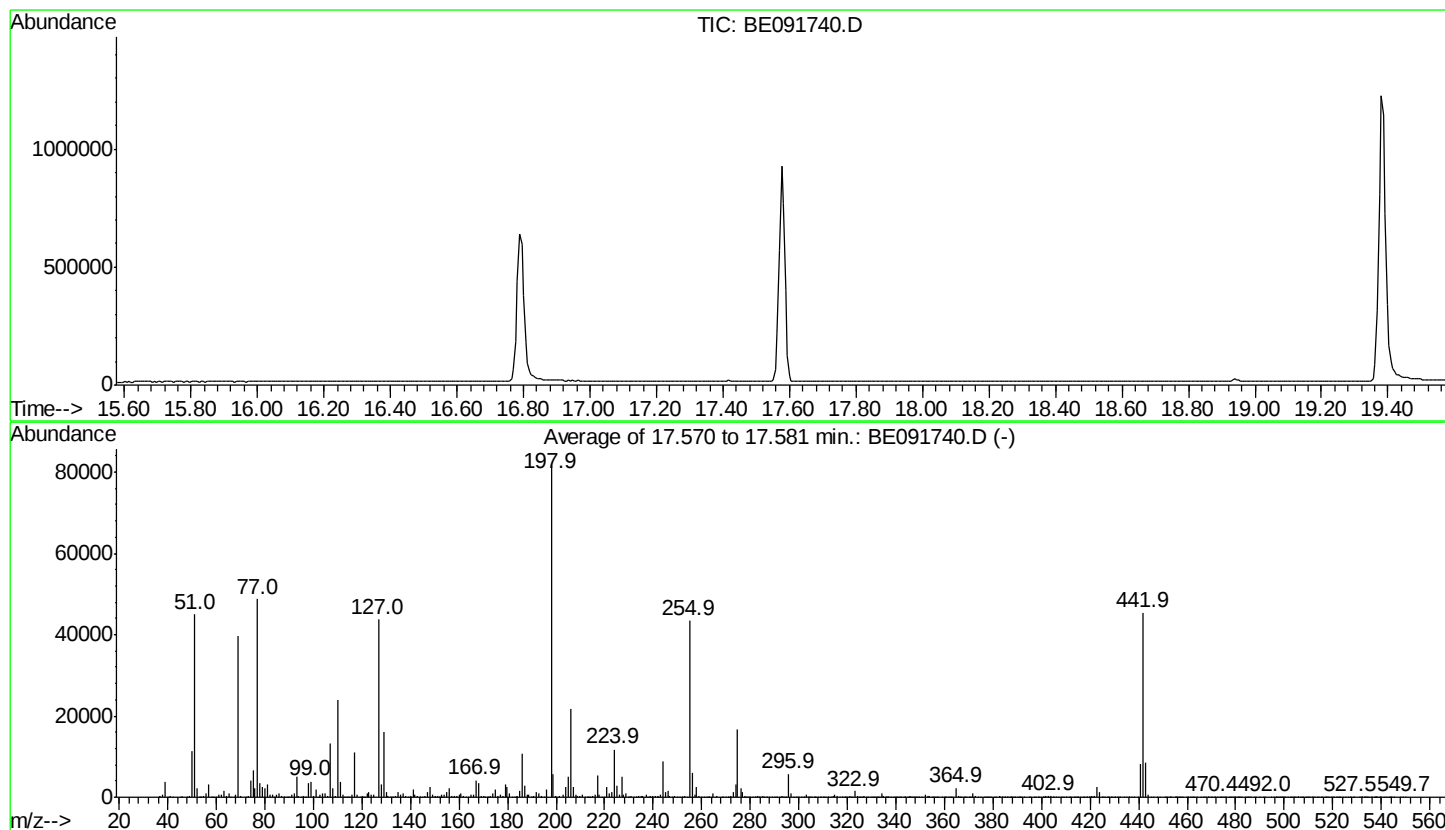

AutoFind: Scans 2550, 2551, 2552; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	44906	PASS
68	69	0.00	2	1.6	626	PASS
69	198	0.00	100	48.5	39578	PASS
70	69	0.00	2	0.6	251	PASS
127	198	10	80	53.6	43725	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81603	PASS
199	198	5	9	6.9	5622	PASS
275	198	10	60	20.5	16701	PASS
365	198	1	100	2.8	2260	PASS
441	442	0.01	24	18.2	8269	PASS
442	198	50	100	55.7	45434	PASS
443	442	15	24	19.0	8626	PASS