

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
 Data File : BE096327.D
 Acq On : 3 May 2018 17:36
 Operator : SJ/JU
 Sample : PB108484BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: May 04 01:55:13 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 04 01:53:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	591	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	2572	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.94	164	1629	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.75	188	315220	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.74
20) Perylene-d12	24.35	264	4746	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.73	152	1632	0.35	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	24.18	252	1277	0.084	ng/ul#	Ovalue 89




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096327.D
Acq On : 3 May 2018 17:36
Operator : SJ/JU
Sample : PB108484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: May 04 01:55:13 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

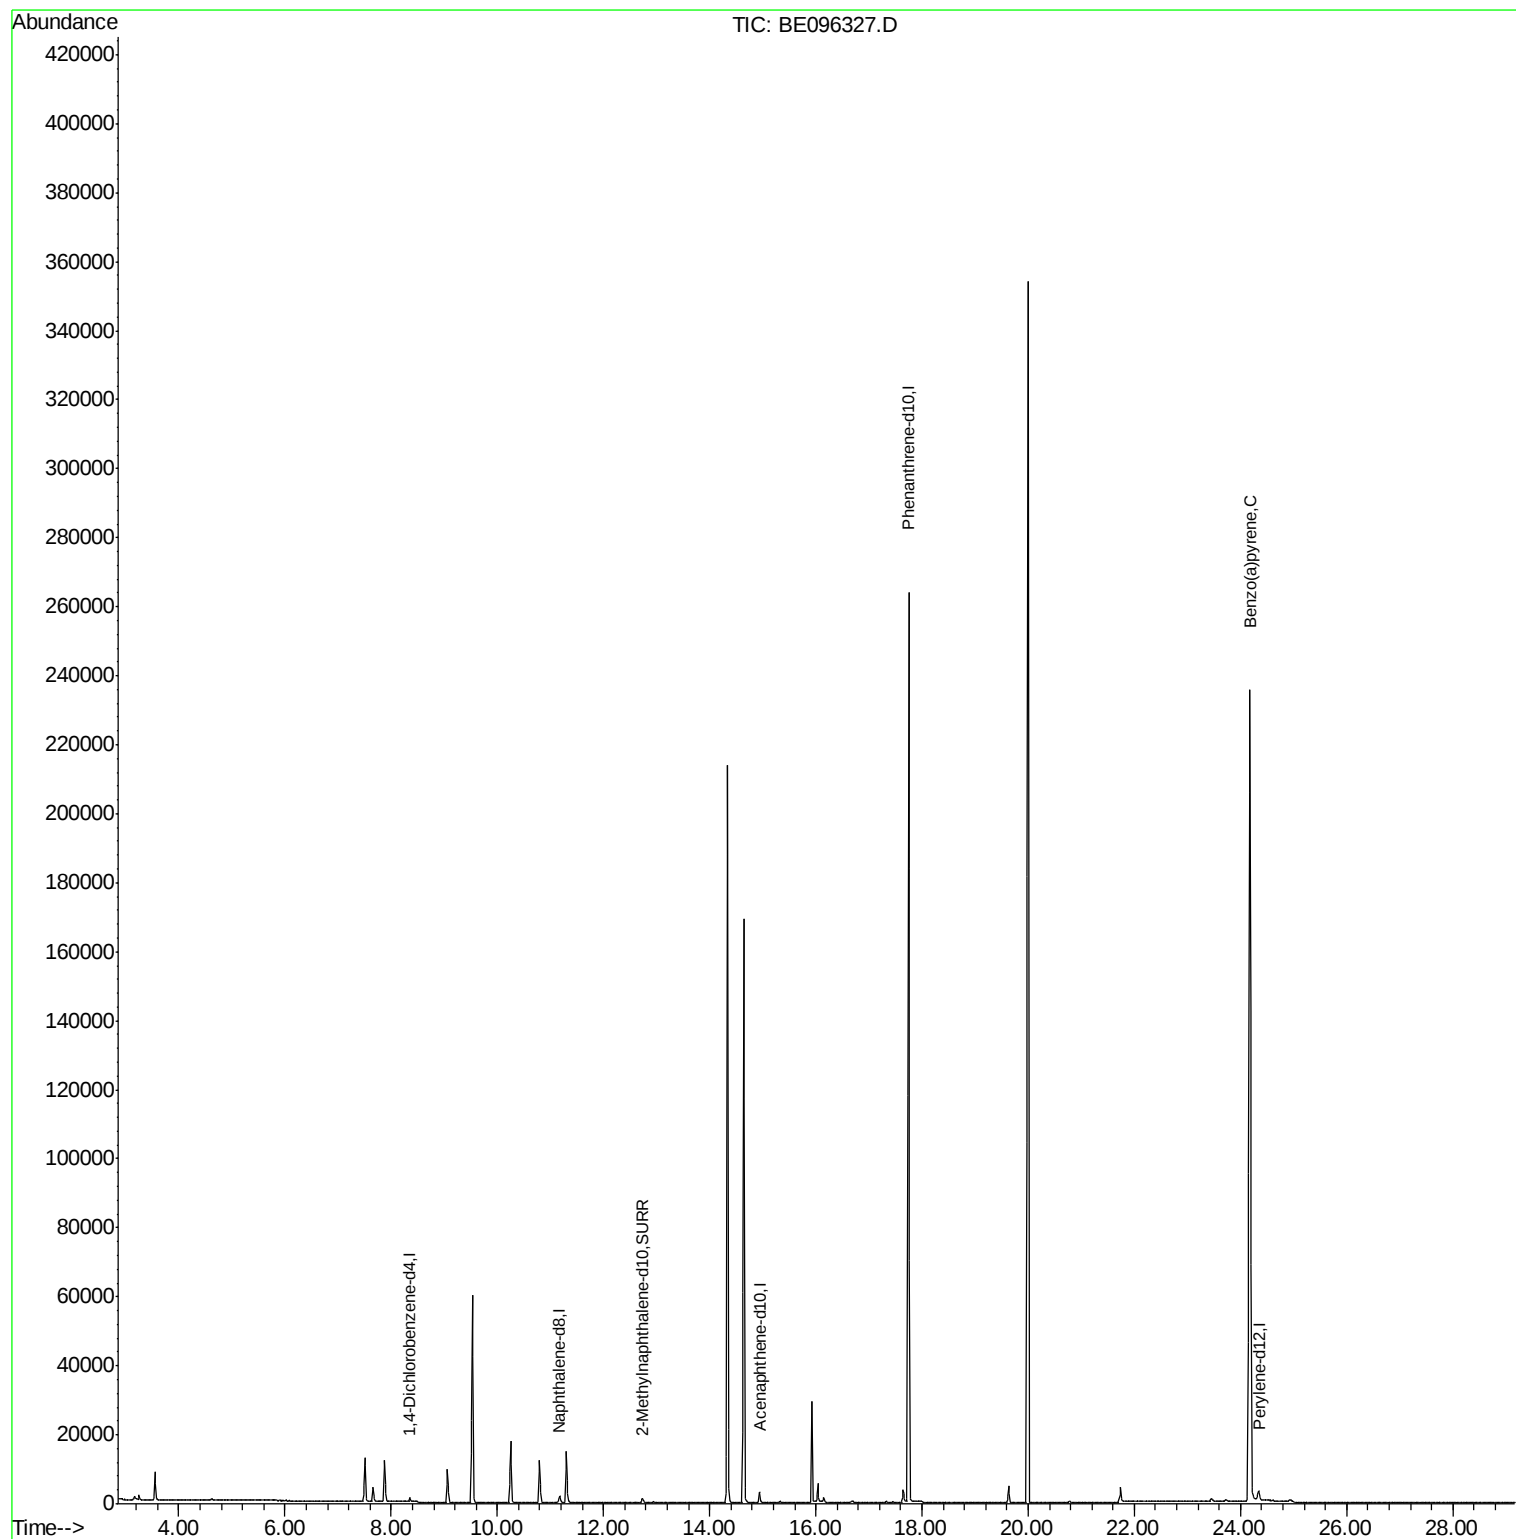

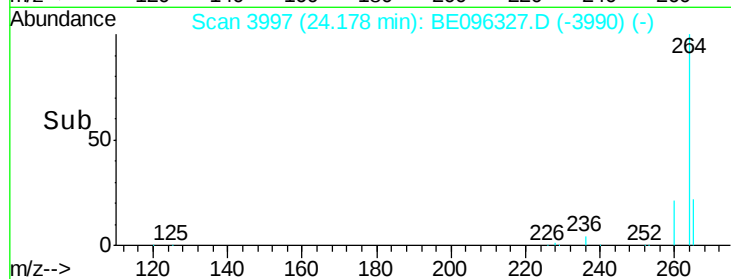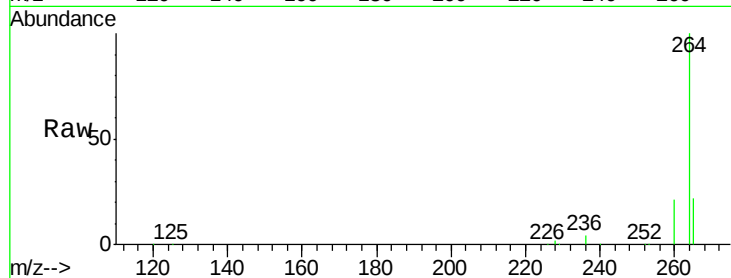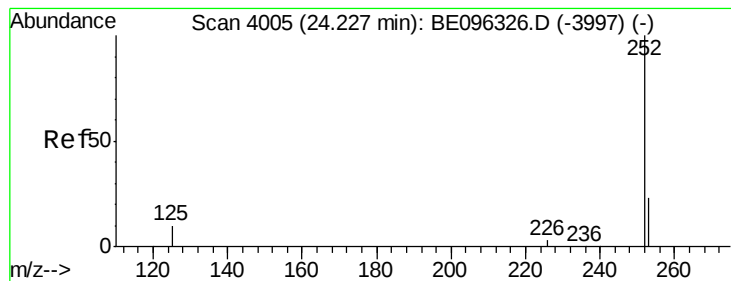

#23

Benzo(a)pyrene

Concen: 0.084 ng/ul

RT: 24.18 min Scan# 3997

Delta R.T. -0.05 min

Lab File: BE096327.D

Acq: 3 May 2018 17:36

Instrument :

BNA_E

ClientSampleId :

Tot Ion:	252	Resp:	1277
Ion	Ratio	Lower	Upper
252	100		
253	38.2	28.5	42.7
125	33.0	18.1	27.1

