

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
 Data File : BE096331.D
 Acq On : 3 May 2018 20:03
 Operator : SJ/JU
 Sample : J2440-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: May 04 01:55:56 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 04 01:53:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	640	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	2723	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.94	164	1773	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.75	188	276656	0.40	ng/ul	0.10
16) Chrysene-d12	21.88	240	7	0.40	ng/ul	0.14
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-24.35
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.73	152	1442	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	20.26	202	29	3.683	ng/ul#	1
18) Benzo(a)anthracene	21.92	228	32	2.927	ng/ul#	1
19) Chrysene	21.92	228	32	1.531	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096331.D
Acq On : 3 May 2018 20:03
Operator : SJ/JU
Sample : J2440-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: May 04 01:55:56 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

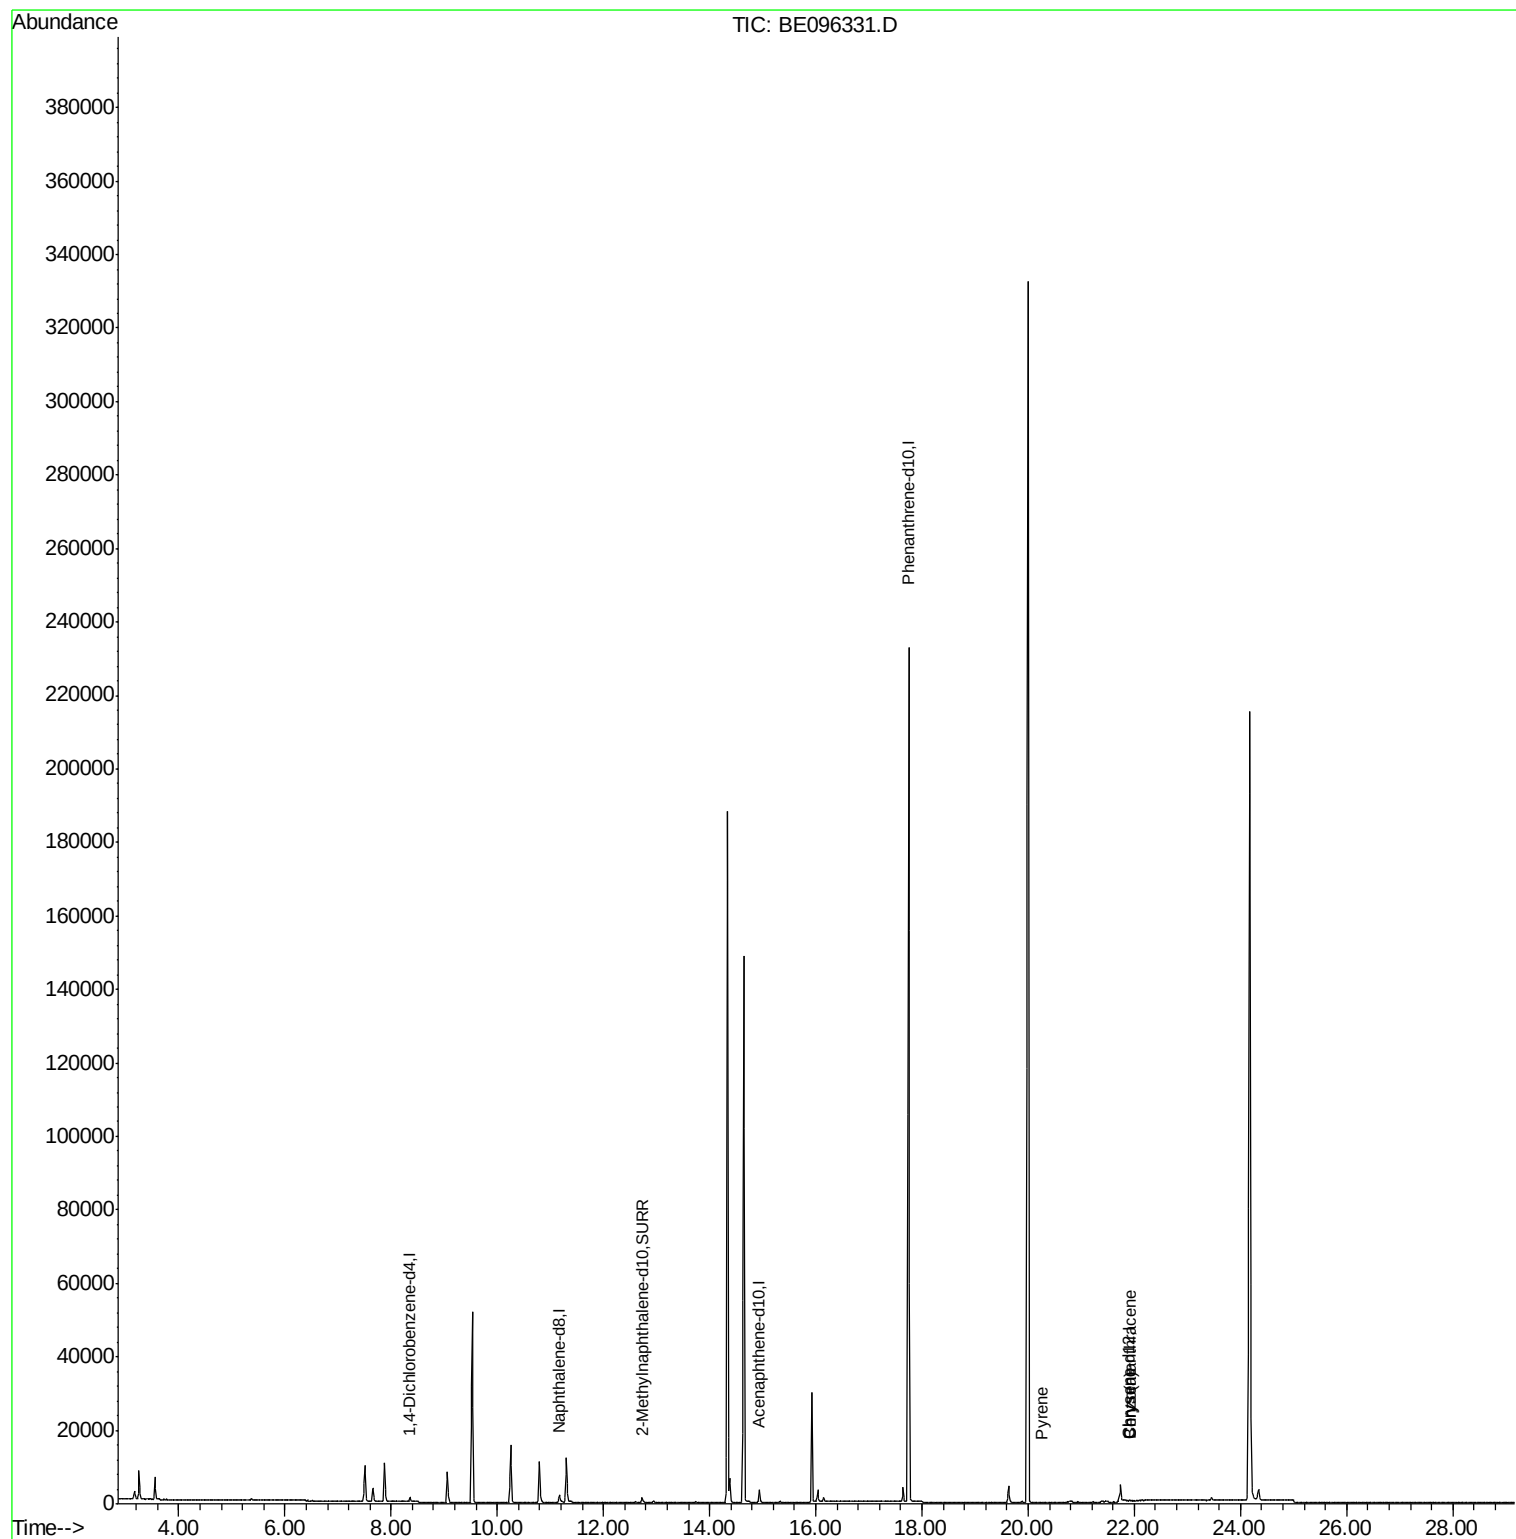

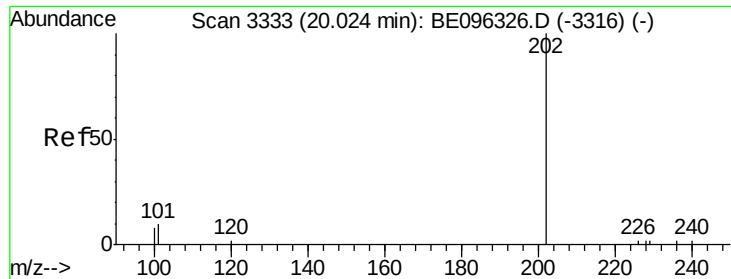

#17

Pvrene

Concen: 3.683 ng/ul

RT: 20.26 min Scan# 3377

Delta R.T. 0.23 min

Lab File: BE096331.D

Acq: 3 May 2018 20:03

Instrument :

BNA_E

ClientSampleId :





Tot Ion:202 Resp: 29

Ion Ratio Lower Upper

202 100

101 78.3 18.2 27.4#

100 78.3 15.6 23.4#

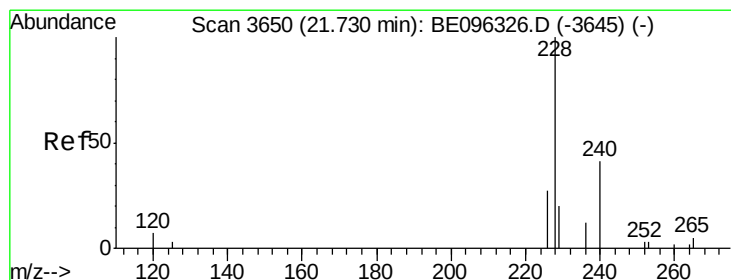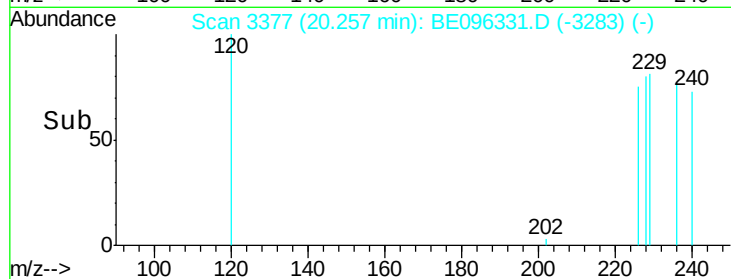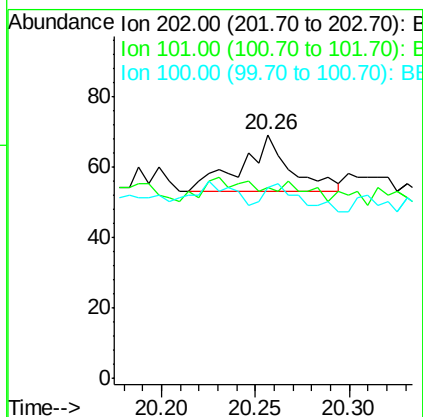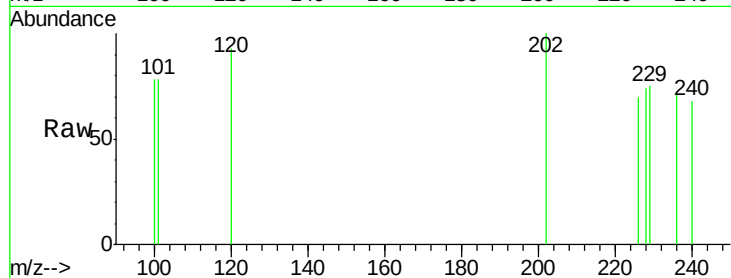

#18

Benzo(a)anthracene

Concen: 2.927 ng/ul

RT: 21.92 min Scan# 3677

Delta R.T. 0.19 min

Lab File: BE096331.D

Acq: 3 May 2018 20:03




Tgt Ion:228 Resp: 32




Ion Ratio Lower Upper

228 100

229 100.0 22.8 34.2#

226 96.8 17.0 25.6#

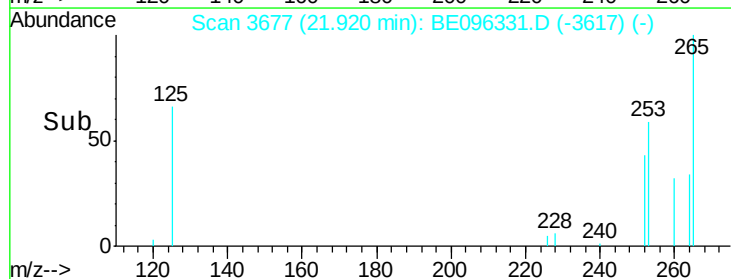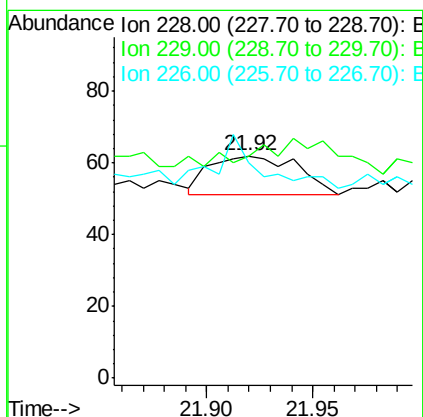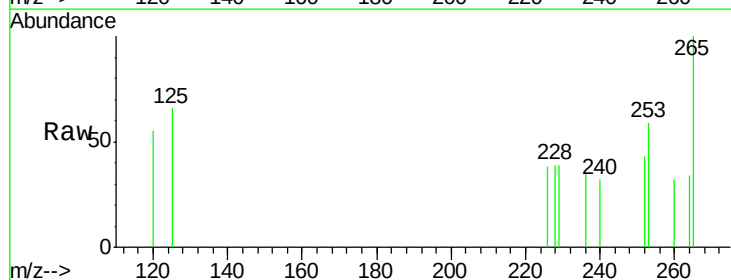

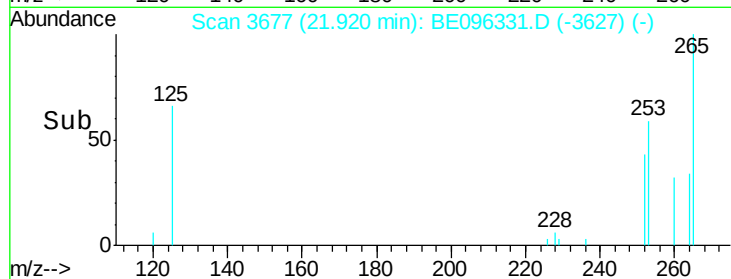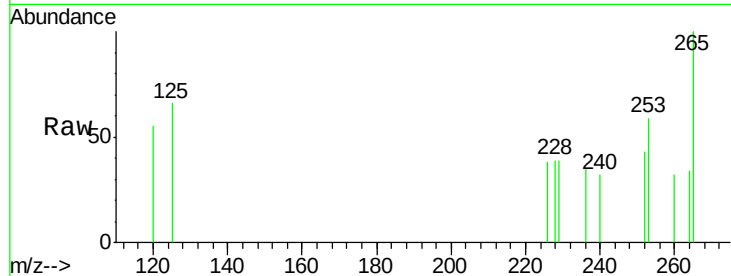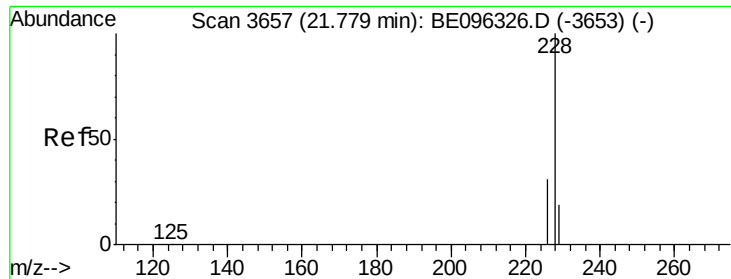

#19

Chrysene

Concen: 1.531 ng/ul

RT: 21.92 min Scan# 3677

Delta R.T. 0.14 min

Lab File: BE096331.D

Acq: 3 May 2018 20:03

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 228 Resp: 32

Ion Ratio Lower Upper

228 100

226 96.8 23.4 35.0#

229 100.0 17.7 26.5#

