

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
 Data File : BE096332.D
 Acq On : 3 May 2018 20:41
 Operator : SJ/JU
 Sample : J2440-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: May 04 01:56:04 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 04 01:53:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	611	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	2622	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.94	164	1704	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.75	188	230323	0.40	ng/ul	0.10
16) Chrysene-d12	21.92	240	5	0.40	ng/ul	0.18
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-24.35
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.73	152	1168	0.25	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	20.06	202	10	1.778	ng/ul#	1
18) Benzo(a)anthracene	21.91	228	45	5.762	ng/ul#	1
19) Chrysene	21.91	228	45	3.014	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096332.D
Acq On : 3 May 2018 20:41
Operator : SJ/JU
Sample : J2440-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: May 04 01:56:04 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration




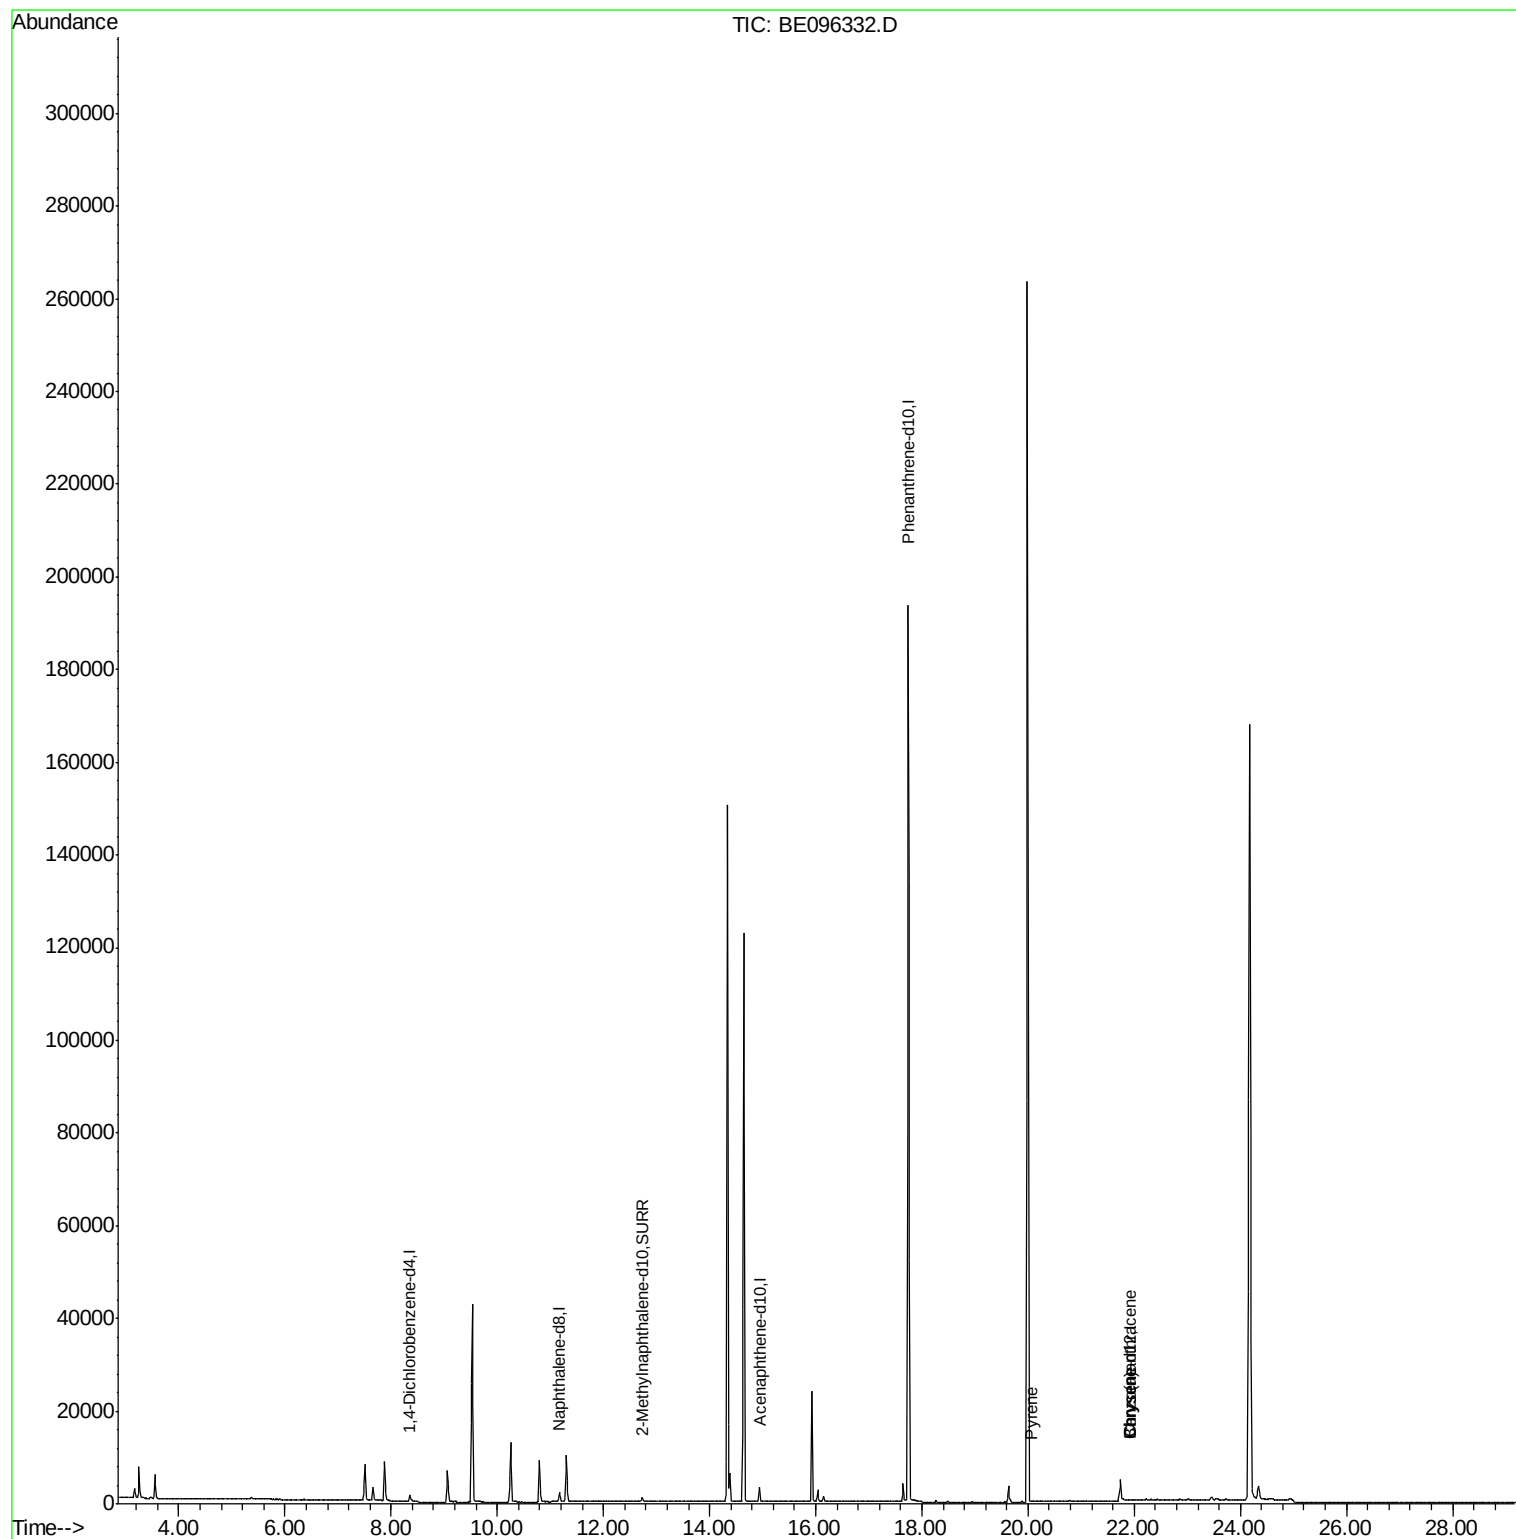


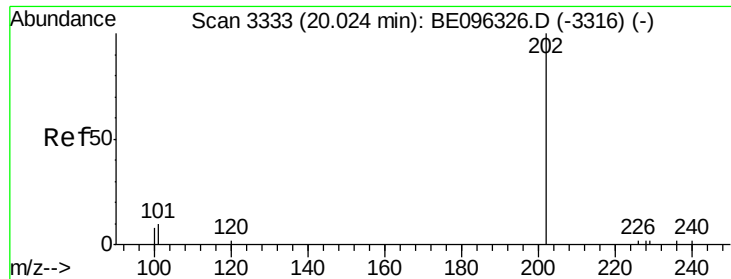

#17
Pvrene
Concen: 1.778 ng/ul
RT: 20.06 min Scan# 3340
Delta R.T. 0.04 min
Lab File: BE096332.D
Acq: 3 May 2018 20:41




Instrument :
BNA_E
ClientSampleId :




Tot Ion:202 Resp: 10
Ion Ratio Lower Upper
202 100
101 85.2 18.2 27.4#
100 88.5 15.6 23.4#

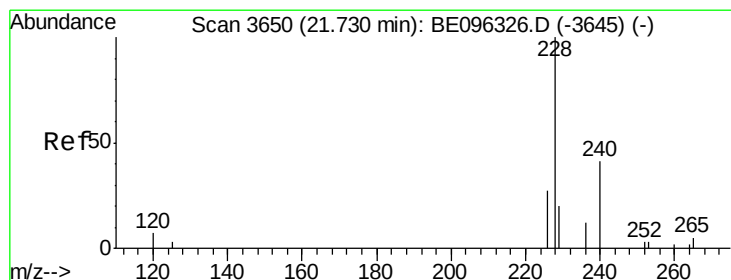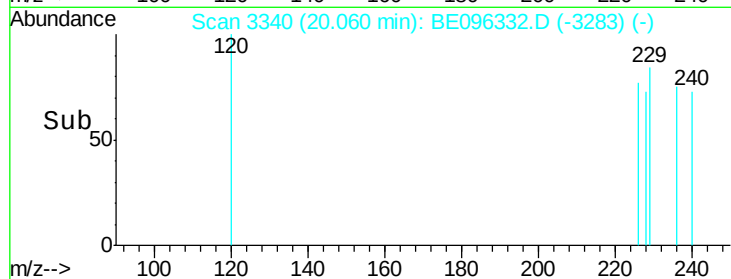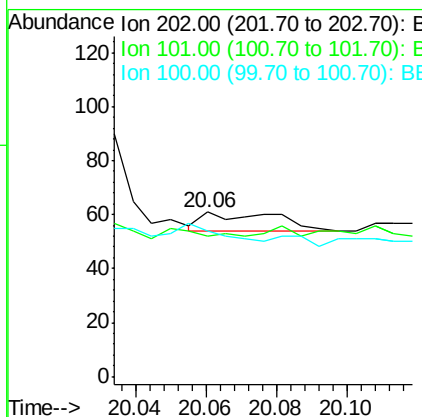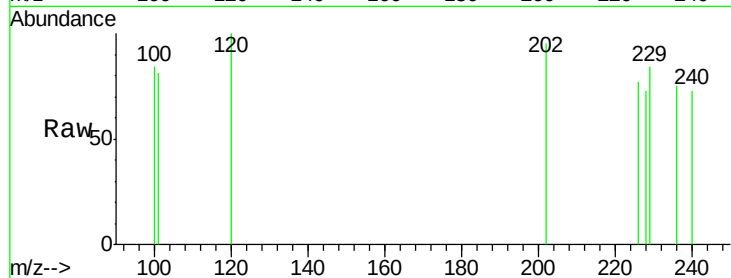

#18
Benzo(a)anthracene
Concen: 5.762 ng/ul
RT: 21.91 min Scan# 3676
Delta R.T. 0.18 min
Lab File: BE096332.D
Acq: 3 May 2018 20:41

Tgt Ion:228 Resp: 45
Ion Ratio Lower Upper
228 100
229 91.0 22.8 34.2#
226 97.0 17.0 25.6#

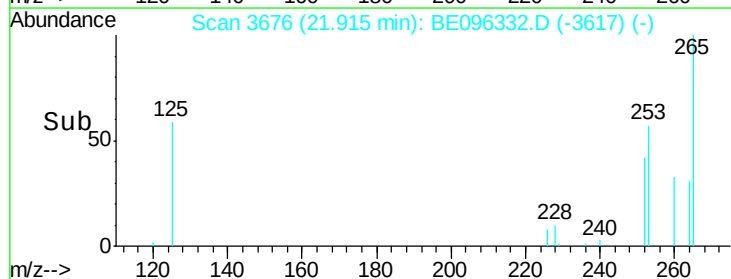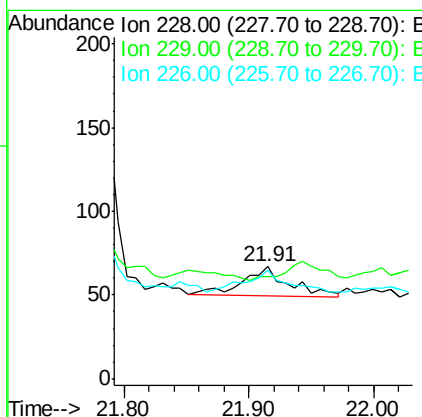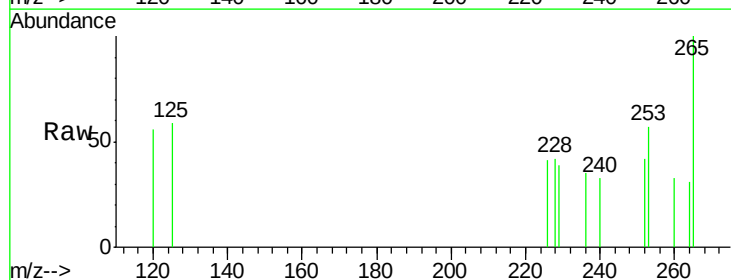

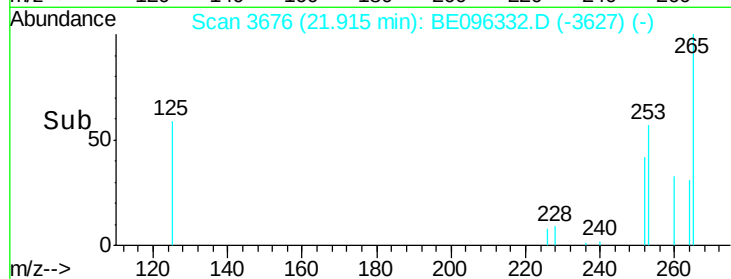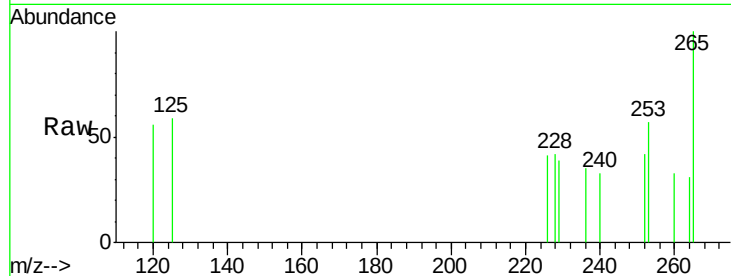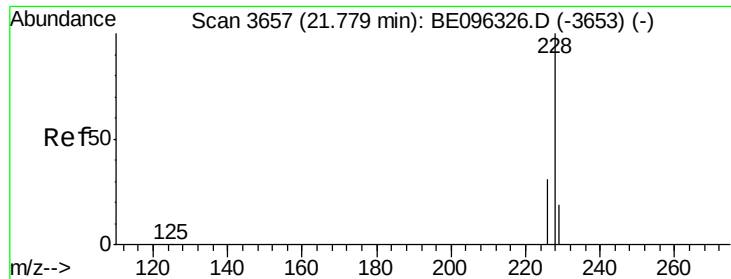

#19

Chrysene

Concen: 3.014 ng/ul

RT: 21.91 min Scan# 3676

Delta R.T. 0.14 min

Lab File: BE096332.D

Acq: 3 May 2018 20:41

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 228 Resp: 45

Ion Ratio Lower Upper

228 100

226 97.0 23.4 35.0#

229 91.0 17.7 26.5#

