

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
 Data File : BE096338.D
 Acq On : 4 May 2018 00:19
 Operator : SJ/JU
 Sample : J2440-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: May 04 01:57:00 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 04 01:53:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	710	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	3076	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.94	164	1952	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.75	188	216041	0.40	ng/ul	0.10
16) Chrysene-d12	21.83	240	24	0.40	ng/ul	0.09
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-24.35
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.73	152	1274	0.23	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds				Ovalue		
17) Pyrene	20.08	202	157	5.816	ng/ul#	63
18) Benzo(a)anthracene	21.73	228	3552	94.747	ng/ul#	74
19) Chrysene	21.91	228	204	2.847	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096338.D
Acq On : 4 May 2018 00:19
Operator : SJ/JU
Sample : J2440-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: May 04 01:57:00 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration




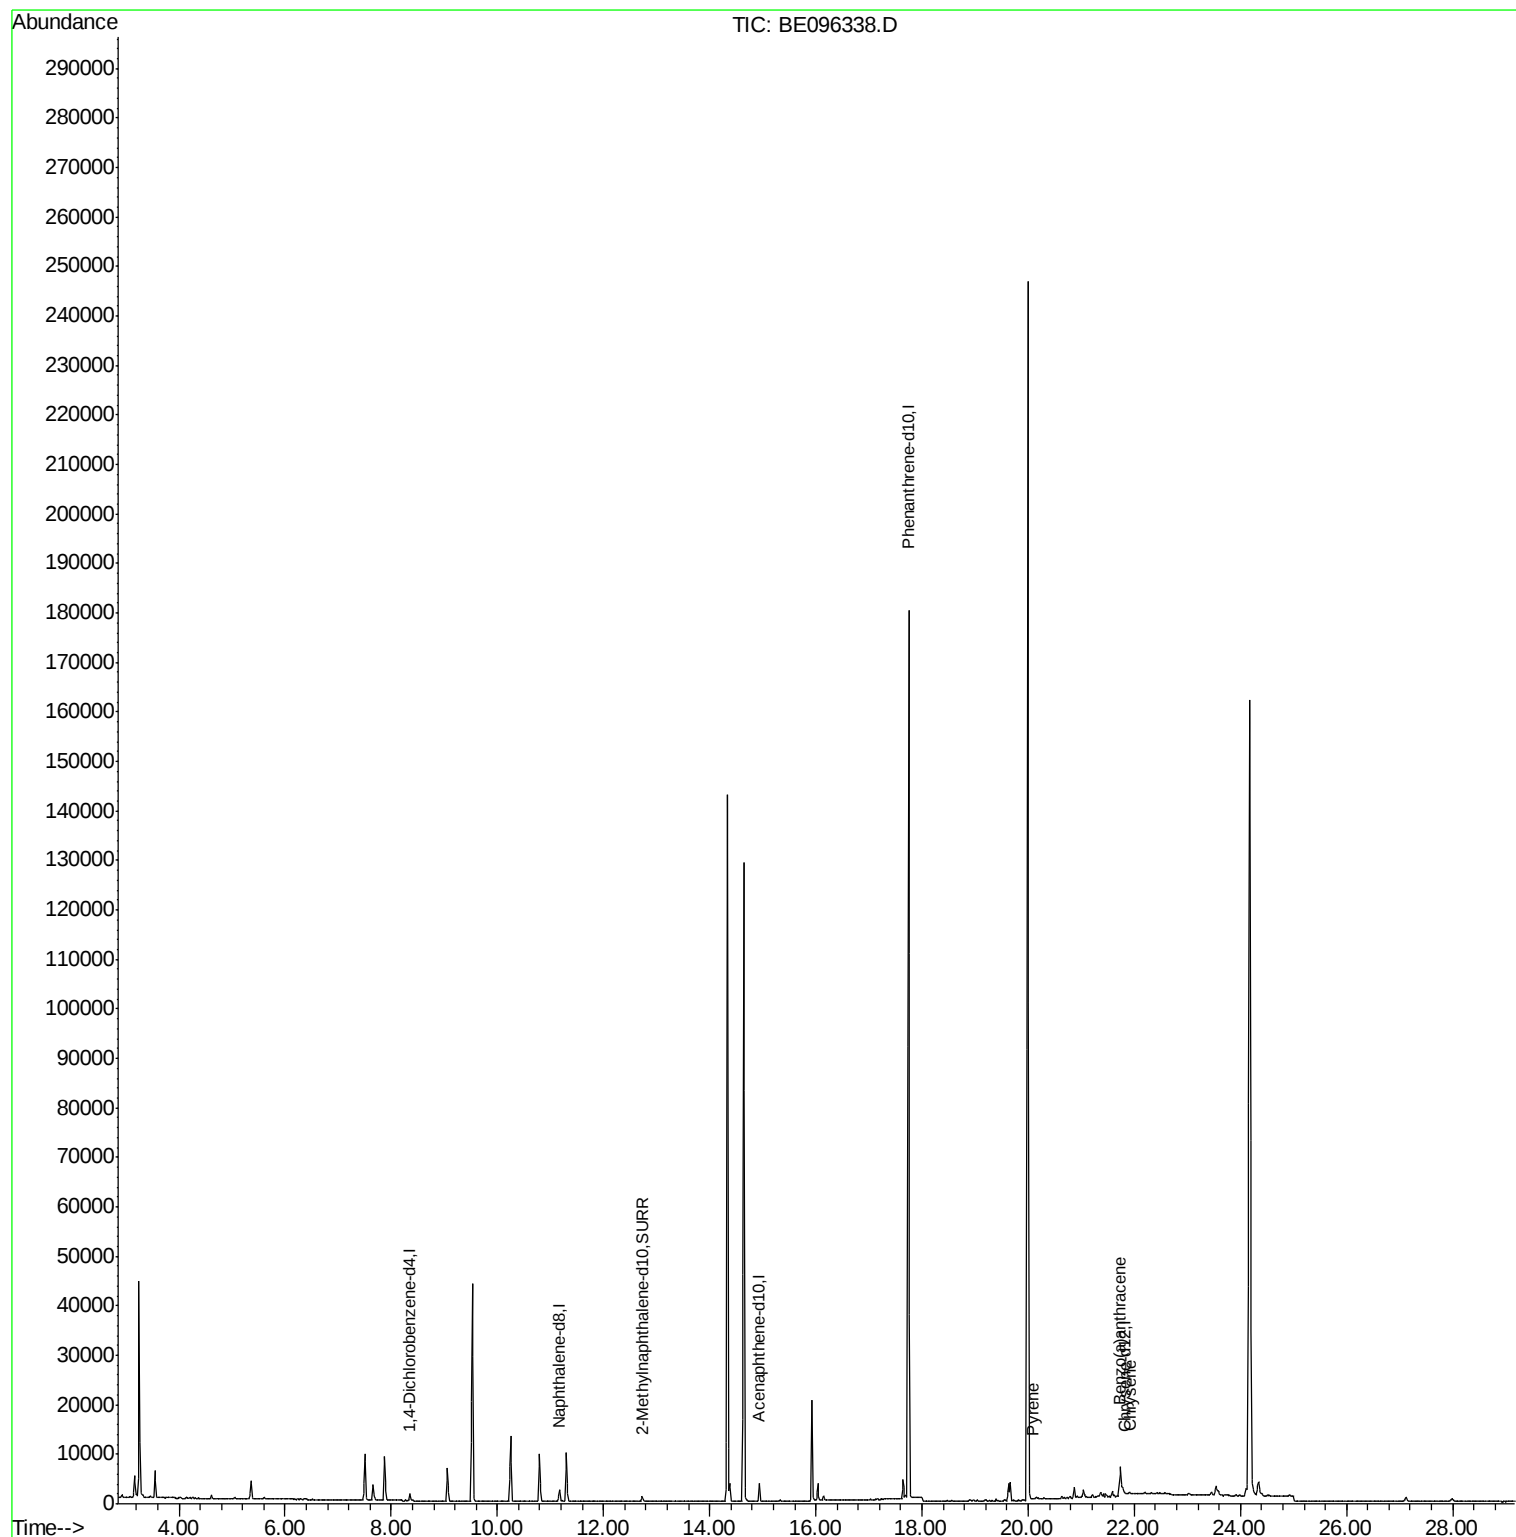


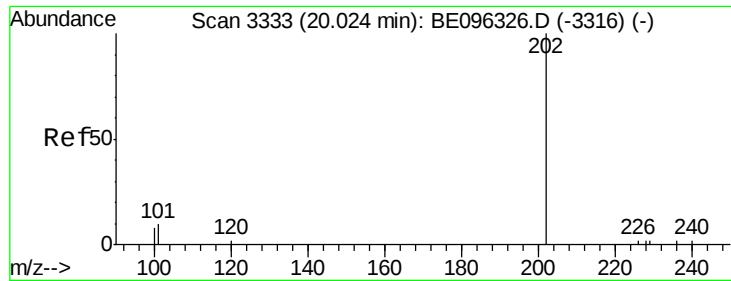

#17
Pvrene
Concen: 5.816 ng/ul
RT: 20.08 min Scan# 3344
Delta R.T. 0.05 min
Lab File: BE096338.D
Acq: 4 May 2018 00:19




Instrument :
BNA_E
ClientSampled :




Tot Ion:202 Resp: 157
Ion Ratio Lower Upper
202 100
101 48.7 18.2 27.4#
100 27.8 15.6 23.4#

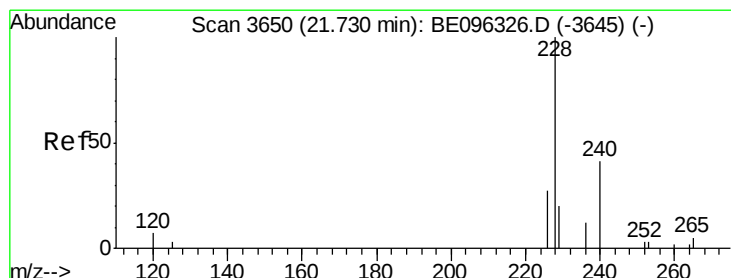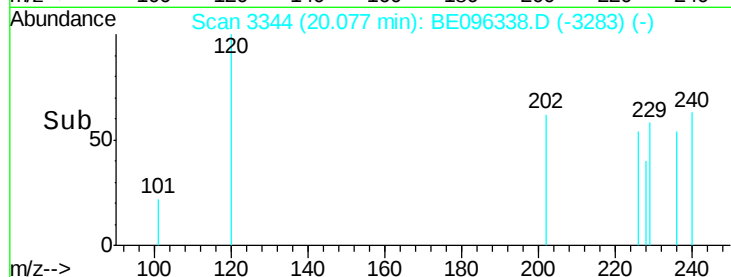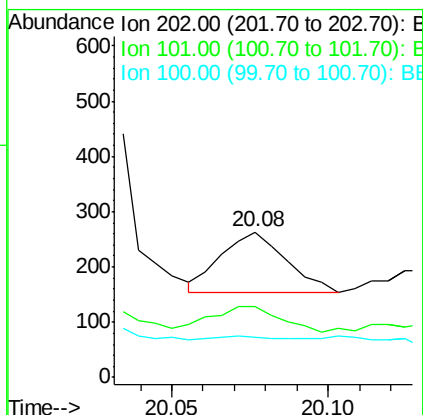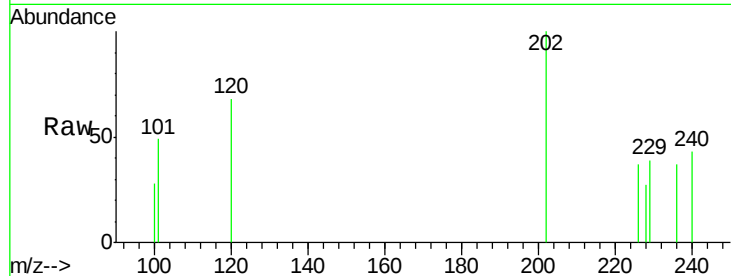

#18
Benzo(a)anthracene
Concen: 94.747 ng/ul
RT: 21.73 min Scan# 3651
Delta R.T. 0.00 min
Lab File: BE096338.D
Acq: 4 May 2018 00:19

Tgt Ion:228 Resp: 3552
Ion Ratio Lower Upper
228 100
229 40.6 22.8 34.2#
226 36.0 17.0 25.6#

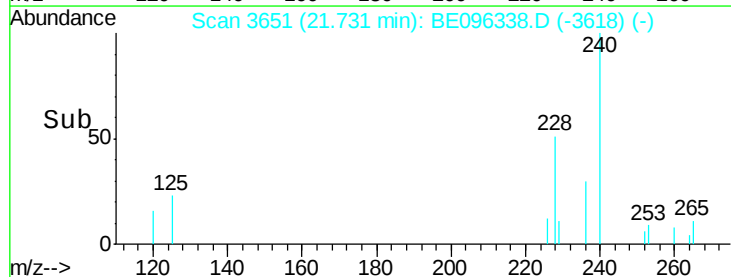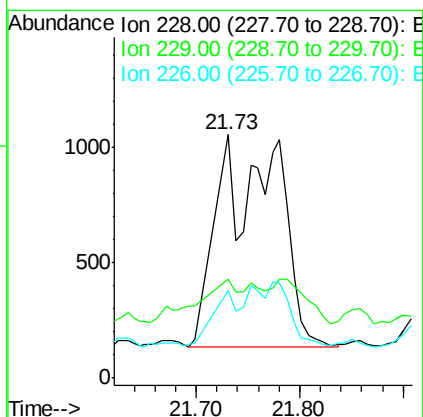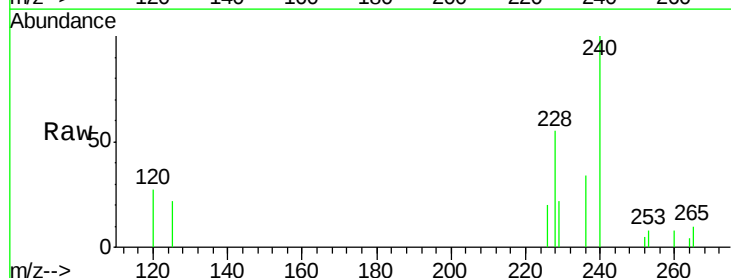

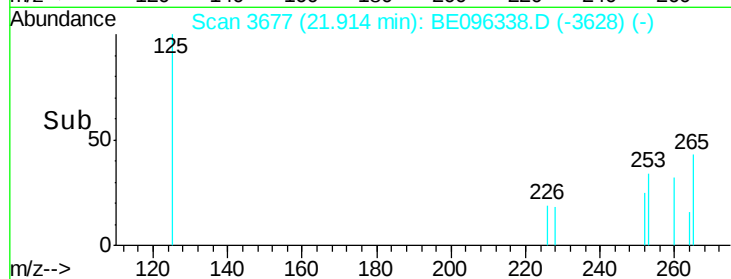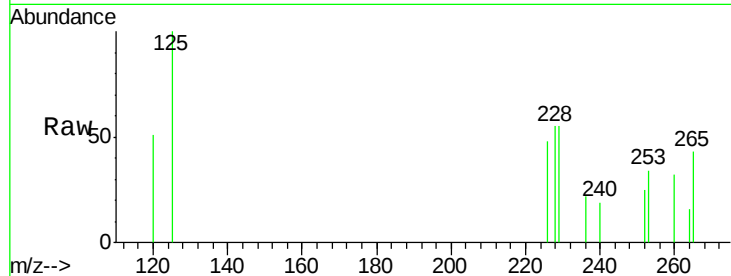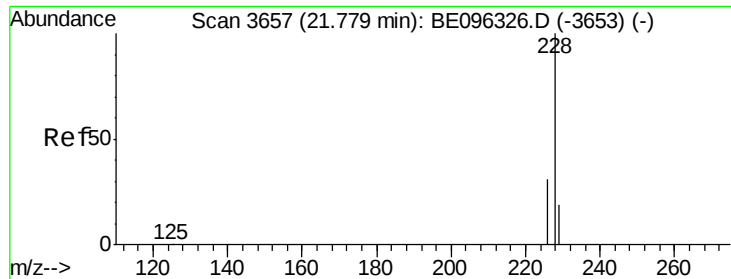

#19

Chrysene

Concen: 2.847 ng/ul

RT: 21.91 min Scan# 3677

Delta R.T. 0.13 min

Lab File: BE096338.D

Acq: 4 May 2018 00:19

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 228 Resp: 204

Ion Ratio Lower Upper

228 100

226 86.4 23.4 35.0#

229 99.2 17.7 26.5#

