




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 01:56:12 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

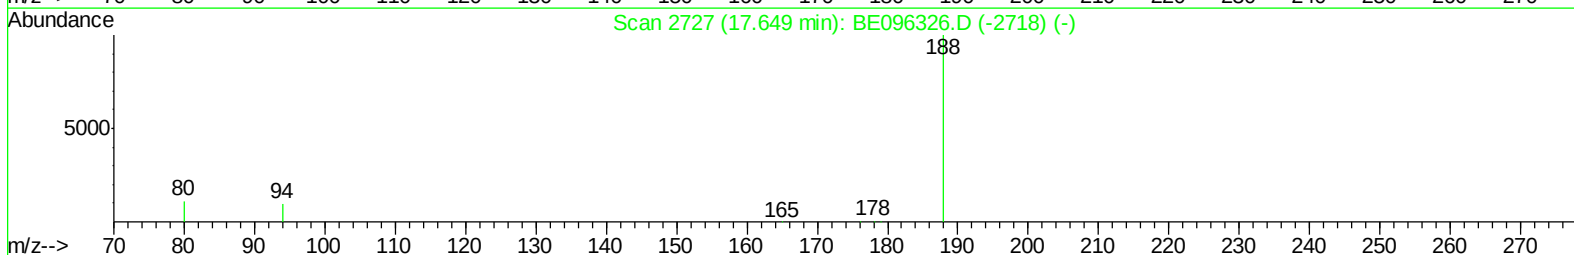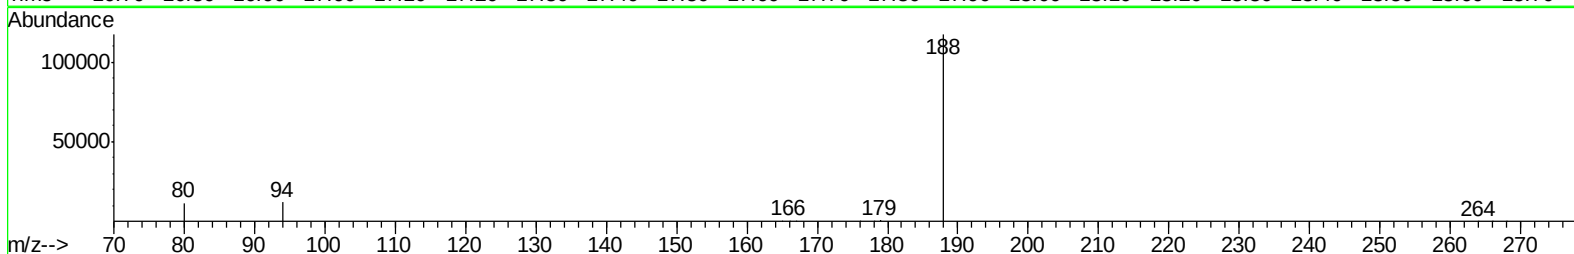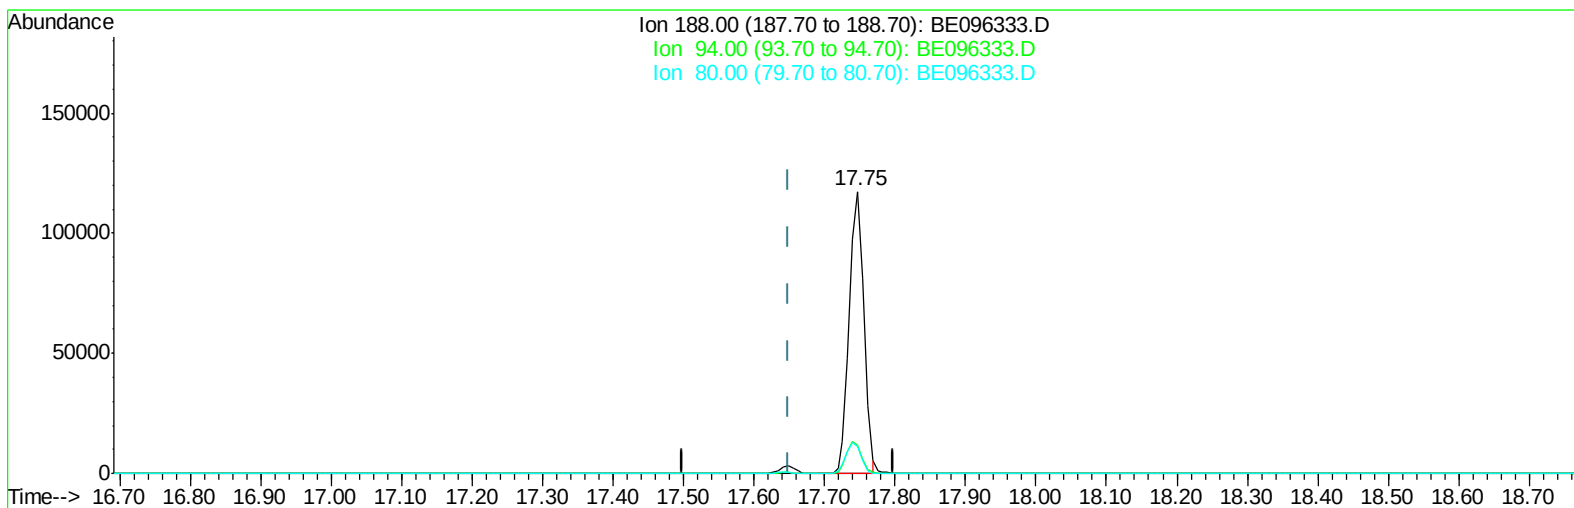

TIC: BE096333.D

(10) Phenanthrene-d10 (I)

17.747min (+0.098) 0.40ng/ul

response 166051

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.18
80.00	11.80	9.69
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 01:56:12 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

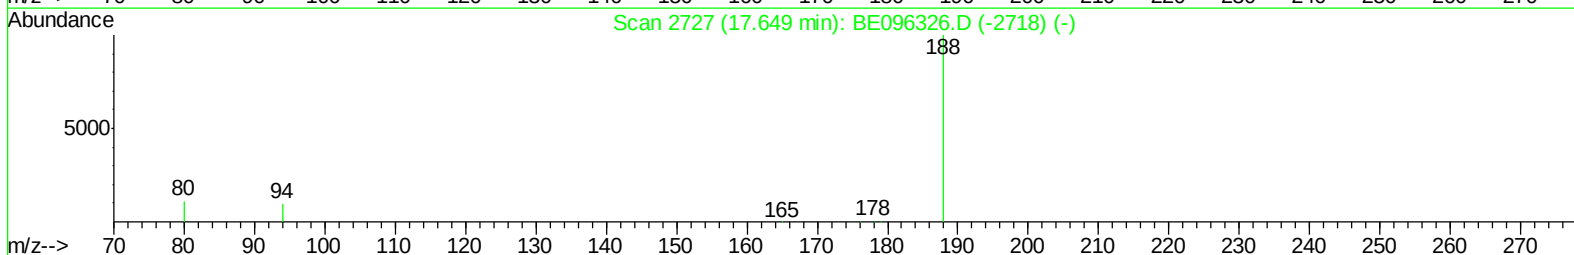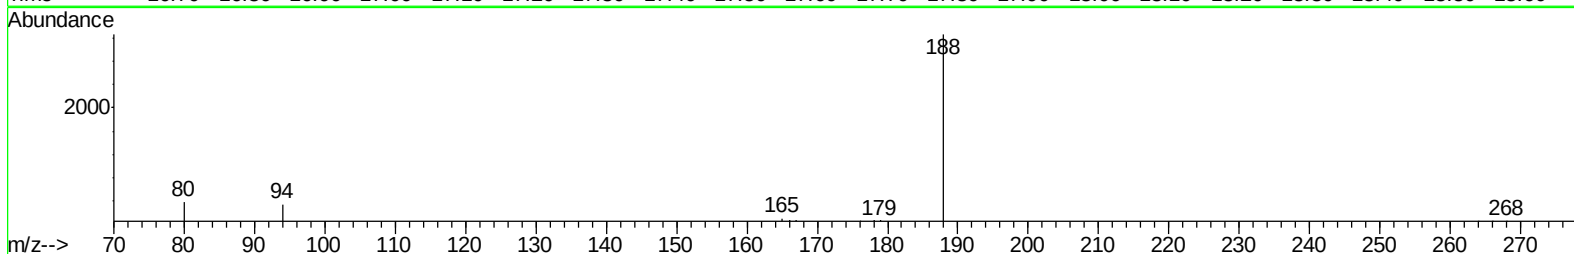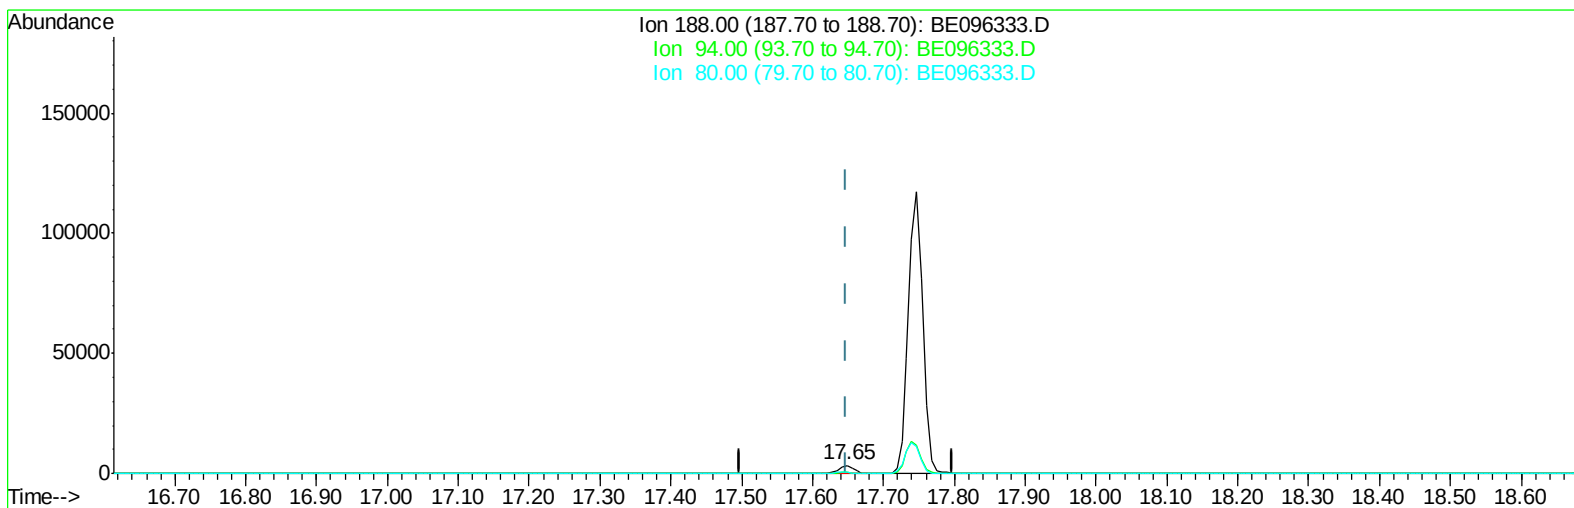

TIC: BE096333.D

(10) Phenanthrene-d10 (I)

17.648min (-0.000) 0.40ng/ul m

response 4667

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.47
80.00	11.80	11.82
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:56:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

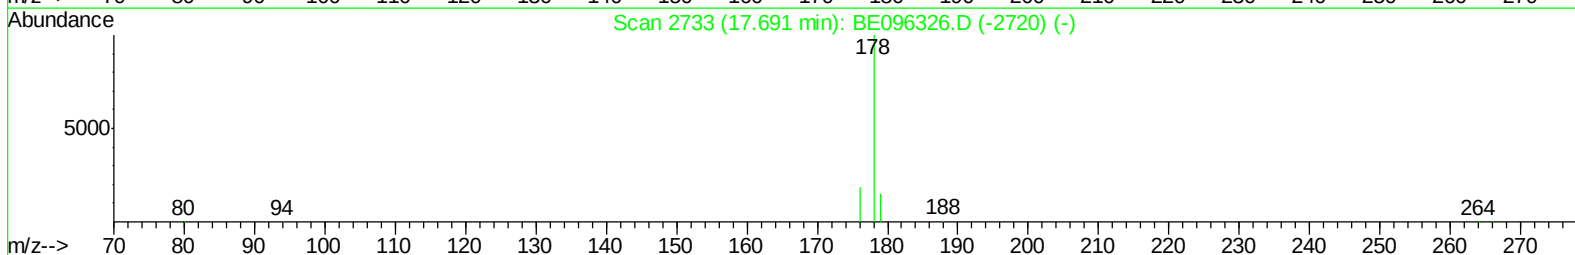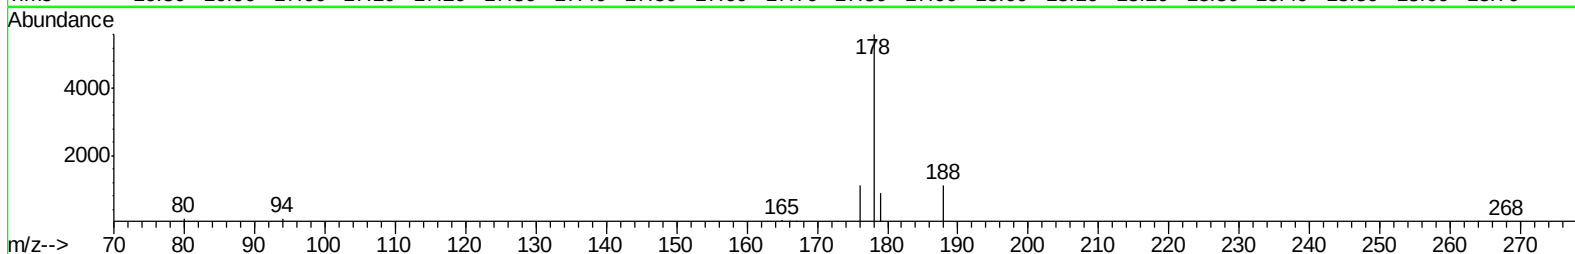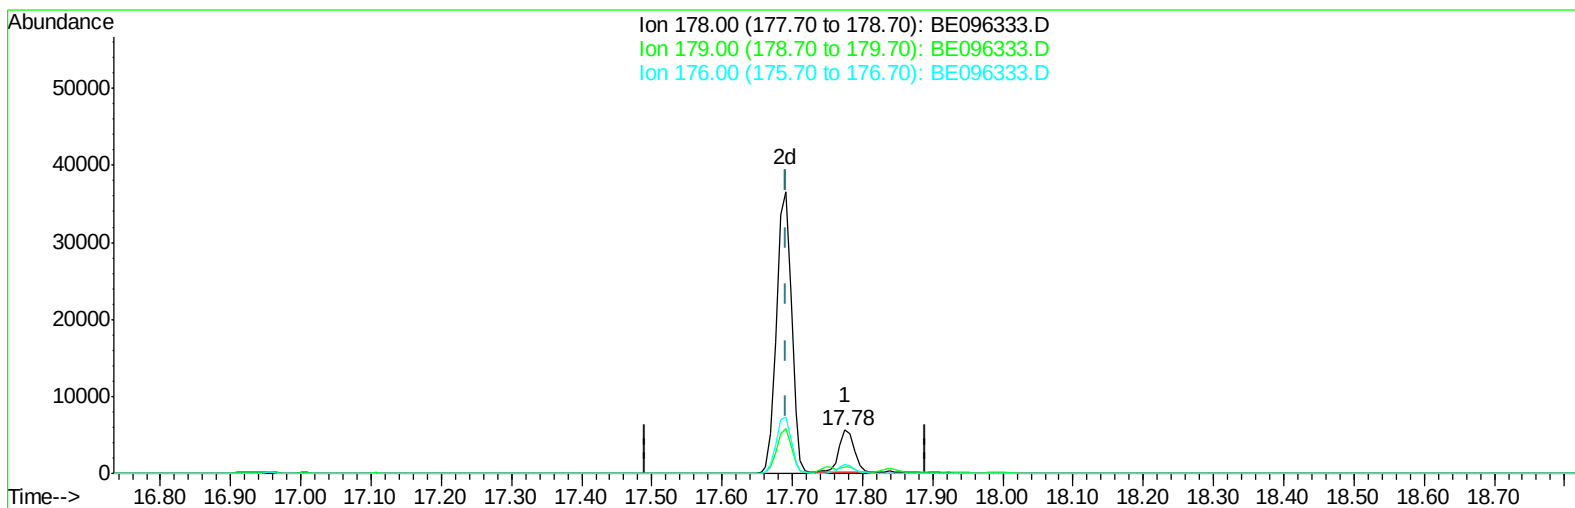

TIC: BE096333.D

(12) Phenanthrene

17.775min (+0.084) 0.59ng/ul

response 8299

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.81#
176.00	17.00	20.07
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:56:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

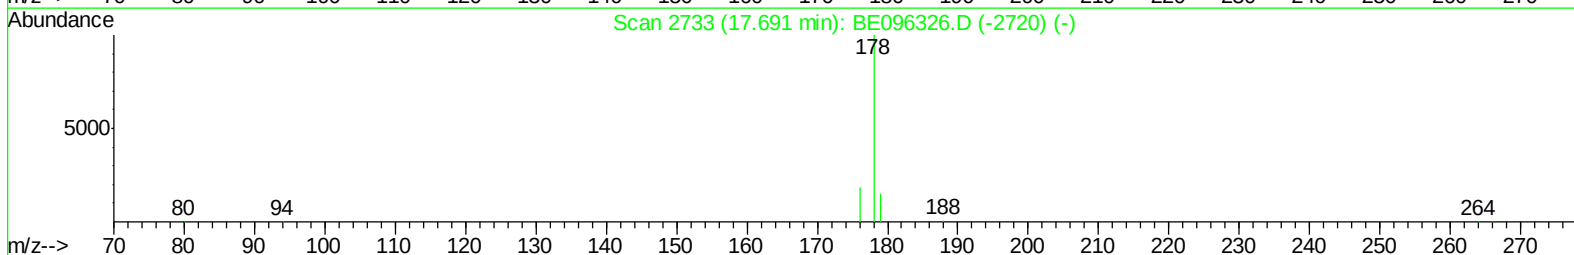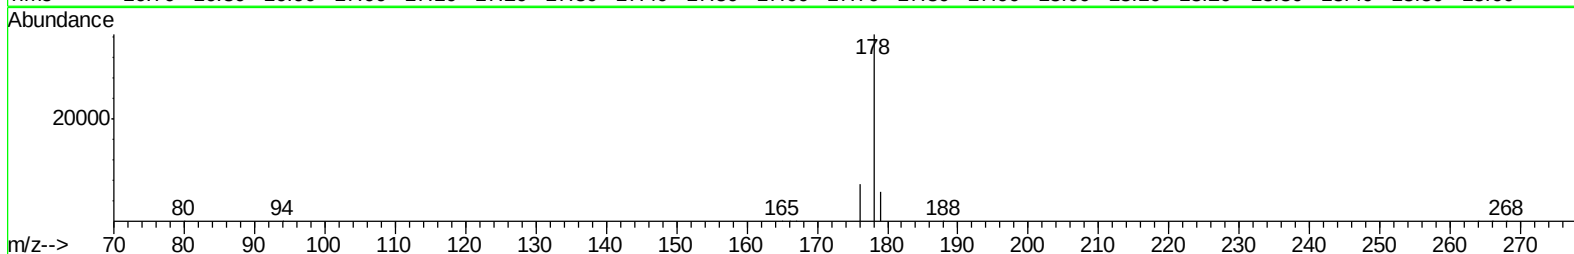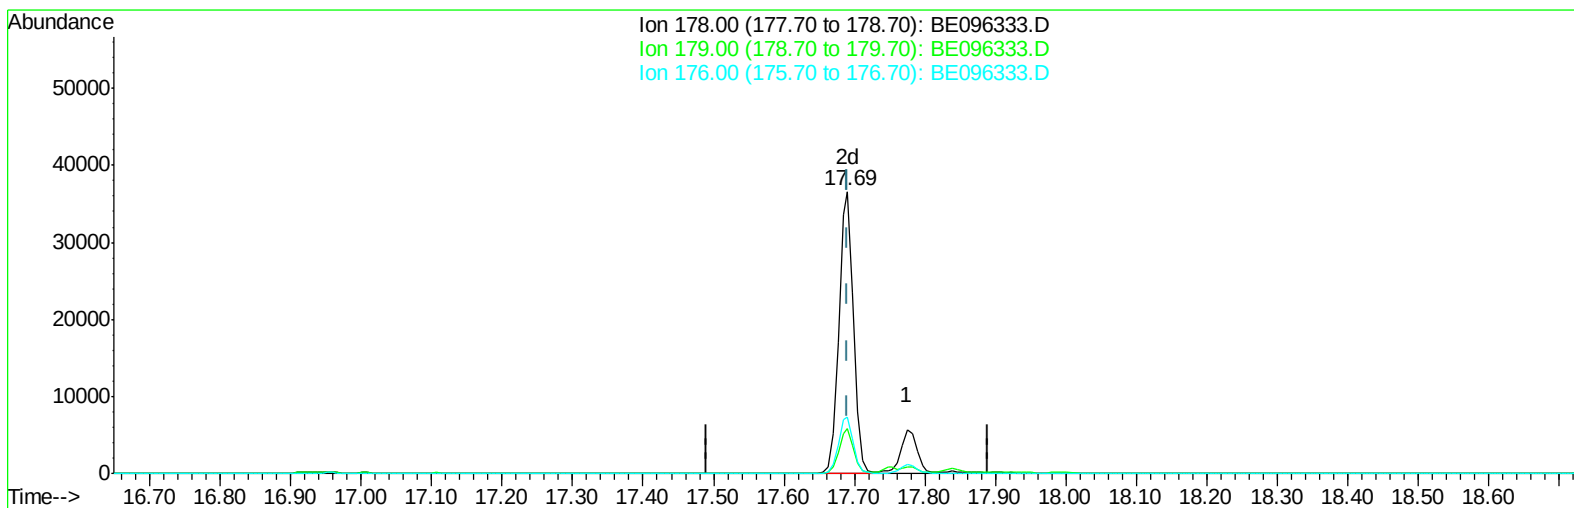

TIC: BE096333.D

(12) Phenanthrene

17.691min (-0.000) 3.81ng/ul m

response 53537

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.75#
176.00	17.00	19.82
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:56:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

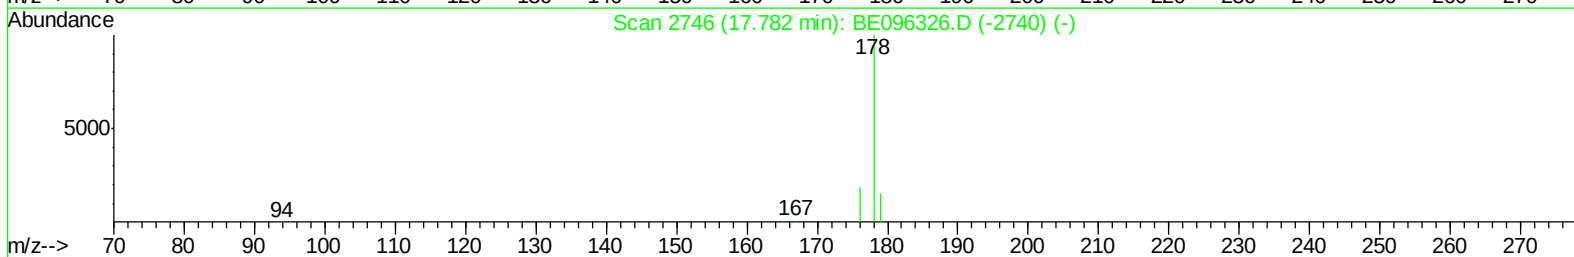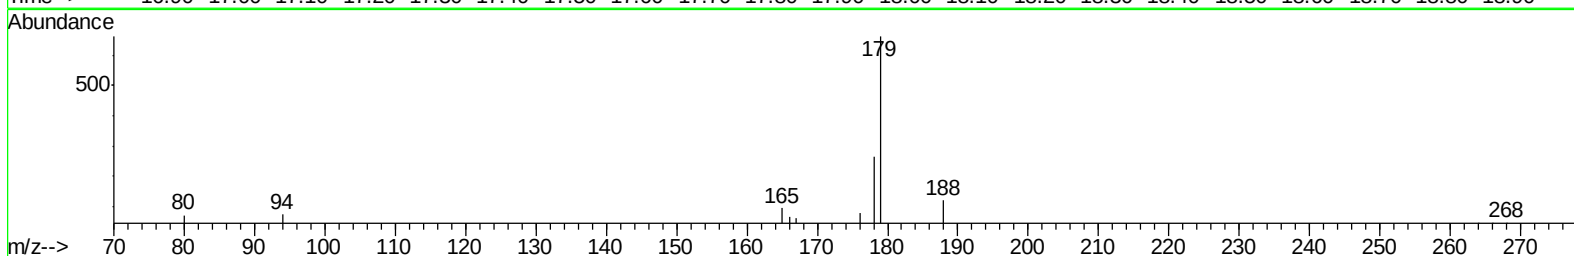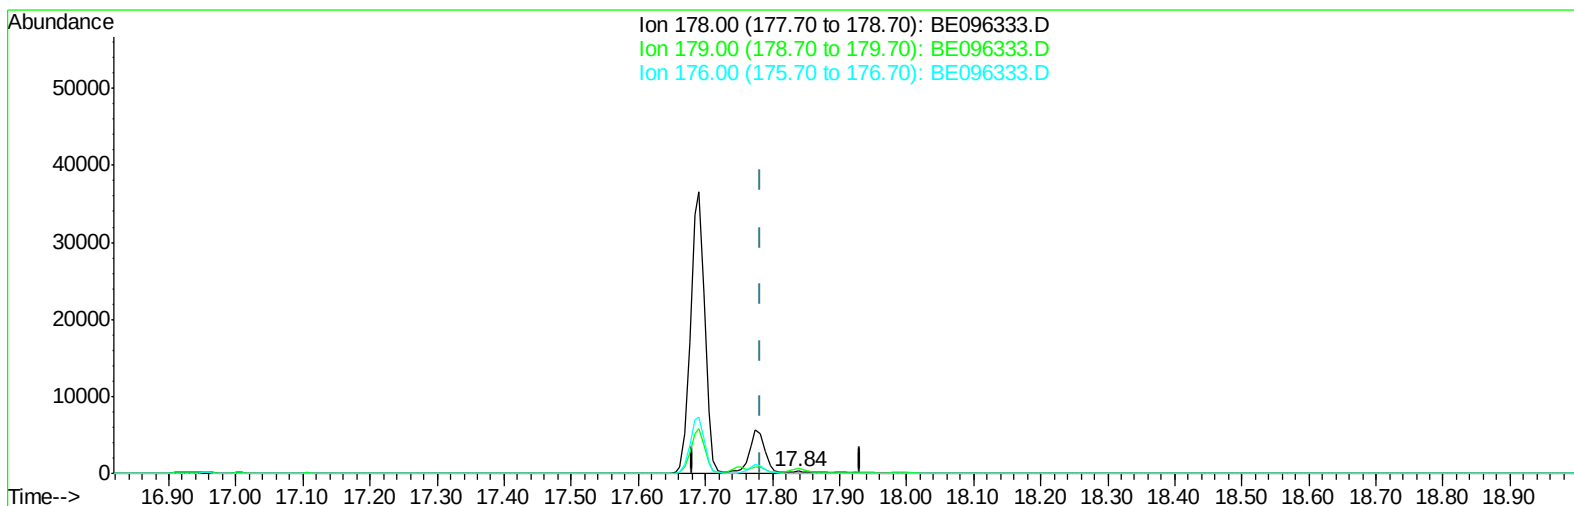

TIC: BE096333.D

(13) Anthracene

17.838min (+0.056) 0.02ng/ul

response 295

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	249.81#
176.00	18.40	29.06#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:56:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

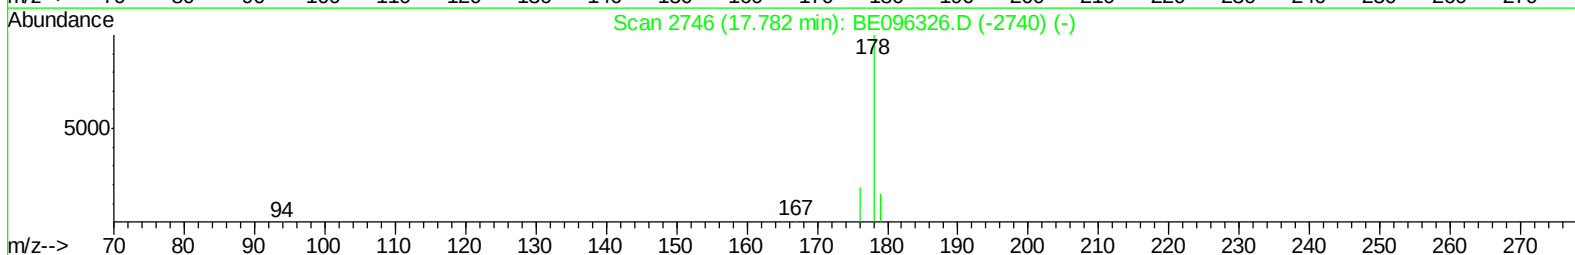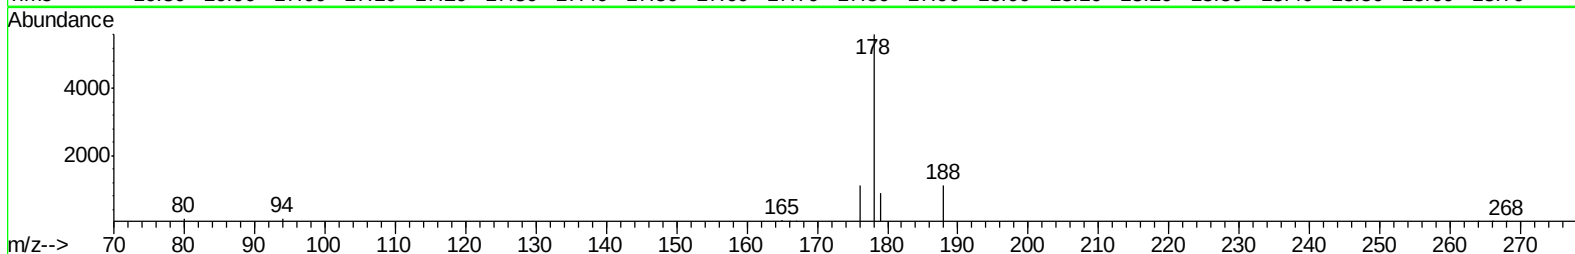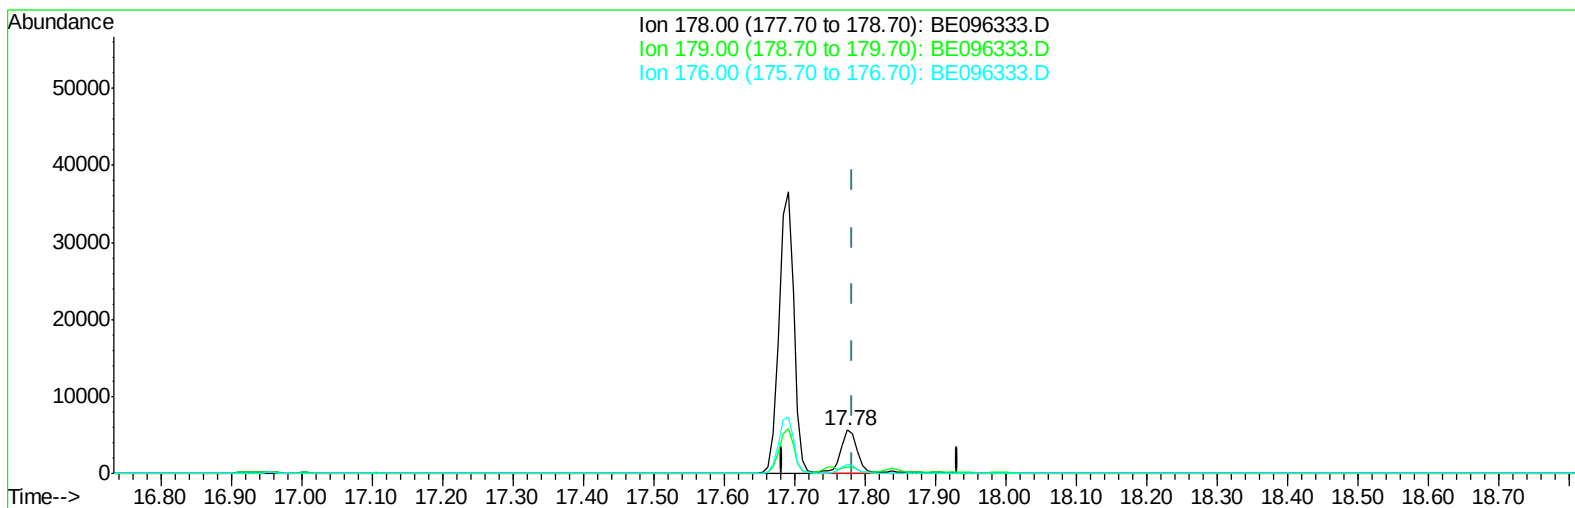

TIC: BE096333.D

(13) Anthracene

17.775min (-0.007) 0.63ng/ul m

response 8513

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	15.81#
176.00	18.40	20.07
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:56:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

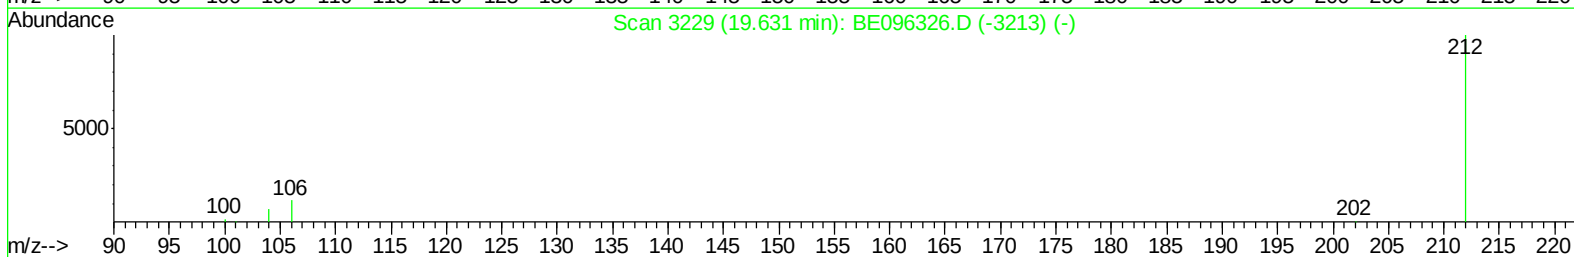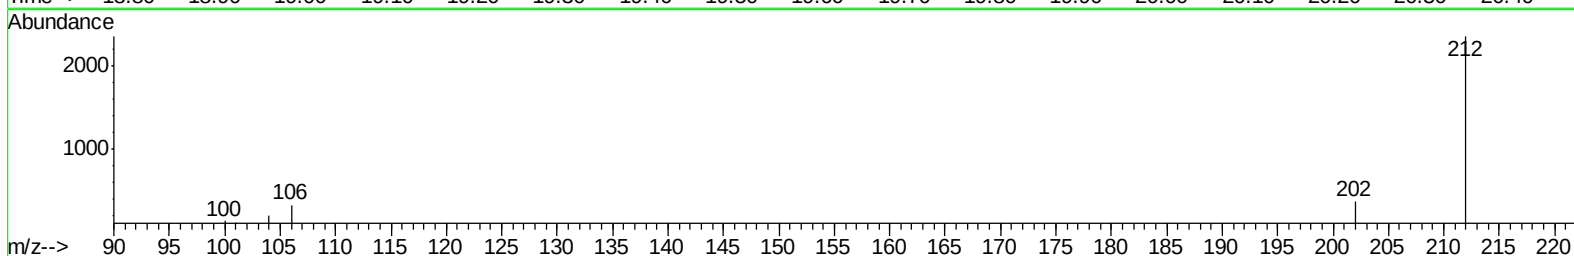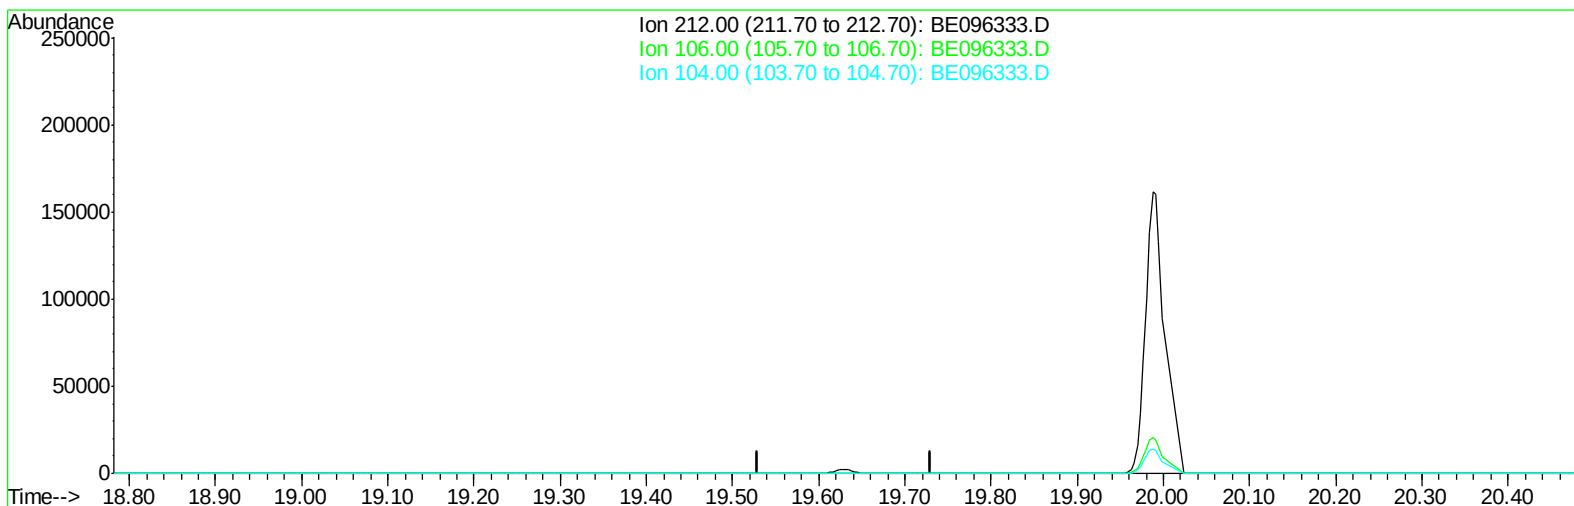

TIC: BE096333.D

(14) Fluoranthene-d10 (SURR)

19.631min (-19.631) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:56:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

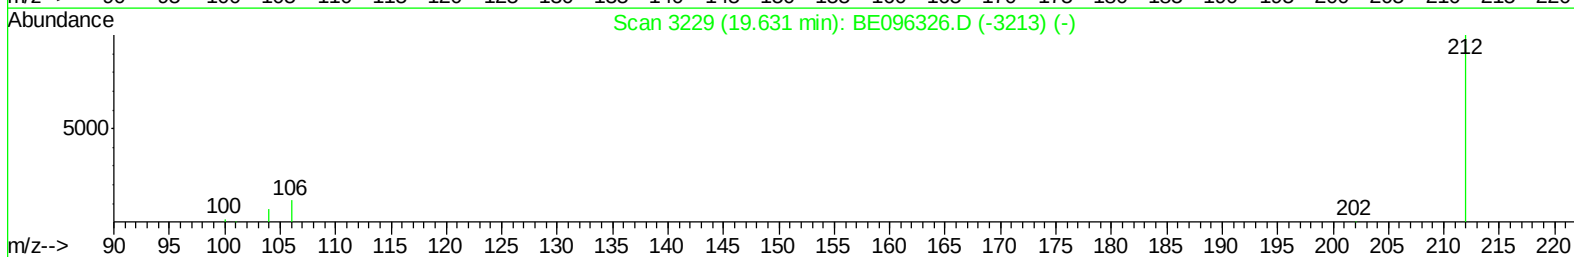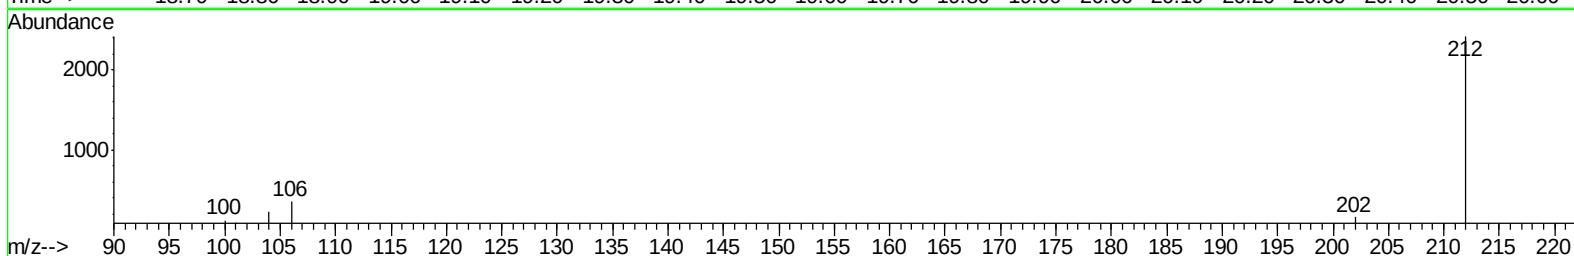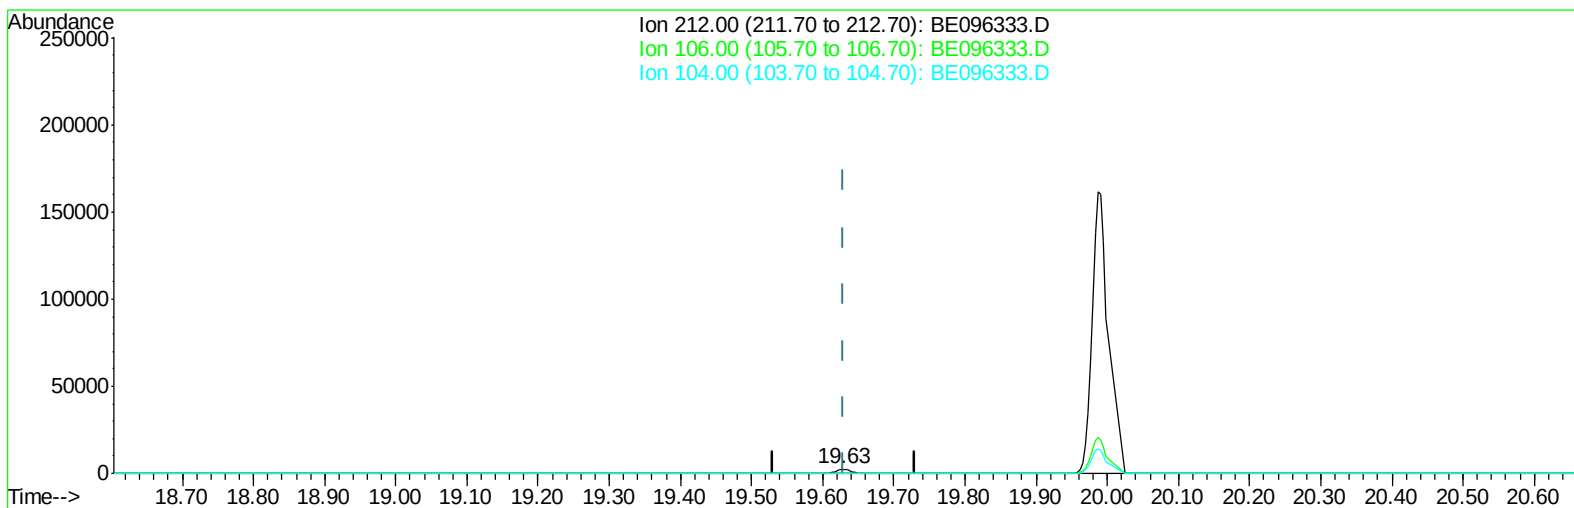

TIC: BE096333.D

(14) Fluoranthene-d10 (SURR)

19.627min (-0.003) 0.16ng/ul m

response 3229

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:56:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

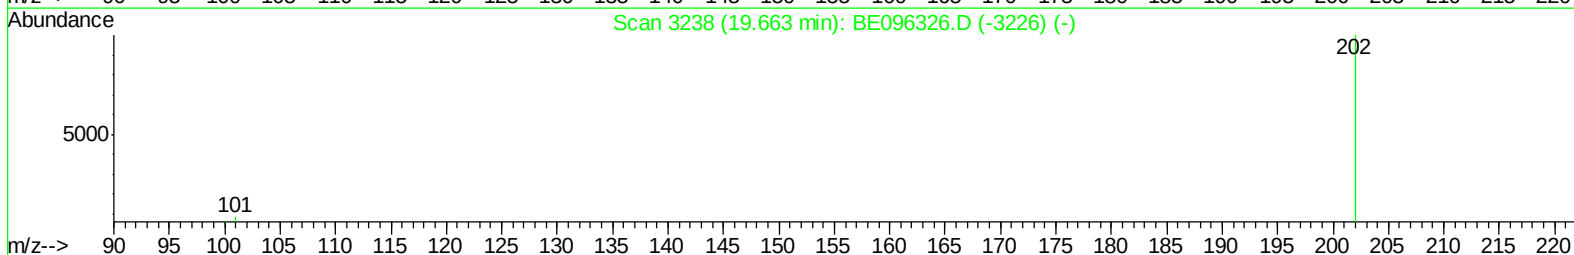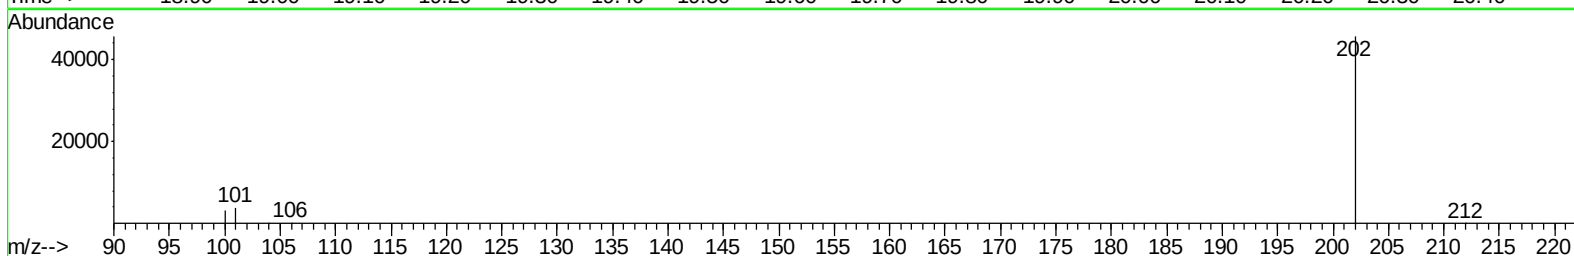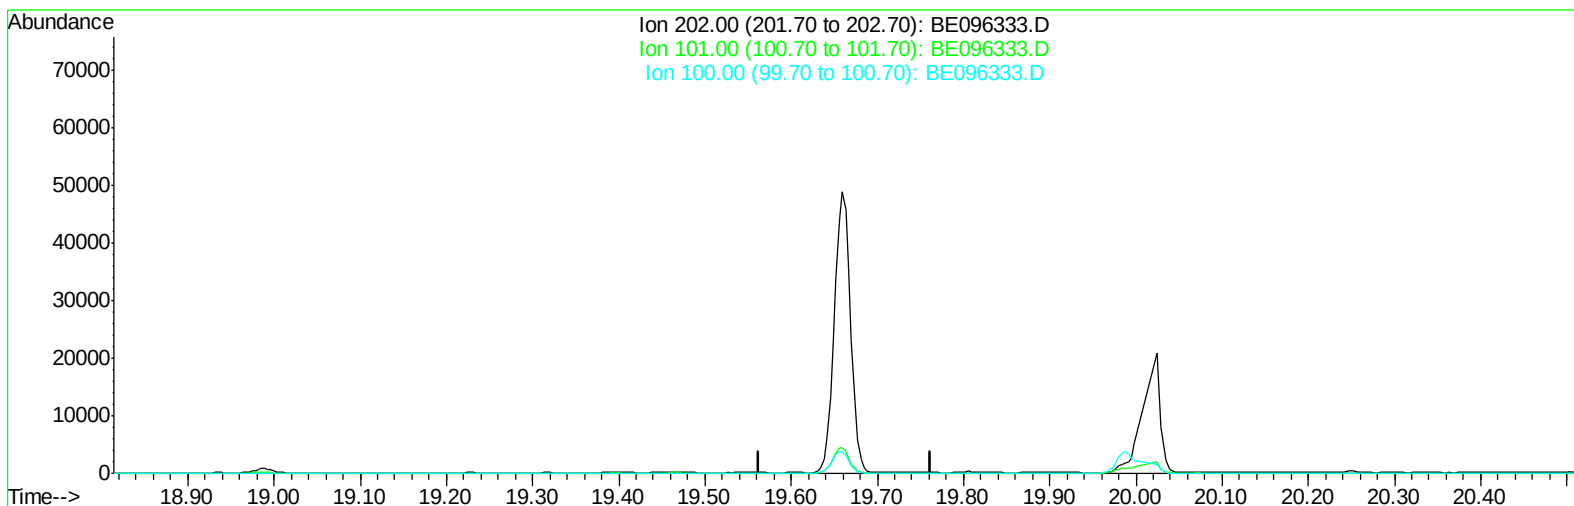

TIC: BE096333.D

(15) Fluoranthene (C)

19.663min (-19.663) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.30	0.00
100.00	19.50	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:56:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

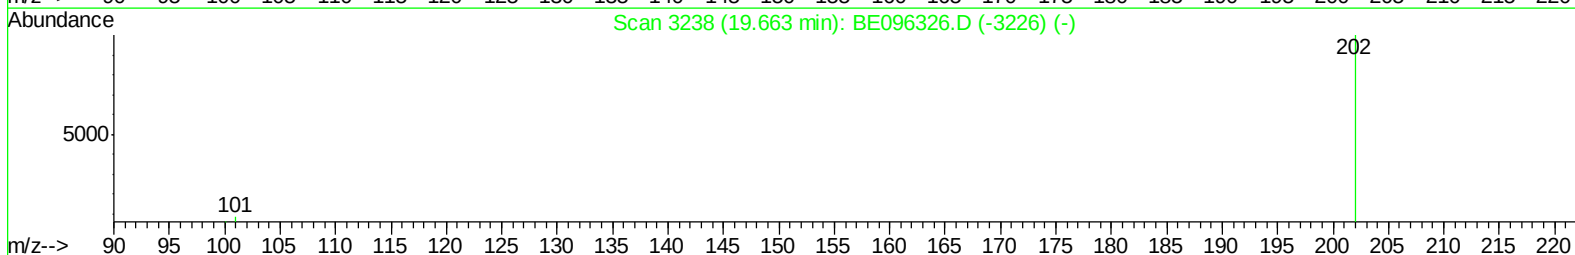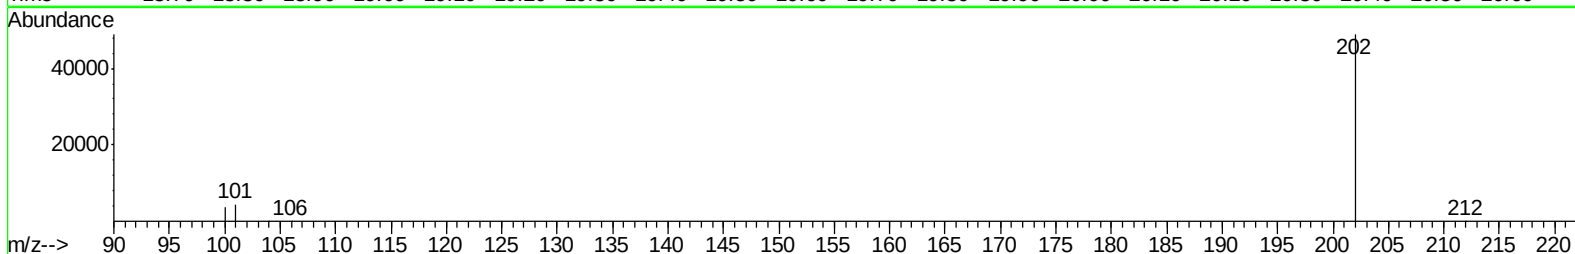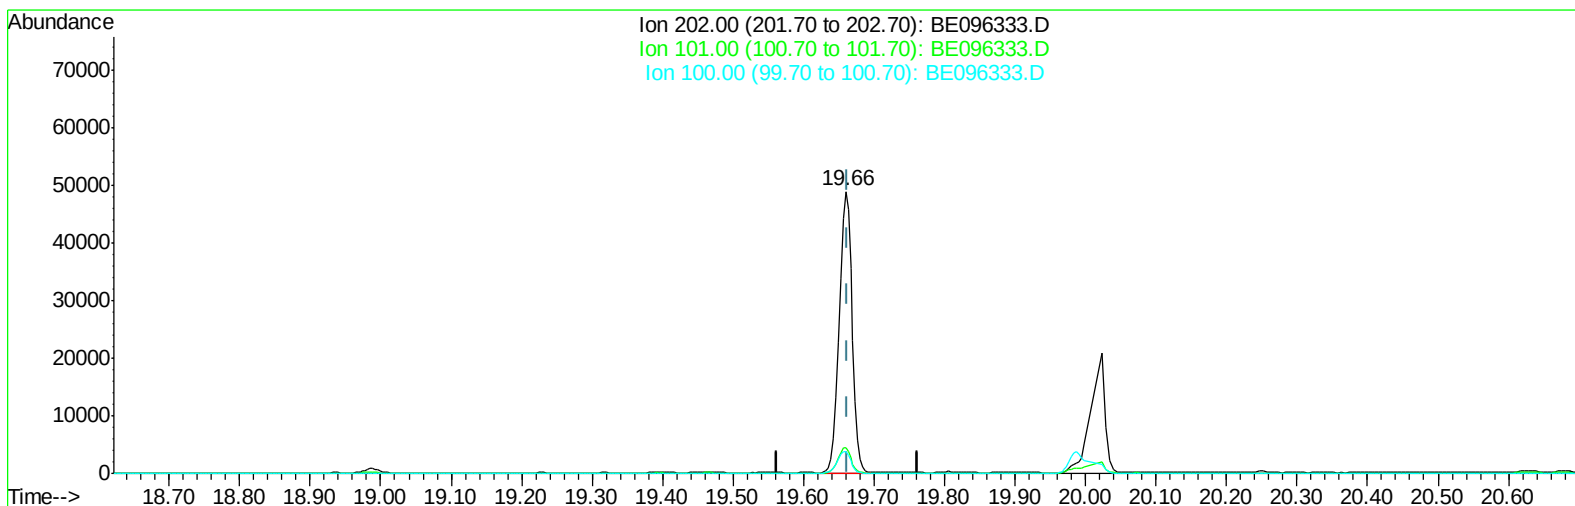

TIC: BE096333.D

(15) Fluoranthene (C)

19.659min (-0.003) 3.21ng/ul m

response 64166

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	9.06
100.00	19.50	7.70
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:56:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

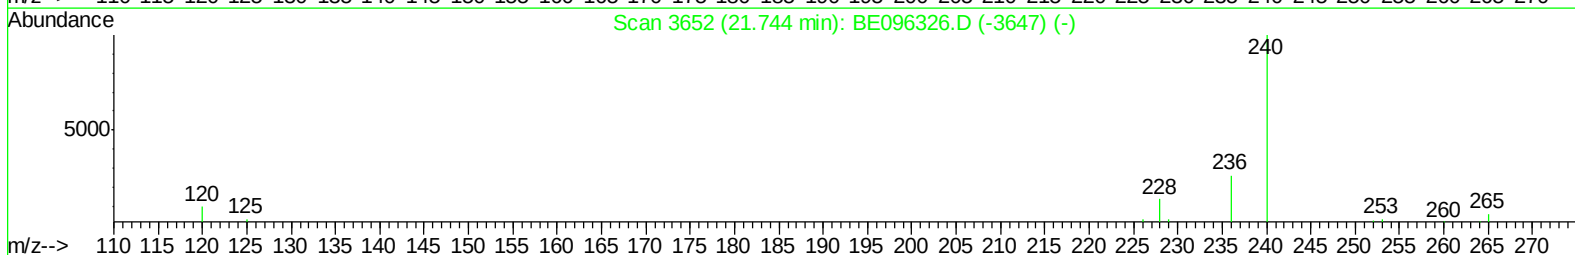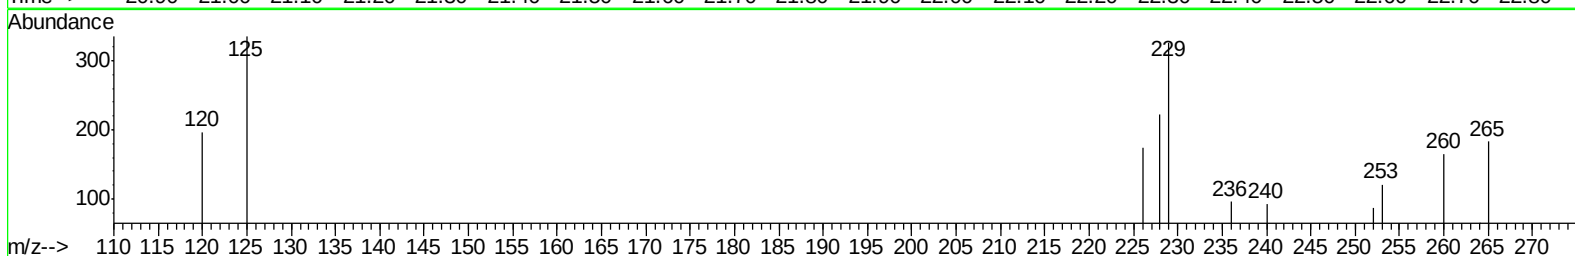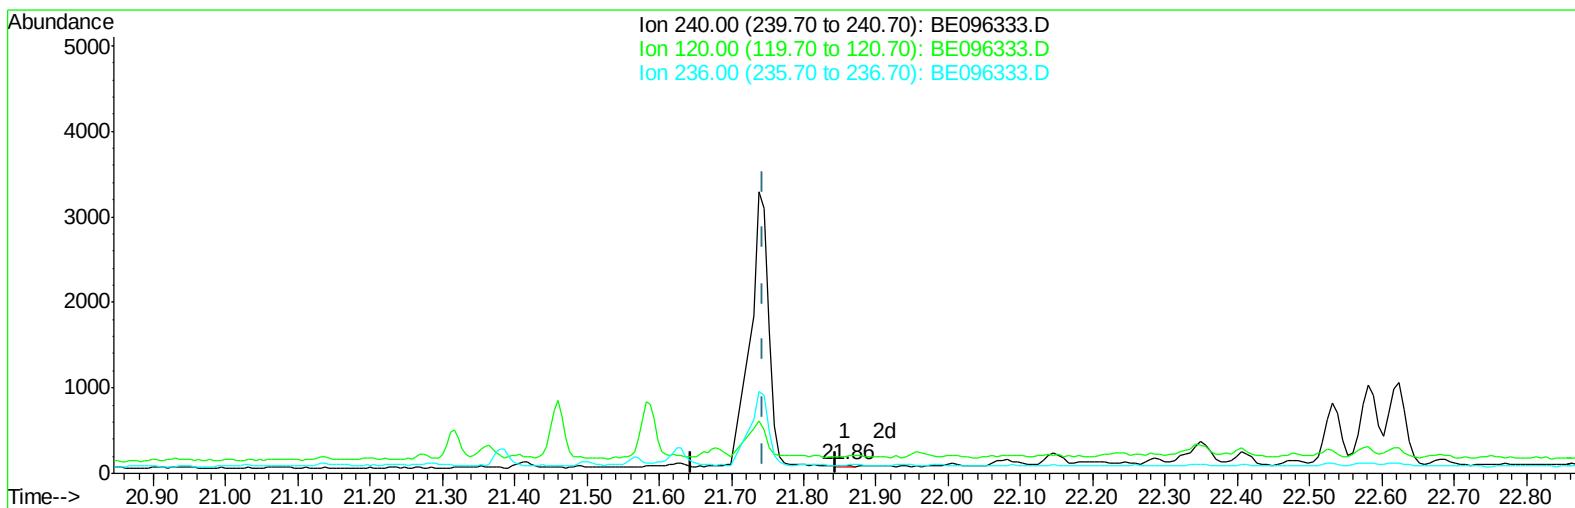

TIC: BE096333.D

(16) Chrysene-d12 (I)

21.857min (+0.113) 0.40ng/ul

response 11

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	211.83#
236.00	34.90	103.23#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:56:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

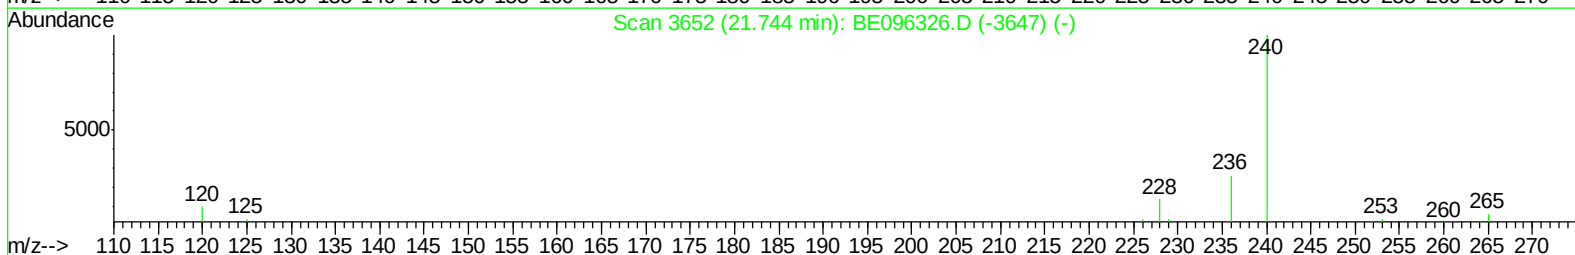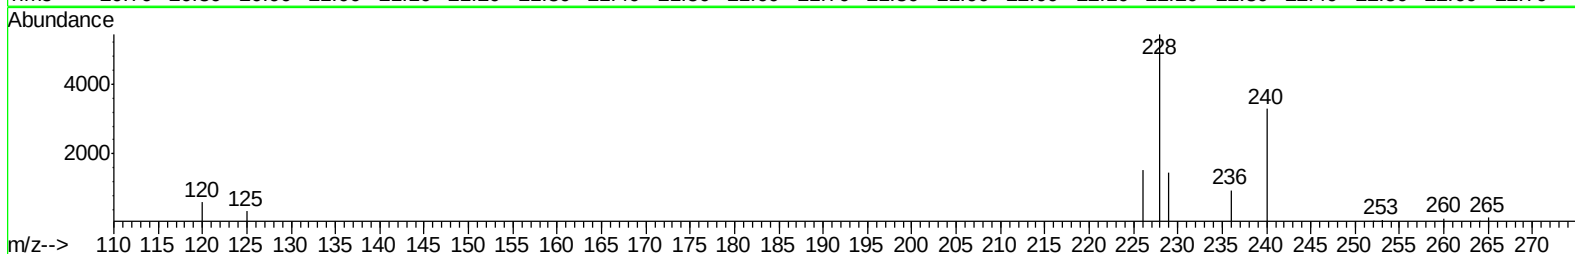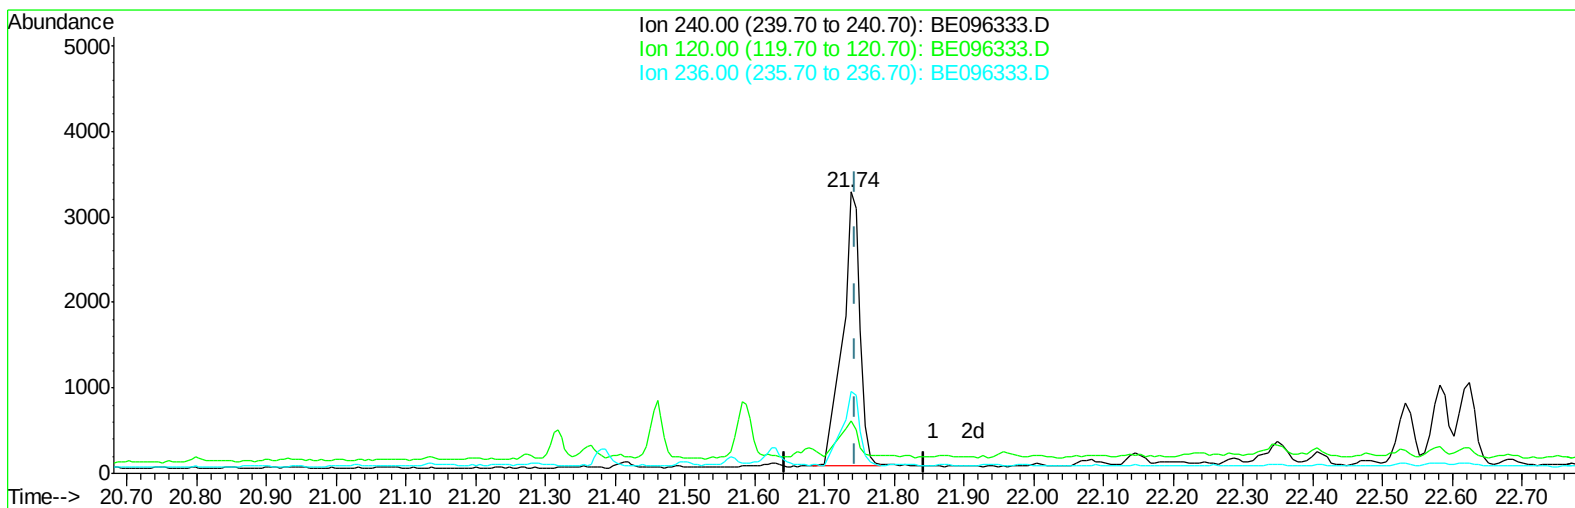

TIC: BE096333.D

(16) Chrysene-d12 (I)

21.738min (-0.007) 0.40ng/ul m

response 5418

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	18.68
236.00	34.90	29.22
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:59:08 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

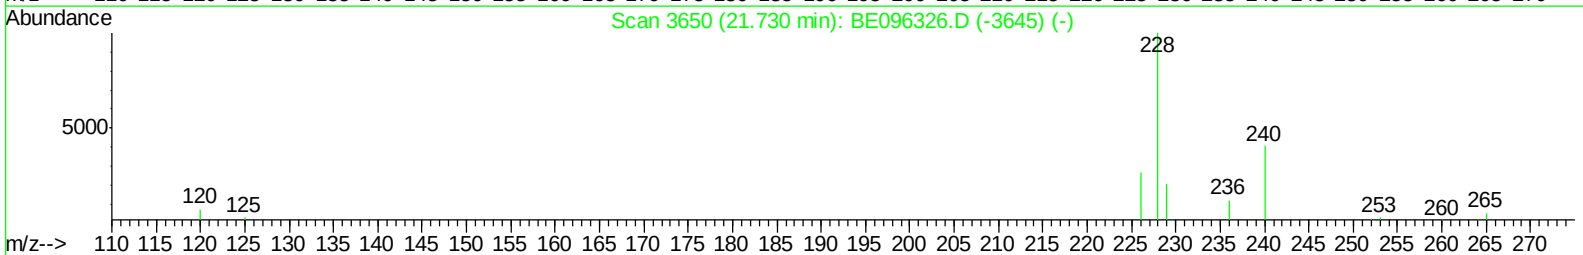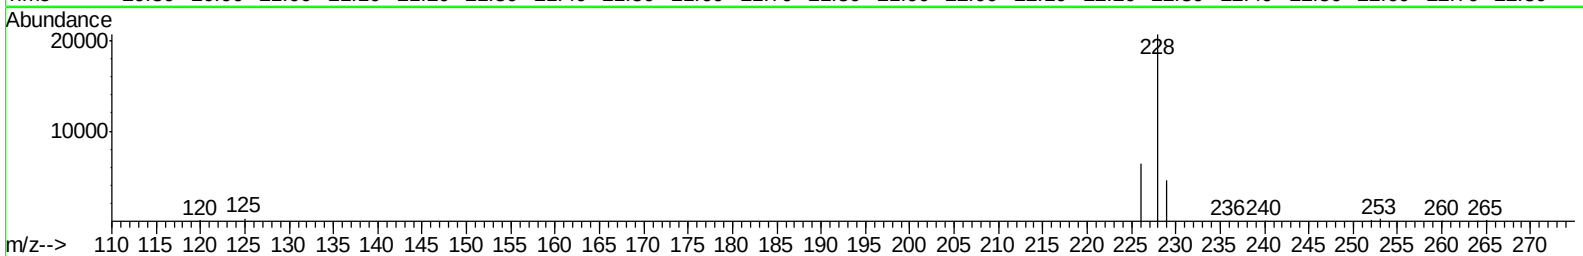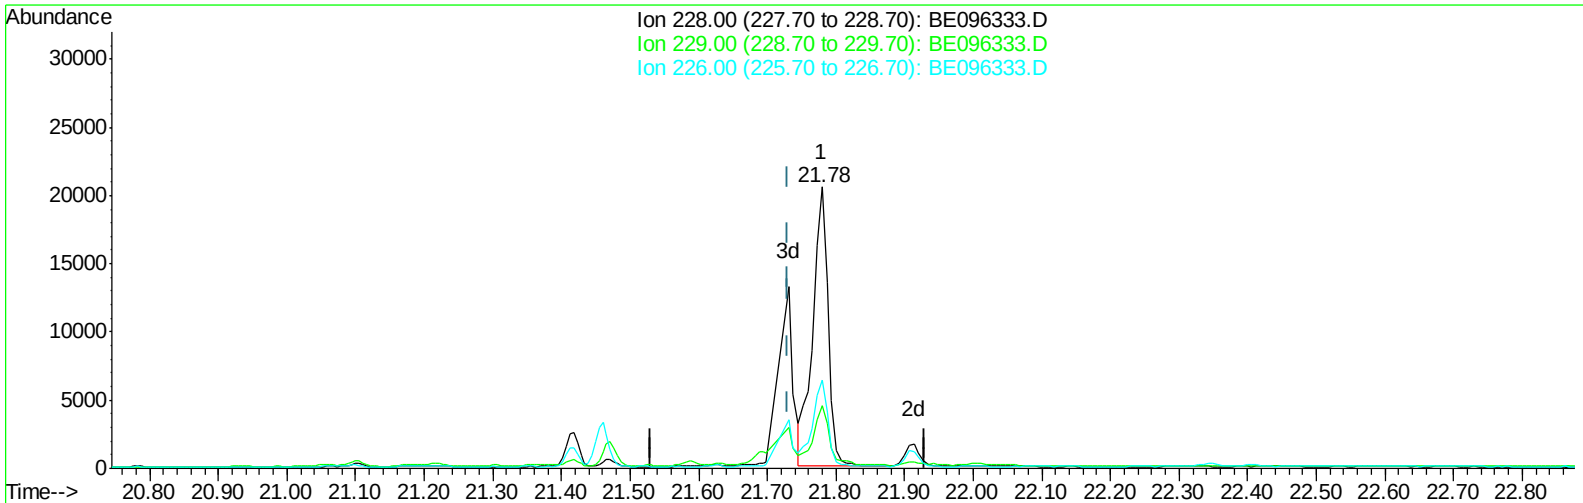

TIC: BE096333.D

(18) Benzo(a)anthracene
21.780min (+0.050) 3.77ng/ul
response 31914

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	22.25#
226.00	21.30	31.23#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:59:08 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

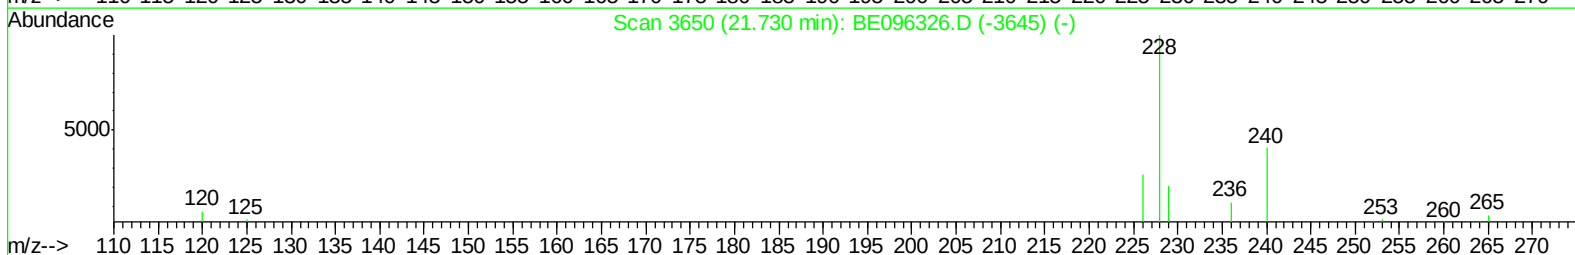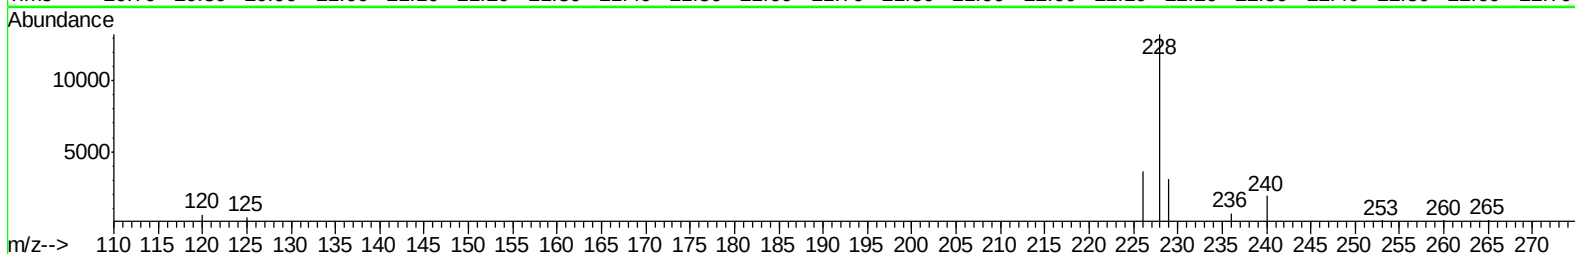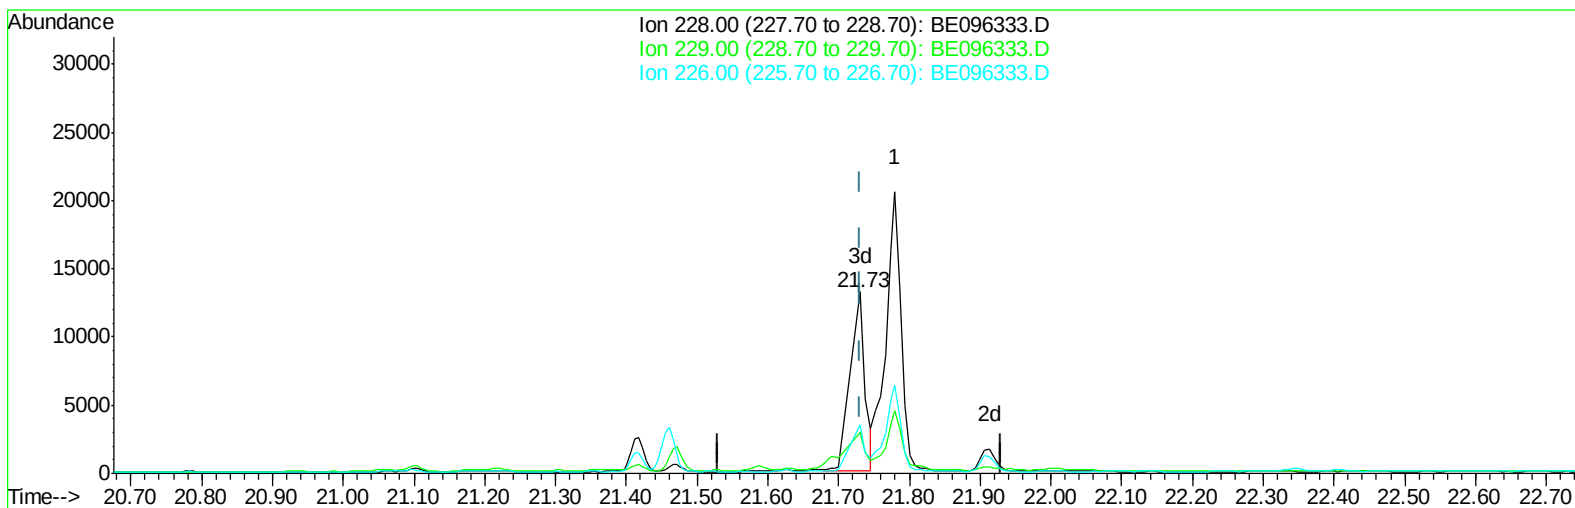

TIC: BE096333.D

(18) Benzo(a)anthracene

21.731min (+0.000) 1.49ng/ul m

response 12629

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	22.76#
226.00	21.30	26.89#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:59:08 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

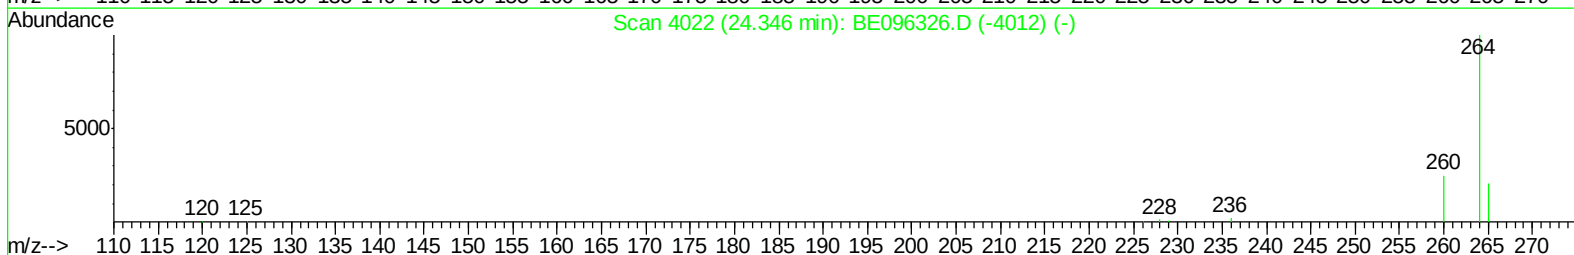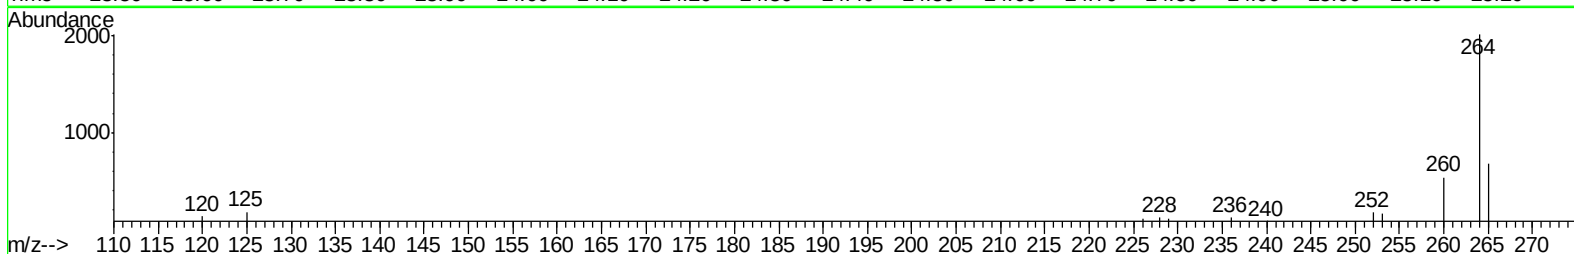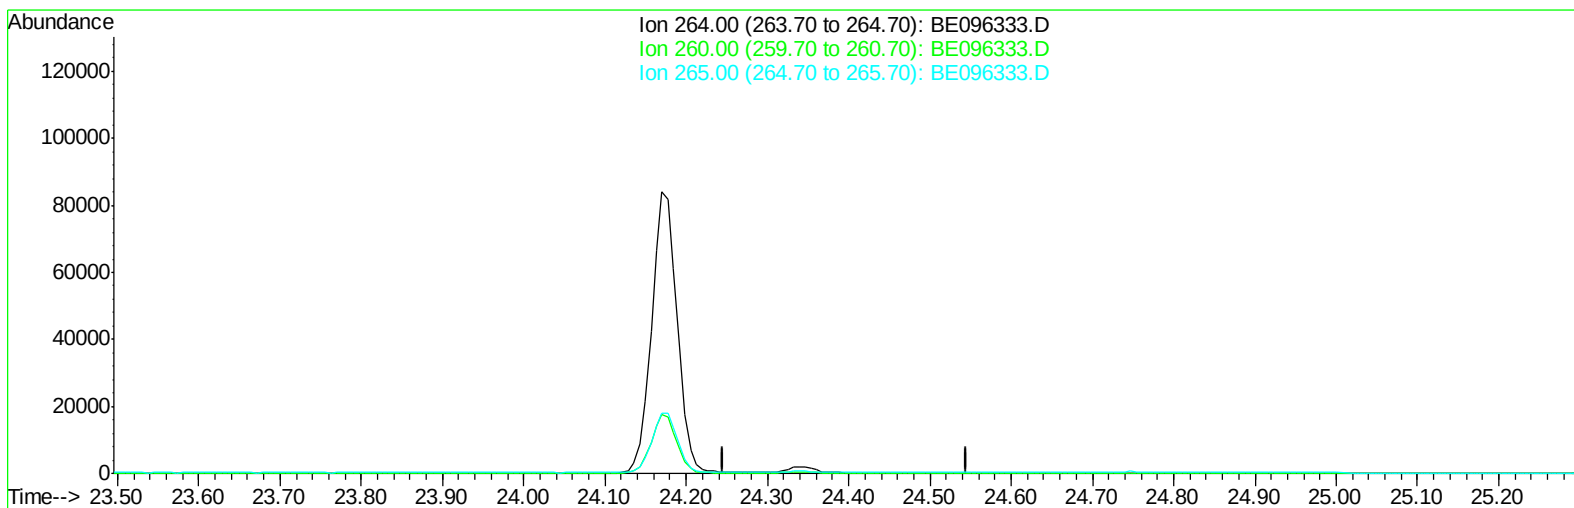

TIC: BE096333.D

(20) Perylene-d12 (I)

24.346min (-24.346) 0.00ng/ul

response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	30.10	0.00#
265.00	103.50	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 02:59:08 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

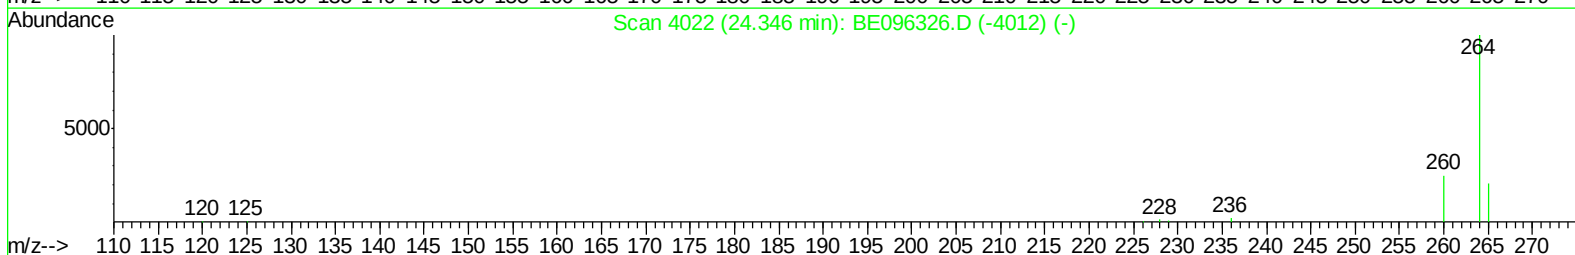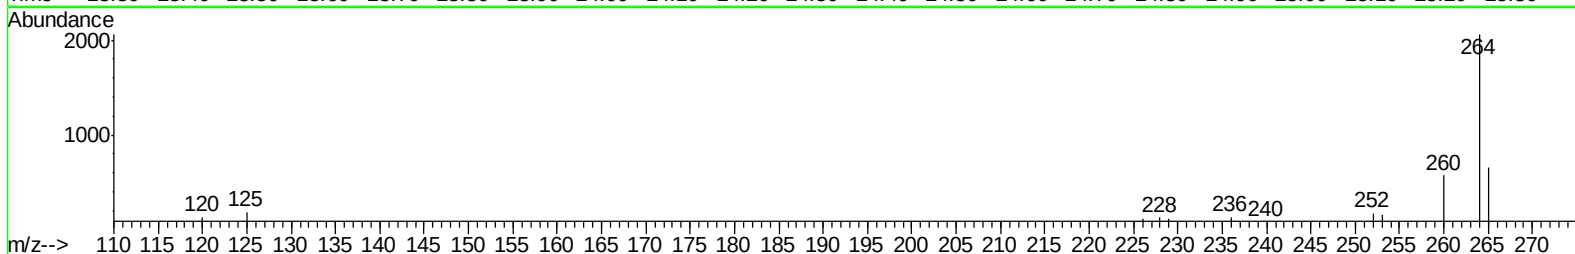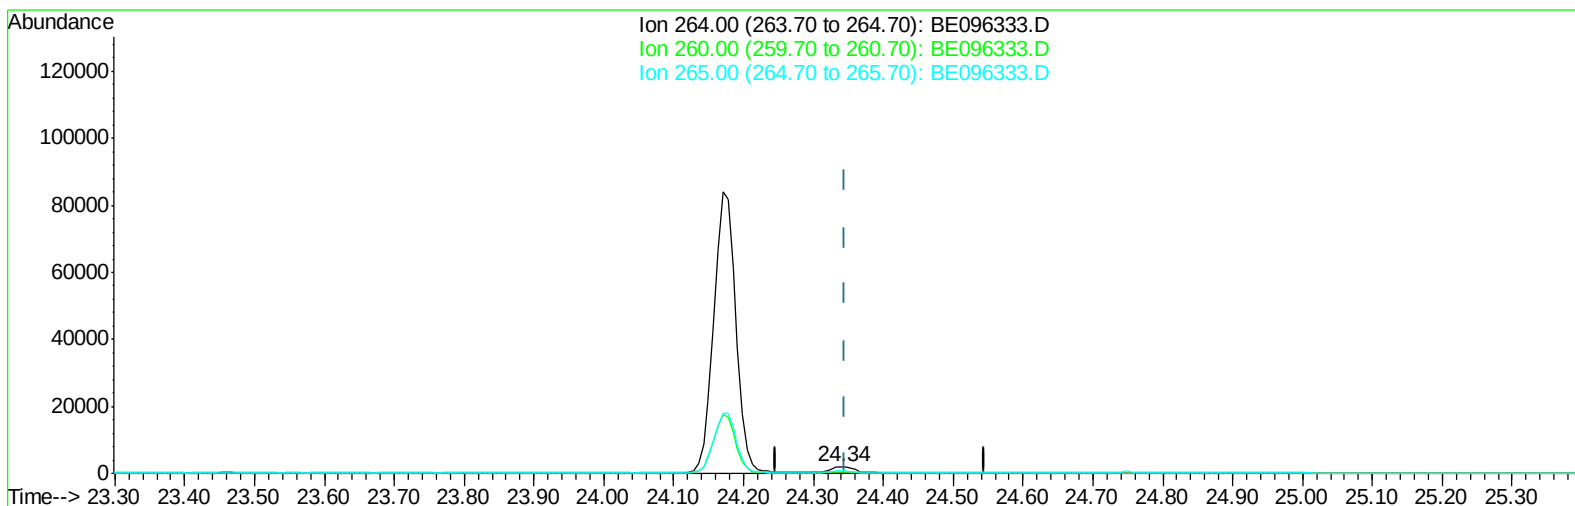

TIC: BE096333.D

(20) Perylene-d12 (I)

24.339min (-0.007) 0.40ng/ul m

response 4156

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	27.61
265.00	103.50	31.88#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 03:00:00 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

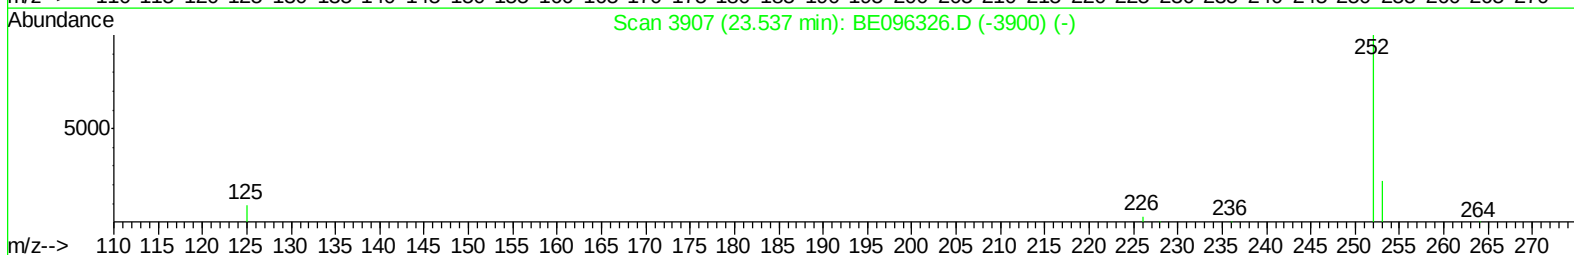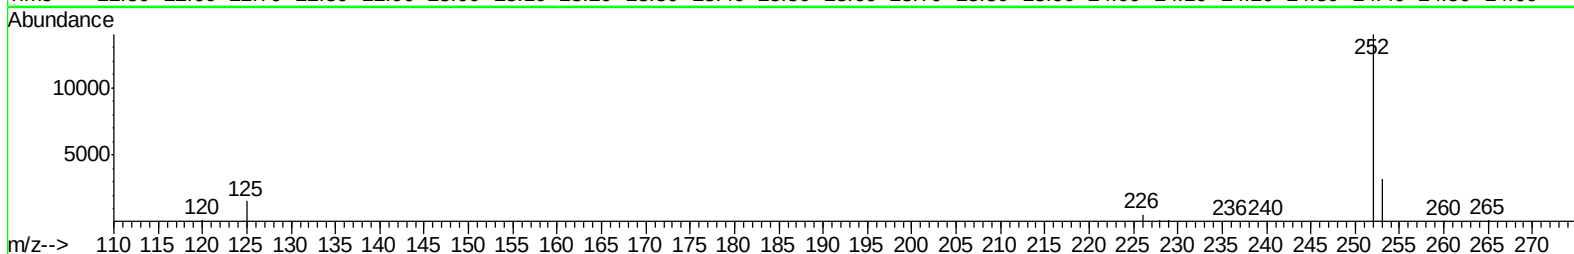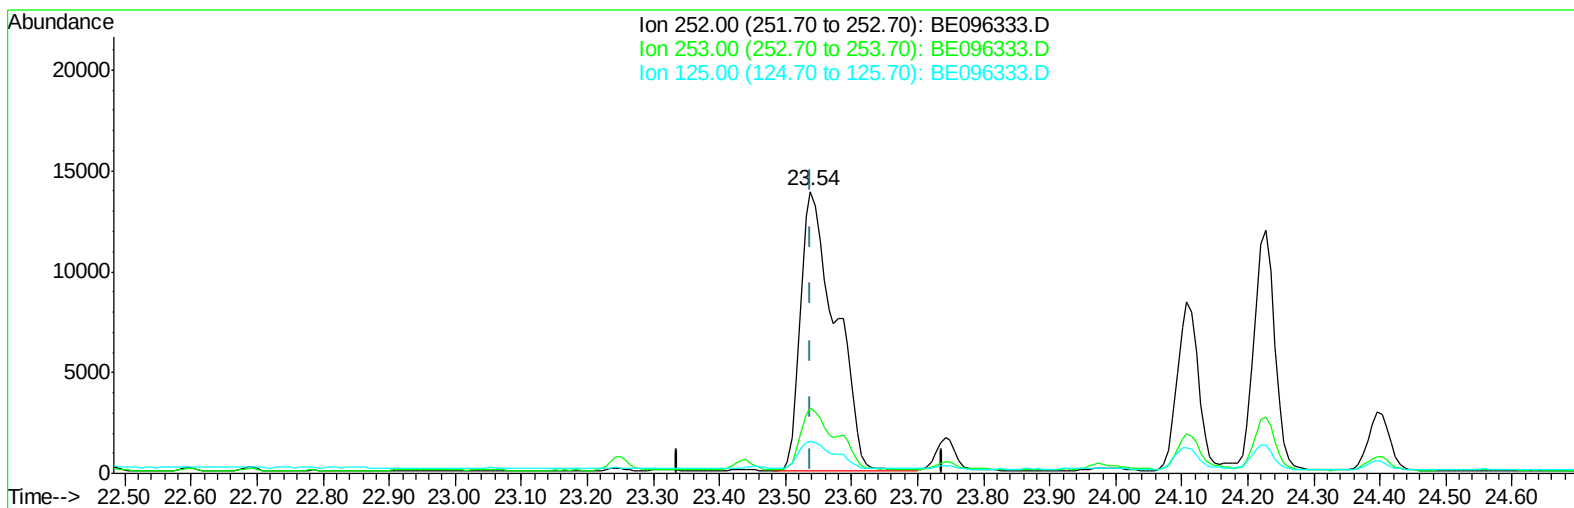

TIC: BE096333.D

(21) Benzo(b)fluoranthene

23.538min (+0.000) 3.57ng/ul

response 50723

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.01
125.00	17.50	11.26
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 03:00:00 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

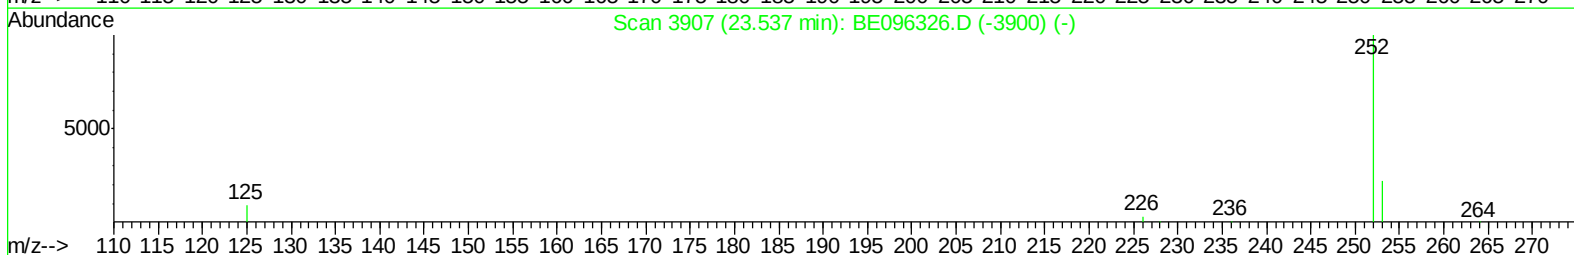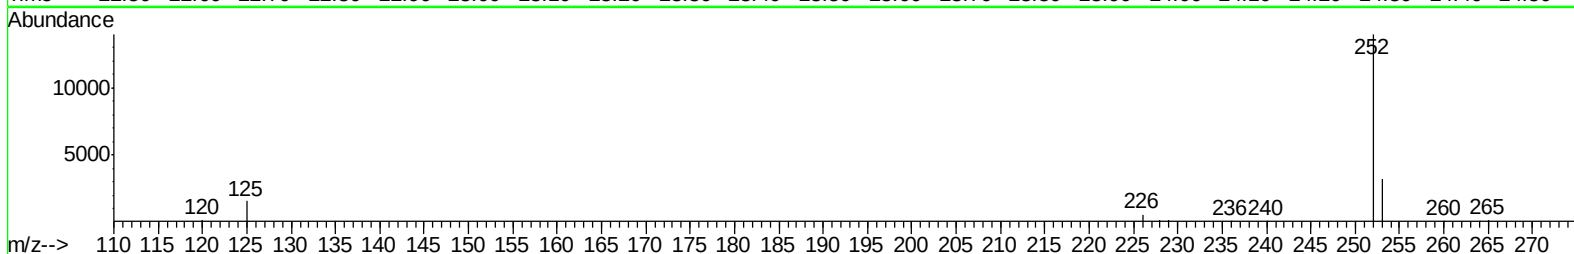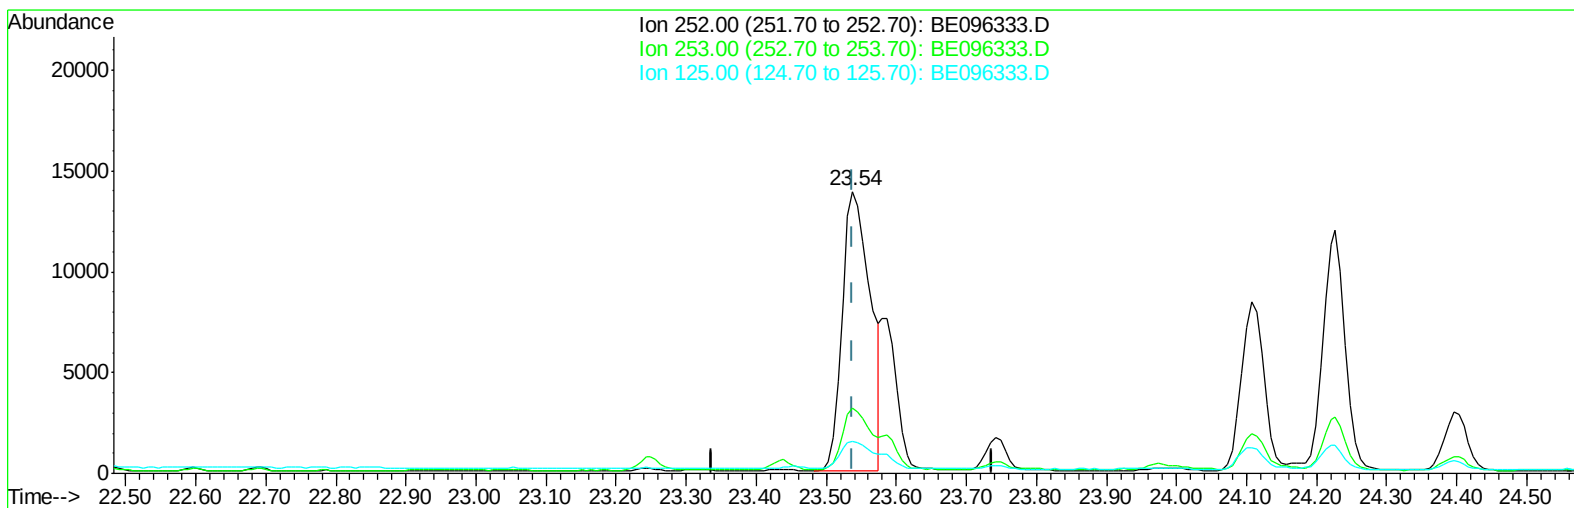

TIC: BE096333.D

(21) Benzo(b)fluoranthene

23.538min (+0.000) 2.71ng/ul m

response 38482

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.01
125.00	17.50	11.26
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 03:00:00 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

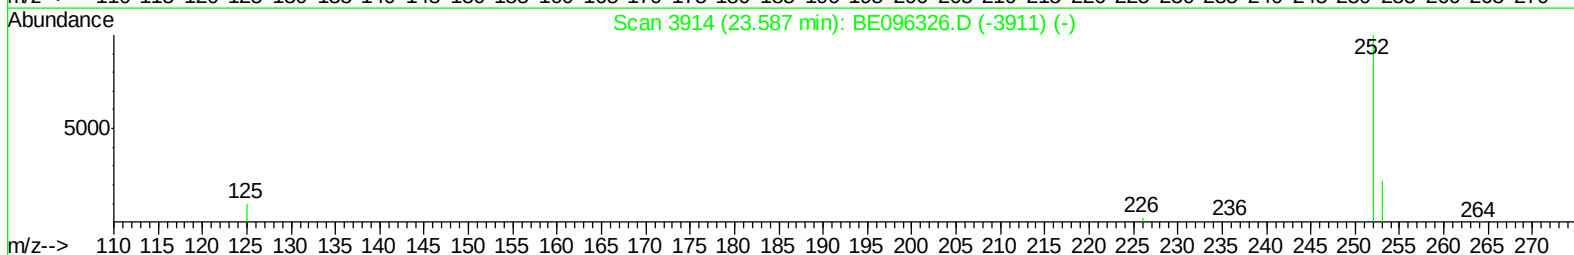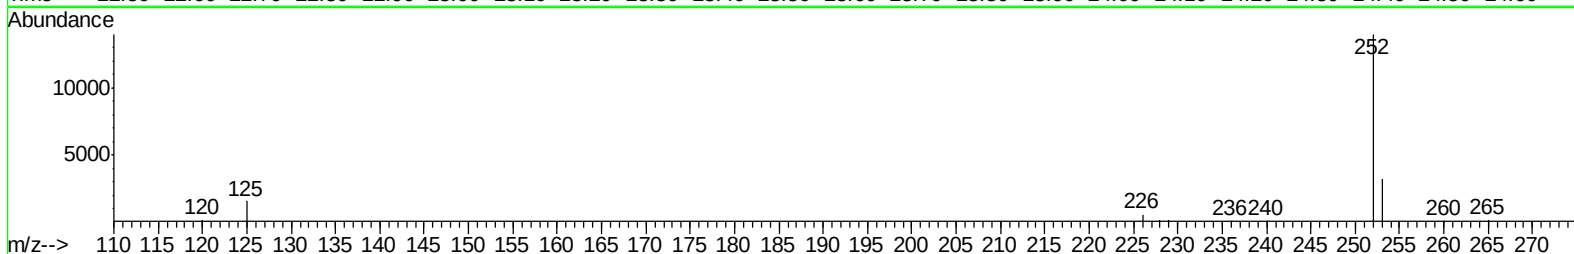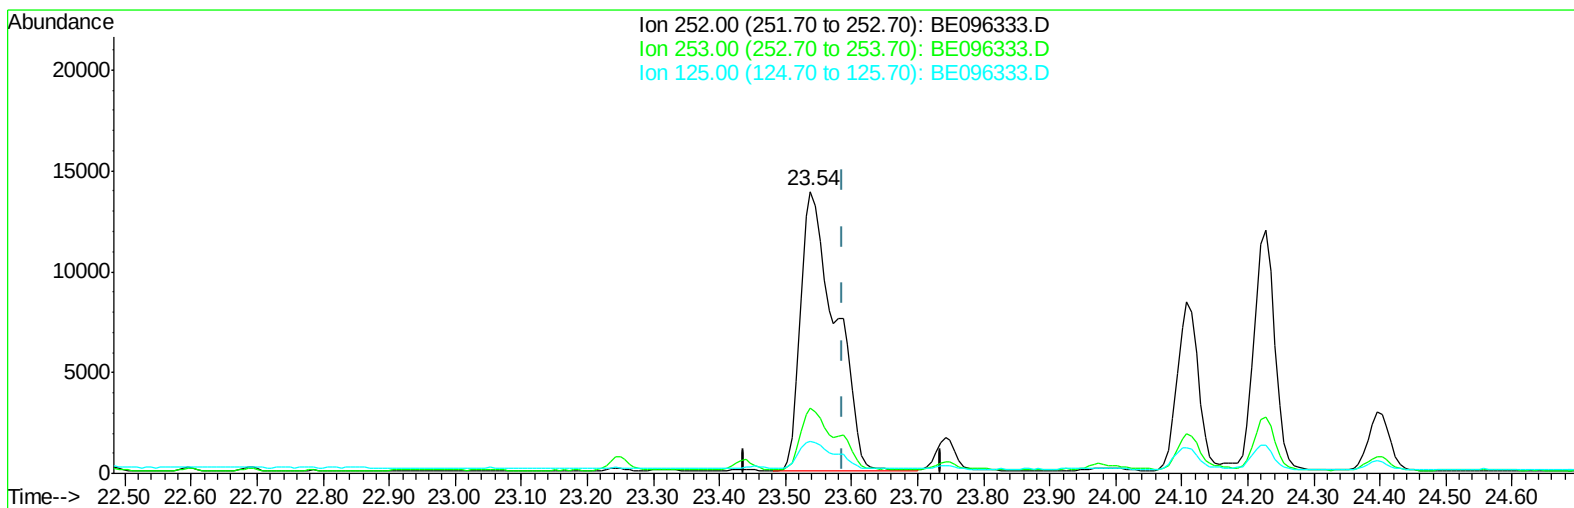

TIC: BE096333.D

(22) Benzo(k)fluoranthene

23.538min (-0.049) 3.69ng/ul

response 50723

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.01#
125.00	17.10	11.26#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096333.D
Acq On : 3 May 2018 21:17
Operator : SJ/JU
Sample : J2440-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y29

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:04 PM

Quant Time: May 04 03:00:00 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

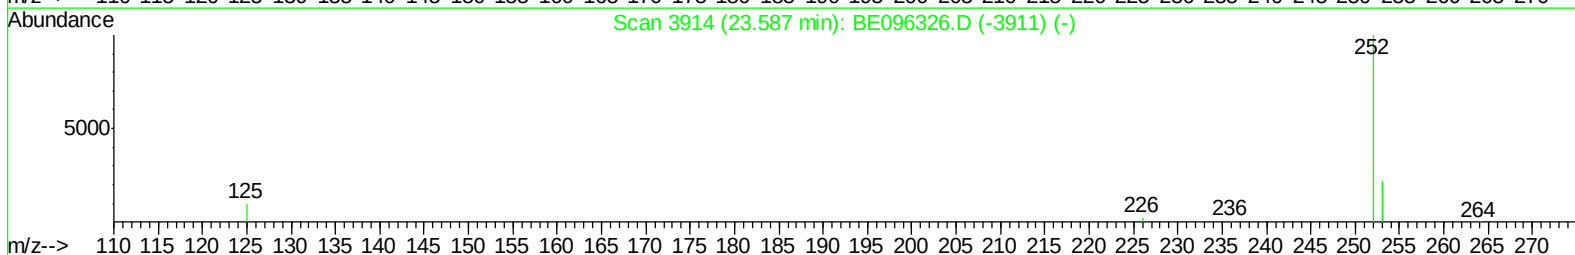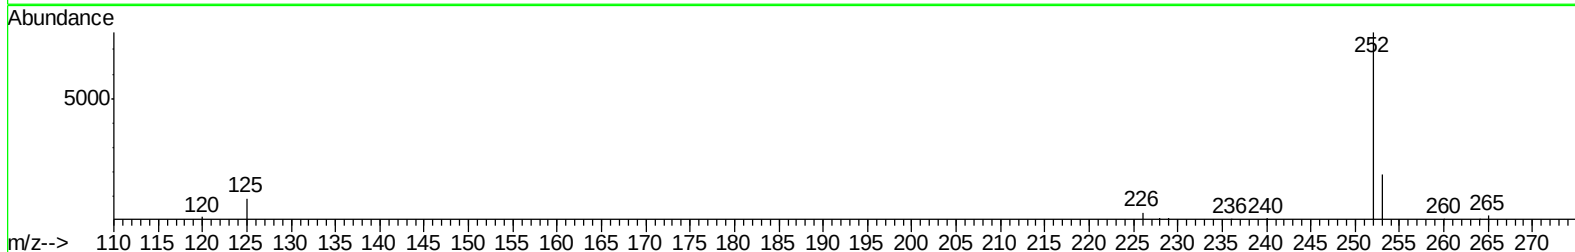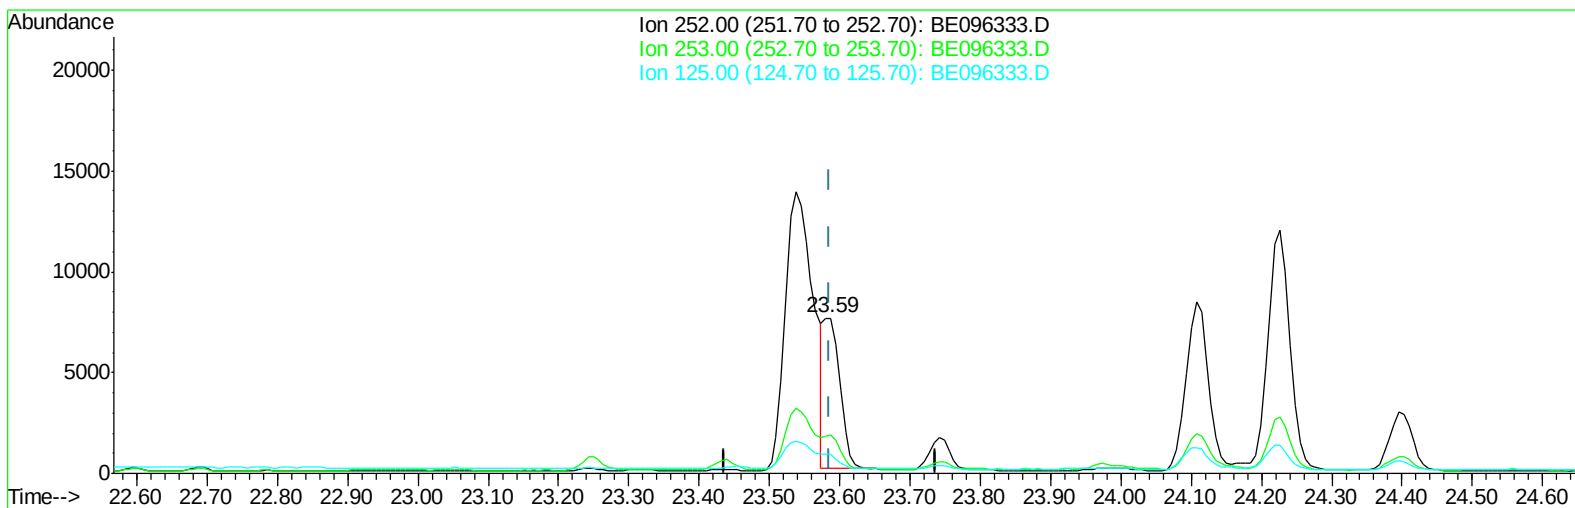

TIC: BE096333.D

(22) Benzo(k)fluoranthene

23.587min (+0.000) 0.86ng/ul m

response 11764

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	24.55
125.00	17.10	12.06#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
 Data File : BE096333.D
 Acq On : 3 May 2018 21:17
 Operator : SJ/JU
 Sample : J2440-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y29

Manual Integrations
 APPROVED

Sohil
 5/4/2018 1:35:04 PM

Quant Time: May 04 03:00:56 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 04 01:53:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	653	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	2816	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.94	164	1811	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.65	188	4667m	0.40	ng/ul	0.00
16) Chrysene-d12	21.74	240	5418m	0.40	ng/ul	0.00
20) Perylene-d12	24.34	264	4156m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.73	152	946	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.63	212	3229m	0.16	ng/ul	0.00
Target Compounds					Ovalue	
3) Naphthalene	11.22	128	26262	3.393	ng/ul#	88
5) 2-Methylnaphthalene	12.80	142	3056	0.594	ng/ul	100
7) Acenaphthylene	14.67	152	829	0.088	ng/ul#	86
8) Acenaphthene	15.00	153	4790	0.706	ng/ul	93
9) Fluorene	15.97	166	6375	0.693	ng/ul#	91
12) Phenanthrene	17.69	178	53537m	3.812	ng/ul	
13) Anthracene	17.78	178	8513m	0.627	ng/ul	
15) Fluoranthene	19.66	202	64166m	3.210	ng/ul	
17) Pyrene	20.02	202	15024	2.465	ng/ul#	73
18) Benzo(a)anthracene	21.73	228	12629m	1.492	ng/ul	
19) Chrysene	21.78	228	31850	1.969	ng/ul	98
21) Benzo(b)fluoranthene	23.54	252	38482m	2.706	ng/ul	
22) Benzo(k)fluoranthene	23.59	252	11764m	0.856	ng/ul	
23) Benzo(a)pyrene	24.23	252	26029	1.954	ng/ul#	78
24) Indeno(1,2,3-cd)pyrene	27.11	276	15725	1.066	ng/ul#	73
25) Dibenzo(a,h)anthracene	27.12	278	3882	0.322	ng/ul	97
26) Benzo(a,h,i)perylene	27.97	276	14916	1.201	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

