

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
 Data File : BE096332.D
 Acq On : 3 May 2018 20:41
 Operator : SJ/JU
 Sample : J2440-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y22

Manual Integrations
 APPROVED

Sohil
 5/4/2018 1:35:02 PM

Quant Time: May 04 02:43:35 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 04 01:53:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	611	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	2622	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.94	164	1704	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.65	188	4456m	0.40	ng/ul	0.00
16) Chrysene-d12	21.74	240	5243m	0.40	ng/ul	0.00
20) Perylene-d12	24.34	264	3886m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.73	152	1168	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.63	212	4212m	0.22	ng/ul	0.00
Target Compounds						
15) Fluoranthene	19.66	202	539m	0.028	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE050318\
Data File : BE096332.D
Acq On : 3 May 2018 20:41
Operator : SJ/JU
Sample : J2440-13
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
A3Y22

Manual Integrations
APPROVED

Sohil
5/4/2018 1:35:02 PM

Quant Time: May 04 02:43:35 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE050318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 04 01:53:25 2018
Response via : Initial Calibration

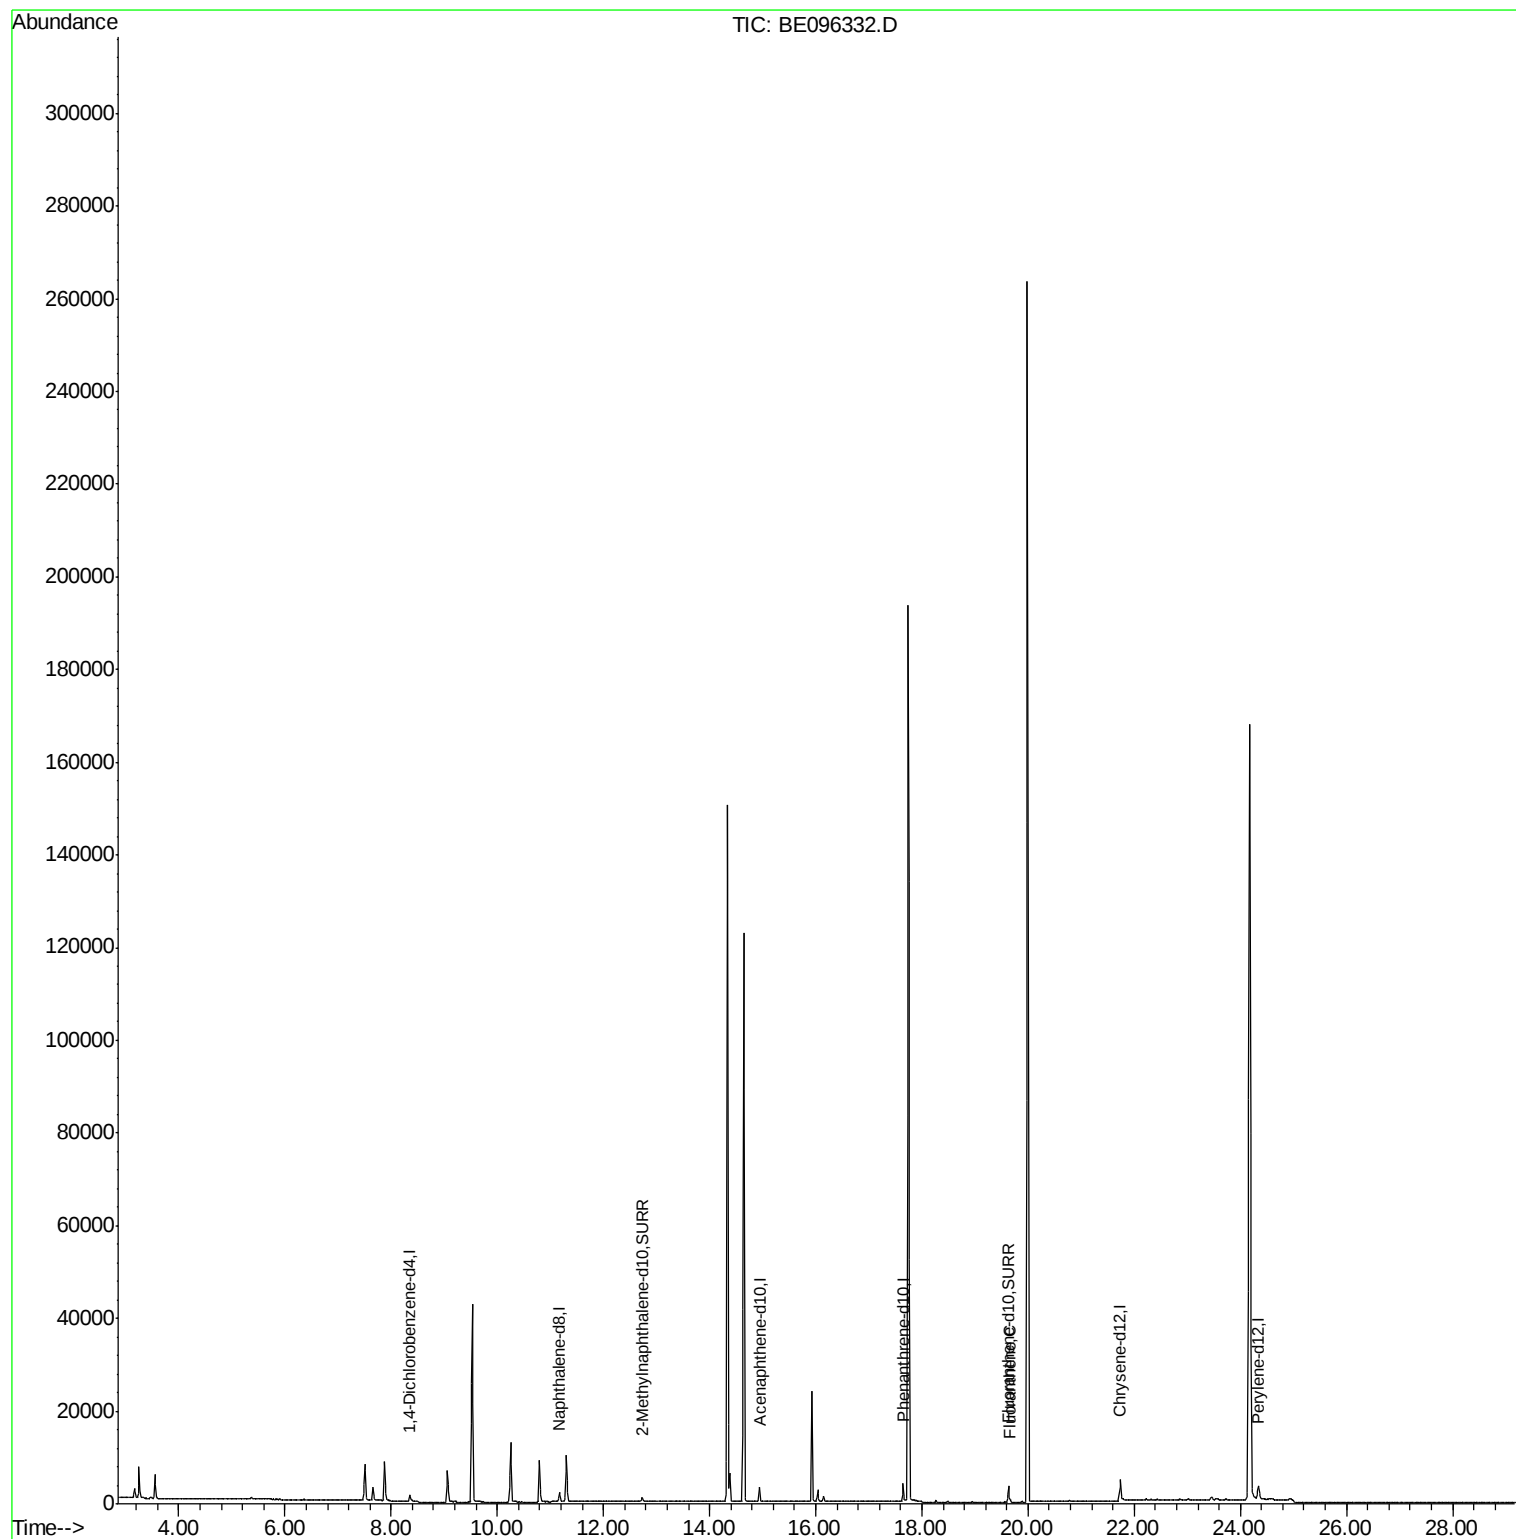

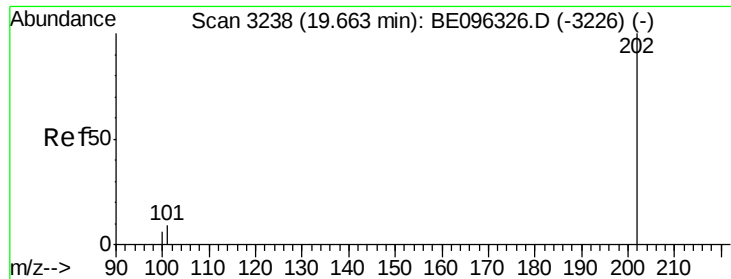

#15
 Fluoranthene
 Concen: 0.028 ng/ul m
 RT: 19.66 min Scan# 3238
 Delta R.T. -0.00 min
 Lab File: BE096332.D
 Acq: 3 May 2018 20:41

Instrument :
 BNA_E
 ClientSampleId :
 A3Y22

Tot Ion:	202	Resp:	539
Ion Ratio	Lower	Upper	
202	100		
101	19.3	0.0	30.3
100	16.7	0.0	39.5

Manual Integrations
 APPROVED

Sohil
 5/4/2018 1:35:02 PM

