

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050517\
 Data File : BE092936.D
 Acq On : 5 May 2017 19:11
 Operator : SJ/MA
 Sample : PB98667BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: May 06 01:48:33 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE050517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 05 14:05:07 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	976	0.40	ng	0.00
7) Naphthalene-d8	10.53	136	3818	0.40	ng	0.00
13) Acenaphthene-d10	14.39	164	1550	0.40	ng	0.00
19) Phenanthrene-d10	17.13	188	3562	0.40	ng	0.00
26) Chrysene-d12	21.28	240	2739	0.40	ng	0.00
33) Perylene-d12	23.69	264	2297	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.36	112	847	0.39	ng	0.00
5) Phenol-d6	6.94	99	1091	0.36	ng	0.00
8) Nitrobenzene-d5	8.90	82	922	0.36	ng	0.00
11) 2-Methylnaphthalene-d10	12.13	152	2086	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.87	330	75	0.31	ng	0.00
15) 2-Fluorobiphenyl	13.01	172	2382	0.33	ng	0.00
24) Fluoranthene-d10	19.15	212	2236	0.27	ng	0.00
28) Terphenyl-d14	19.74	244	1772	0.37	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.32	88	415	0.22	ng	# 90
3) n-Nitrosodimethylamine	3.61	42	467	0.32	ng	# 84
6) bis(2-Chloroethyl)ether	7.20	93	1119	0.31	ng	# 98
9) Naphthalene	10.58	128	3149	0.31	ng	# 87
10) Hexachlorobutadiene	10.89	225	436	0.31	ng	# 96
12) 2-Methylnaphthalene	12.19	142	1959	0.31	ng	# 95
16) Acenaphthylene	14.10	152	8233	0.34	ng	# 99
17) Acenaphthene	14.44	154	1591	0.33	ng	# 95
18) Fluorene	15.43	166	1797	0.30	ng	# 98
20) Hexachlorobenzene	16.47	284	462	0.30	ng	# 100
21) Pentachlorophenol	16.79	266	167	0.59	ng	# 79
22) Phenanthrene	17.18	178	3079	0.31	ng	# 99
23) Anthracene	17.27	178	2422	0.32	ng	# 99
25) Fluoranthene	19.17	202	11551	0.27	ng	# 98
27) Pyrene	19.53	202	12277	0.35	ng	# 97
29) Benzo(a)anthracene	21.25	228	2259	0.35	ng	# 89
30) Chrysene	21.30	228	2671	0.33	ng	# 90
31) Bis(2-ethylhexyl)phthalate	21.20	149	598	0.34	ng	# 94
32) Indeno(1,2,3-cd)pyrene	26.22	276	10677	0.36	ng	# 99
34) Benzo(b)fluoranthene	22.95	252	2317	0.31	ng	# 87
35) Benzo(k)fluoranthene	23.00	252	2314	0.31	ng	# 83
36) Benzo(a)pyrene	23.57	252	1995	0.32	ng	# 77
37) Dibenzo(a,h)anthracene	26.25	278	2235	0.32	ng	# 81
38) Benzo(g,h,i)perylene	26.99	276	9442	0.32	ng	# 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050517\
Data File : BE092936.D
Acq On : 5 May 2017 19:11
Operator : SJ/MA
Sample : PB98667BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: May 06 01:48:33 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE050517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 14:05:07 2017
Response via : Initial Calibration

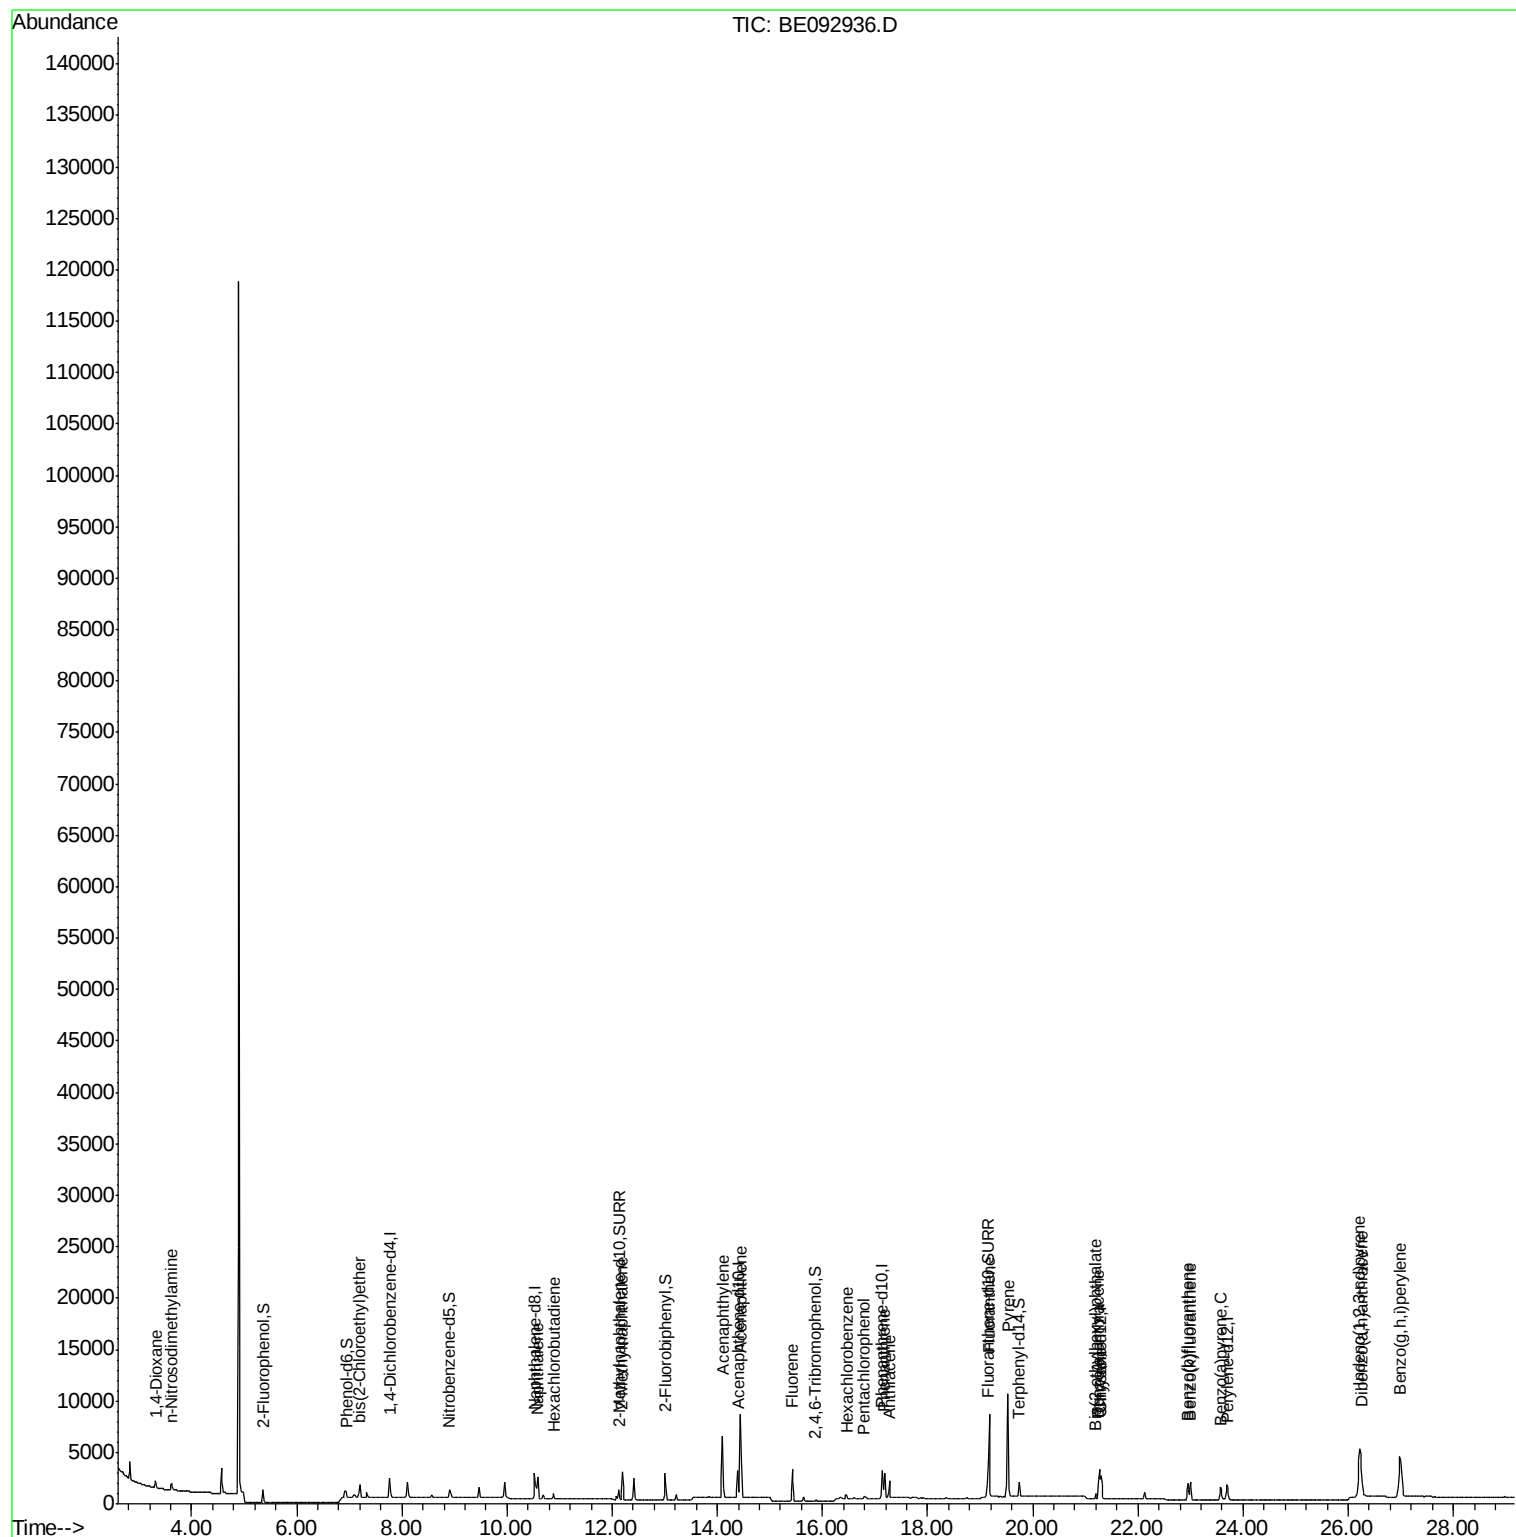

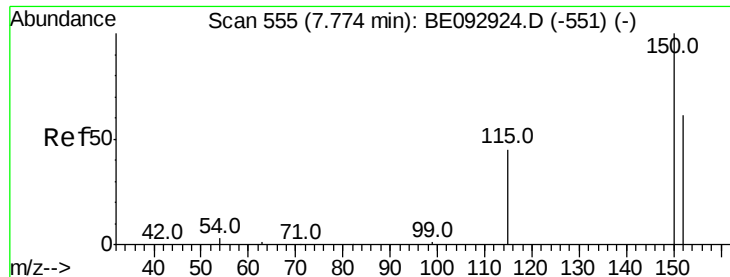


#1




1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.77 min Scan# 555
Delta R.T. 0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11

Instrument :
BNA_E
ClientSampleId :

Tot Ion:152 Resp: 976
Ion Ratio Lower Upper
152 100
150 167.9 129.9 194.9
115 81.2 62.6 93.8

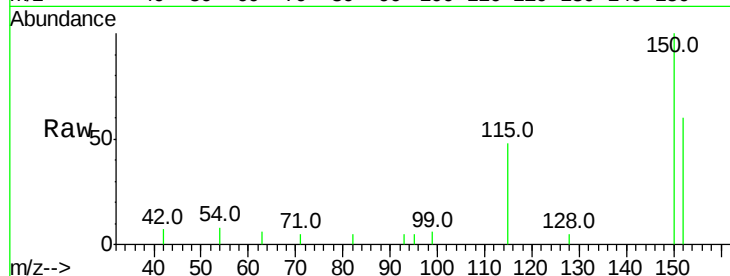


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

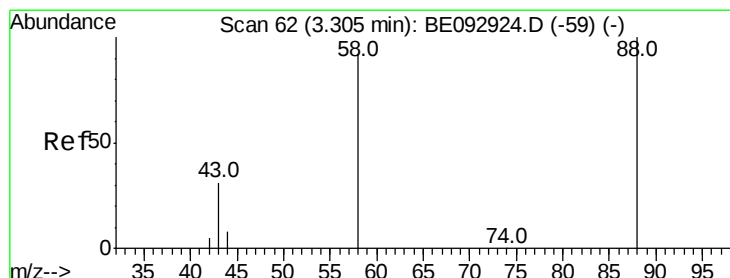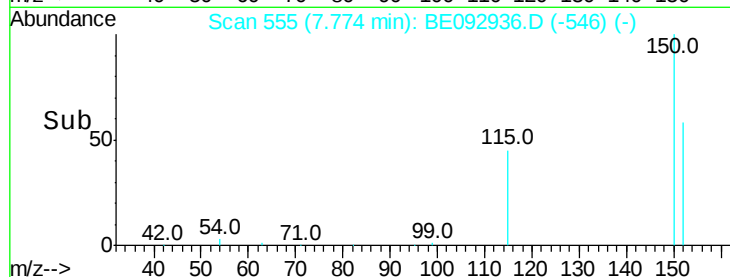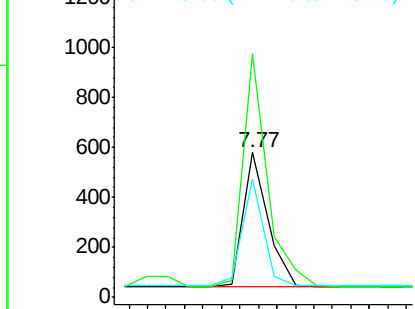



#2


1,4-Dioxane
Concen: 0.22 ng
RT: 3.32 min Scan# 63
Delta R.T. 0.01 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11

Tgt Ion: 88 Resp: 415
Ion Ratio Lower Upper
88 100
58 84.1 64.9 97.3
43 47.7 26.6 40.0#

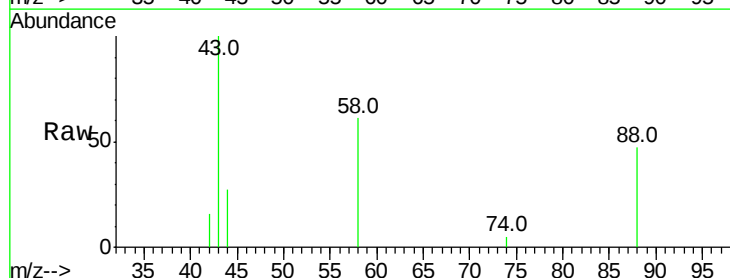

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

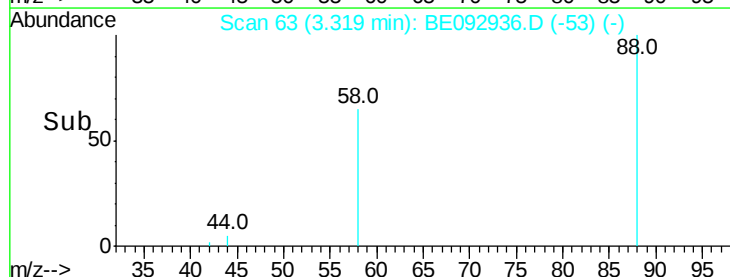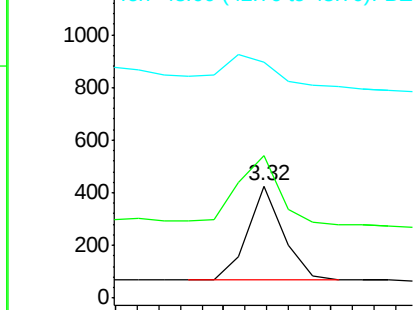



#3

n-Nitrosodimethylamine

Concen: 0.32 ng

RT: 3.61 min Scan# 88

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 42 Resp: 467

Ion Ratio Lower Upper

42 100

74 123.6 106.6 160.0



44 6.0 25.7 38.5#




Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

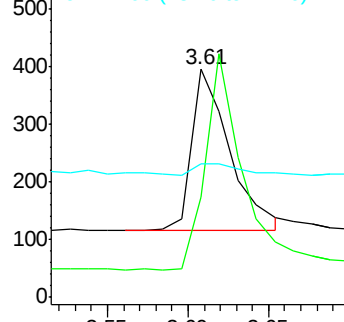

Time-->



#4

2-Fluorophenol

Concen: 0.39 ng

RT: 5.36 min Scan# 267

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11


Tgt Ion: 112 Resp: 847

Ion Ratio Lower Upper

112 100

64 70.1 52.6 79.0



63 36.0 29.0 43.4




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

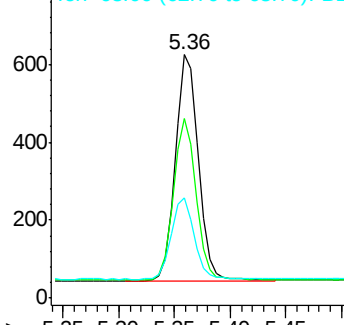

Time-->



#5

Phenol-d6

Concen: 0.36 ng

RT: 6.94 min Scan# 519

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 99 Resp: 1091

Ion Ratio Lower Upper

99 100

42 0.0 0.0 0.0




71 0.0 0.0 0.0



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

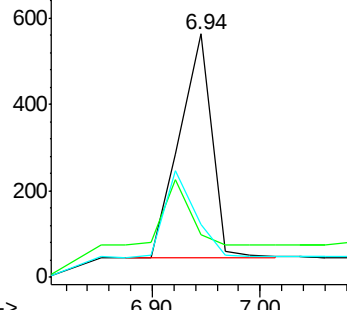

#6

bis(2-Chloroethyl)ether

Concen: 0.31 ng

RT: 7.20 min Scan# 530

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11


Tgt Ion: 93 Resp: 1119

Ion Ratio Lower Upper

93 100

63 79.2 61.2 91.8



95 32.4 25.5 38.3




Abundance Ion 93.00 (92.70 to 93.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Ion 95.00 (94.70 to 95.70): BE0

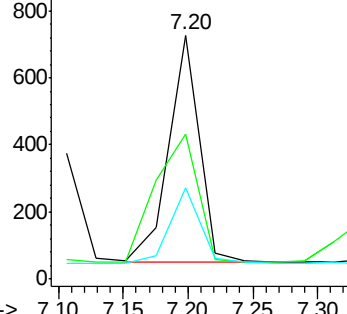



#7

Naphthalene-d8

Concen: 0.40 ng

RT: 10.53 min Scan# 678

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11

Instrument :

BNA_E

ClientSampleId :

Tot Ion:136 Resp: 3818


Ion Ratio Lower Upper

136 100

137 12.0 10.4 15.6

54 14.1 12.6 18.8

68 12.2 10.7 16.1






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

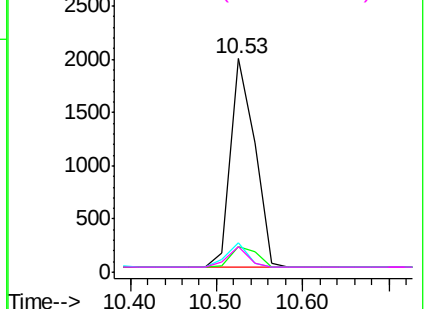

#8

Nitrobenzene-d5

Concen: 0.36 ng

RT: 8.90 min Scan# 604

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11


Tgt Ion: 82 Resp: 922

Ion Ratio Lower Upper

82 100

128 19.6 35.3 52.9#



54 71.3 65.1 97.7




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

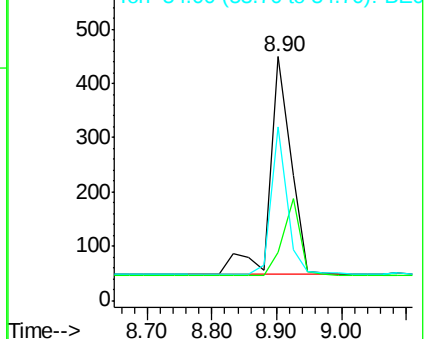



#9

Naphthalene

Concen: 0.31 ng

RT: 10.58 min Scan# 681

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11

Instrument :

BNA_E

ClientSampleId :





Tot Ion:128 Resp: 3149

Ion Ratio Lower Upper

128 100

129 13.8 15.8 23.8#

127 14.0 16.0 24.0#

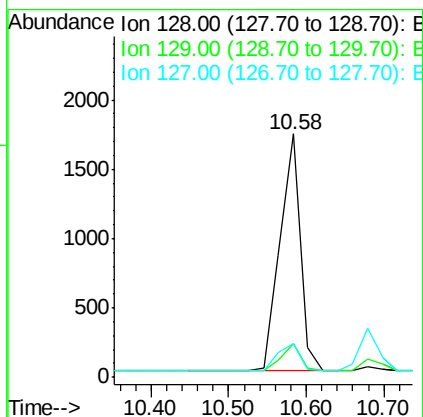

#10

Hexachlorobutadiene

Concen: 0.31 ng

RT: 10.89 min Scan# 697

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11




Tgt Ion:225 Resp: 436


Ion Ratio Lower Upper

225 100

223 64.0 55.4 83.2

227 63.5 52.2 78.4



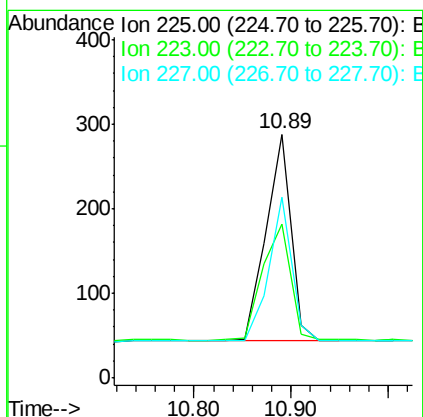



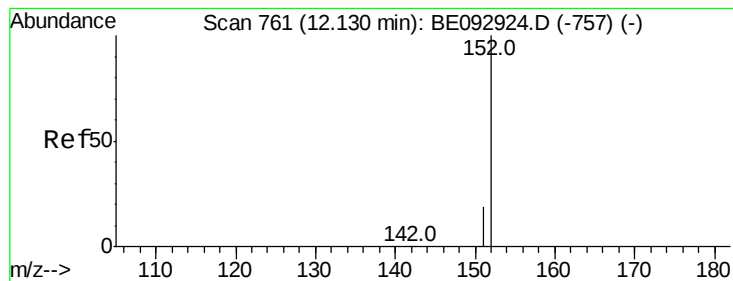

#11
 2-Methylnaphthalene-d10
 Concen: 0.37 ng
 RT: 12.13 min Scan# 761
 Delta R.T. 0.00 min
 Lab File: BE092936.D
 Acq: 5 May 2017 19:11




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:152 Resp: 2086
 Ion Ratio Lower Upper
 152 100
 151 15.1 15.7 23.5#

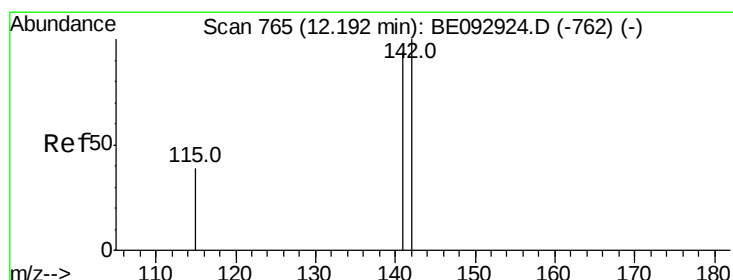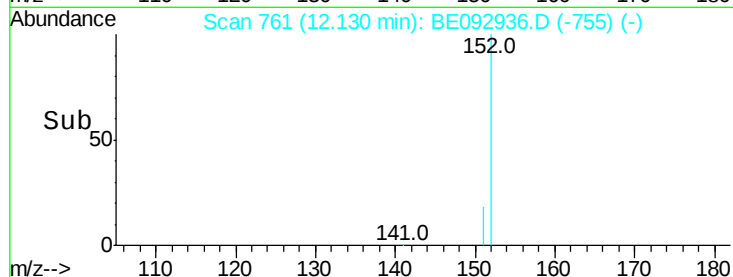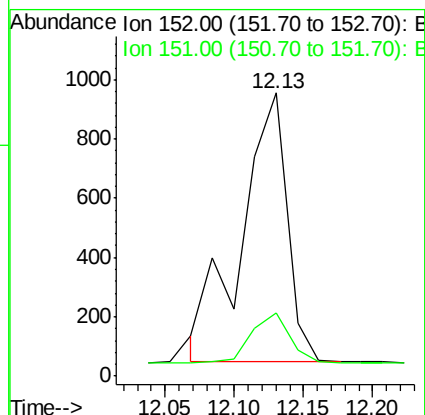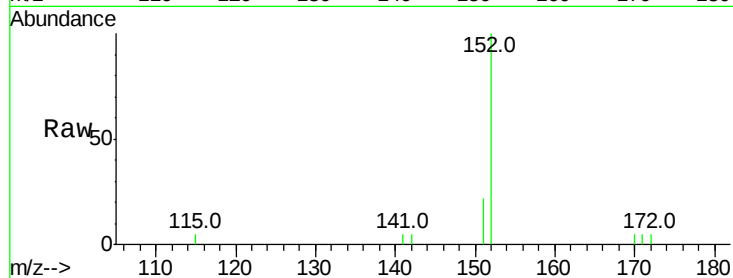

#12
 2-Methylnaphthalene
 Concen: 0.31 ng
 RT: 12.19 min Scan# 765
 Delta R.T. 0.00 min
 Lab File: BE092936.D
 Acq: 5 May 2017 19:11

Tgt Ion:142 Resp: 1959
 Ion Ratio Lower Upper
 142 100
 141 94.4 76.0 114.0
 115 43.2 41.6 62.4


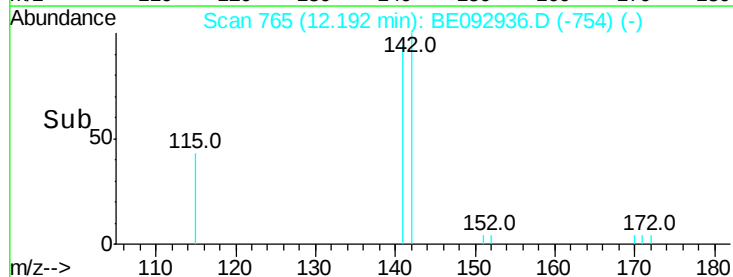
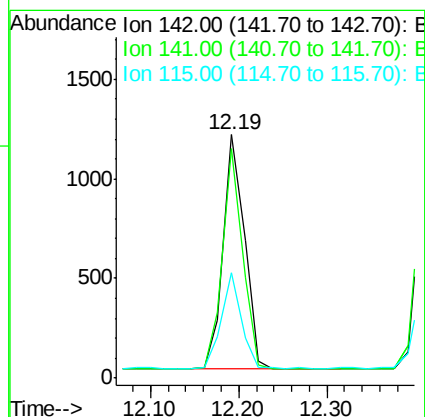
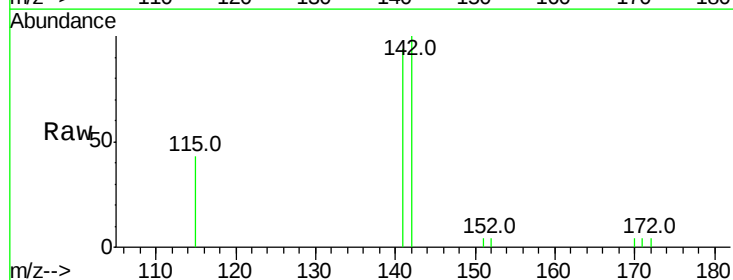




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.39 min Scan# 901
Delta R.T. 0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11




Instrument :
BNA_E
ClientSampleId :


Tot Ion:164 Resp: 1550
Ion Ratio Lower Upper
164 100
162 103.7 86.6 130.0
160 48.6 44.5 66.7

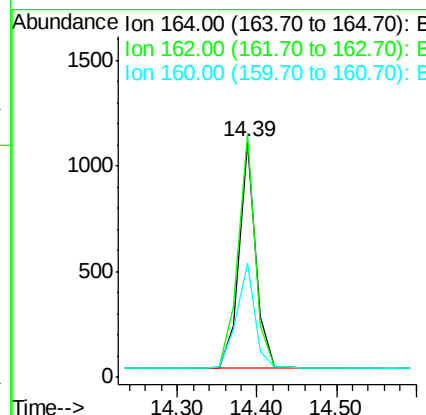

#14
2,4,6-Tribromophenol
Concen: 0.31 ng
RT: 15.87 min Scan# 1010
Delta R.T. -0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11

Tgt Ion:330 Resp: 75
Ion Ratio Lower Upper
330 100
332 96.0 69.1 103.7
141 58.7 54.6 81.8

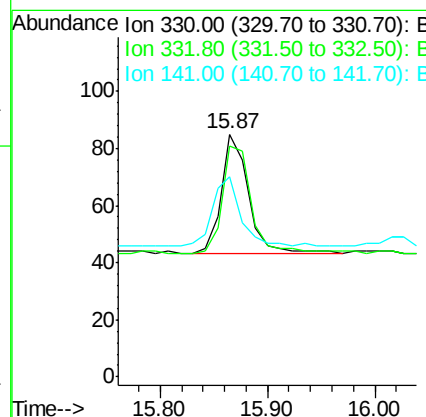

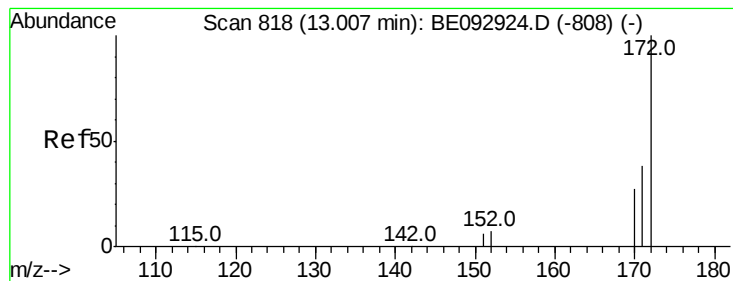

#15

2-Fluorobiphenyl

Concen: 0.33 ng

RT: 13.01 min Scan# 818

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11

Instrument :

BNA_E

ClientSampleId :


Tot Ion:172 Resp: 2382

Ion Ratio Lower Upper

172 100

171 38.2 35.8 53.6




170 27.2 28.5 42.7#

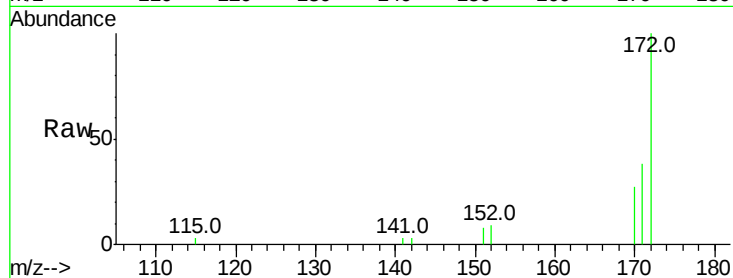

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

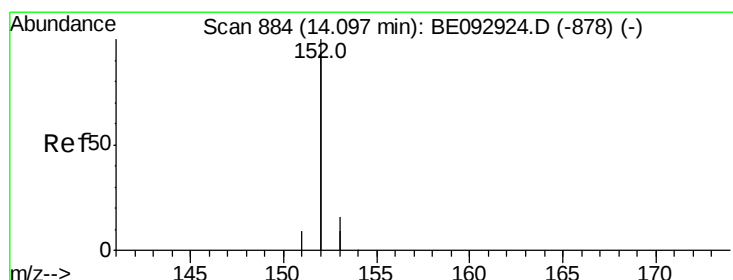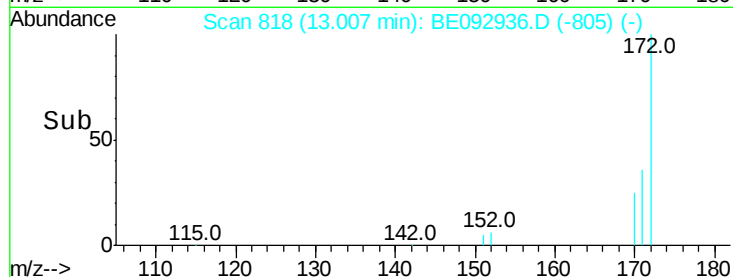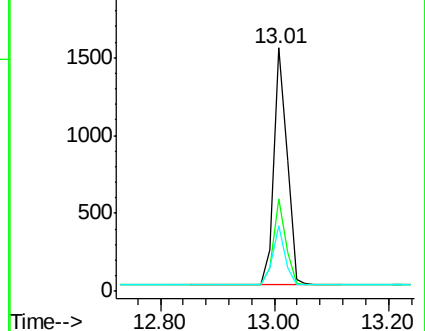

#16

Acenaphthylene

Concen: 0.34 ng

RT: 14.10 min Scan# 884

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11


Tgt Ion:152 Resp: 8233

Ion Ratio Lower Upper

152 100

151 4.8 3.8 5.8



153 13.1 10.0 15.0

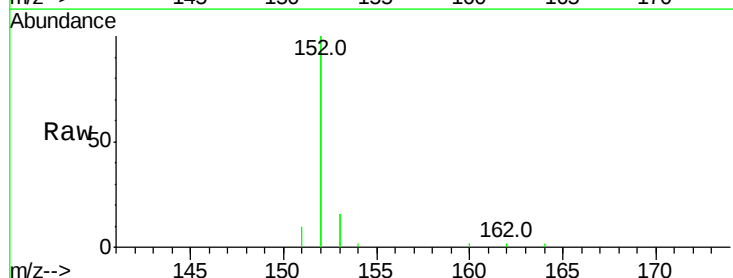


Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E



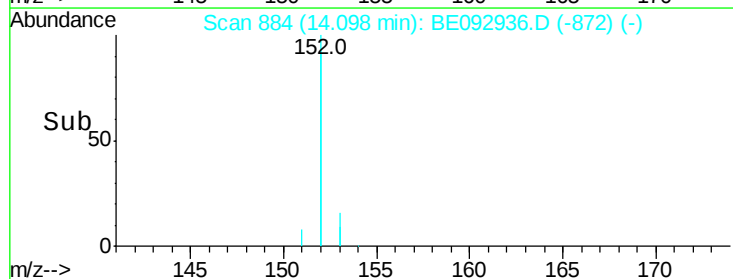
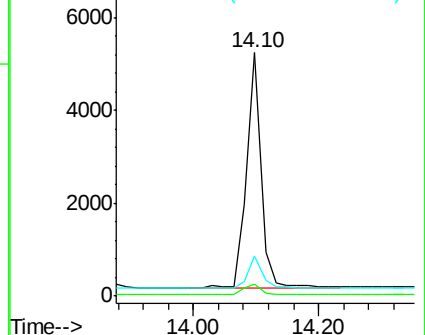




#17
Acenaphthene
Concen: 0.33 ng
RT: 14.44 min Scan# 904
Delta R.T. -0.02 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11




Instrument :
BNA_E
ClientSampleId :


Tot Ion:154 Resp: 1591
Ion Ratio Lower Upper
154 100
153 455.9 355.6 533.4
152 230.2 177.8 266.8

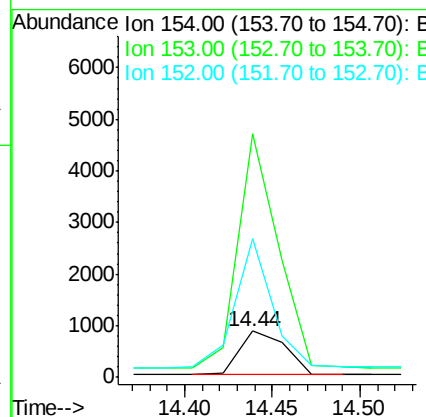

#18
Fluorene
Concen: 0.30 ng
RT: 15.43 min Scan# 972
Delta R.T. -0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11

Tgt Ion:166 Resp: 1797
Ion Ratio Lower Upper
166 100
165 99.0 80.7 121.1
167 14.1 11.3 16.9

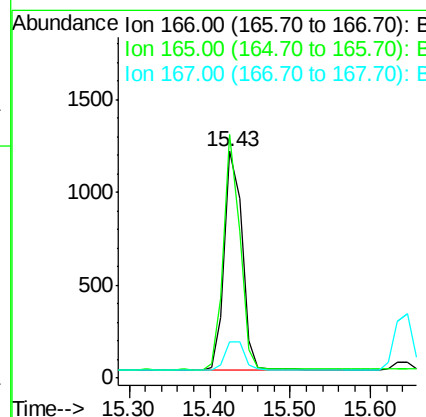



#19

Phenanthrene-d10

Concen: 0.40 ng

RT: 17.13 min Scan# 1078

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11

Instrument :

BNA_E

ClientSampleId :


Tot Ion:188 Resp: 3562

Ion Ratio Lower Upper

188 100

94 11.5 10.2 15.4




80 11.3 10.6 15.8



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

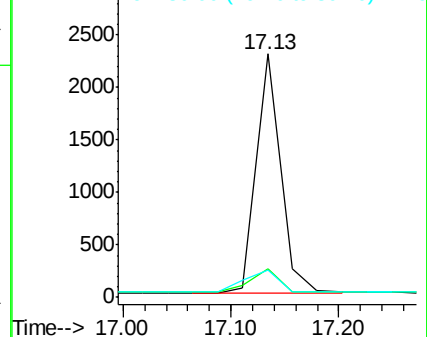

#20

Hexachlorobenzene

Concen: 0.30 ng

RT: 16.47 min Scan# 1049

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11


Tgt Ion:284 Resp: 462

Ion Ratio Lower Upper

284 100

142 0.0 0.0 0.0



249 0.0 0.0 0.0




Abundance Ion 283.80 (283.50 to 284.50): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

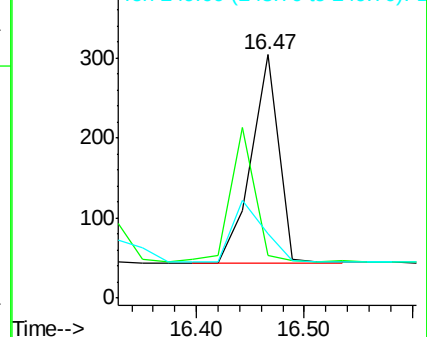







#21
 Pentachlorophenol
 Concen: 0.59 ng
 RT: 16.79 min Scan# 1063
 Delta R.T. 0.00 min
 Lab File: BE092936.D
 Acq: 5 May 2017 19:11

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:266 Resp: 167
 Ion Ratio Lower Upper
 266 100
 264 78.6 75.4 113.2
 268 69.8 75.4 113.2#




Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E


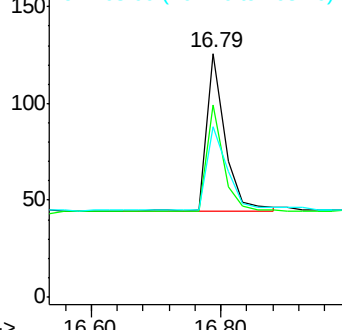



#22
 Phenanthrene
 Concen: 0.31 ng
 RT: 17.18 min Scan# 1080
 Delta R.T. 0.00 min
 Lab File: BE092936.D
 Acq: 5 May 2017 19:11

Tgt Ion:178 Resp: 3079
 Ion Ratio Lower Upper
 178 100
 176 18.4 14.2 21.4
 179 16.3 13.6 20.4



Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

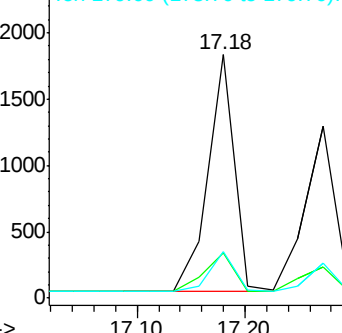



#23

Anthracene

Concen: 0.32 ng

RT: 17.27 min Scan# 1084

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 2422

Ion Ratio Lower Upper

178 100

176 17.9 14.7 22.1




179 16.0 12.8 19.2



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

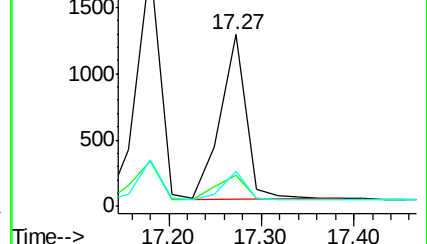

#24

Fluoranthene-d10

Concen: 0.27 ng

RT: 19.15 min Scan# 1165

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11


Tgt Ion:212 Resp: 2236

Ion Ratio Lower Upper

212 100

106 0.0 0.0 0.0



104 0.0 0.0 0.0




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

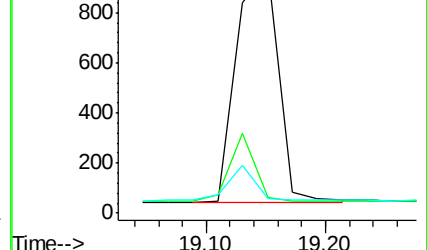



#25

Fluoranthene

Concen: 0.27 ng

RT: 19.17 min Scan# 1166

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 11551

Ion Ratio Lower Upper

202 100

101 0.0 0.0 0.0




203 18.2 15.3 22.9

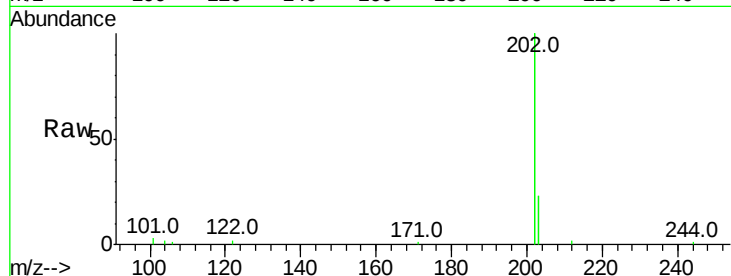

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

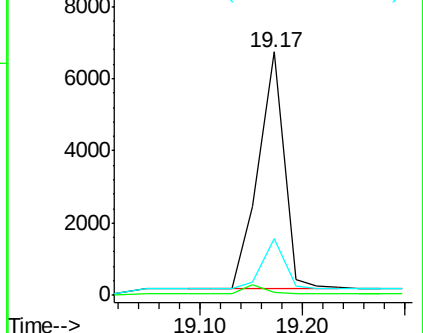

#26

Chrysene-d12

Concen: 0.40 ng

RT: 21.28 min Scan# 1268

Delta R.T. 0.00 min

Lab File: BE092936.D

Acq: 5 May 2017 19:11


Tgt Ion:240 Resp: 2739

Ion Ratio Lower Upper

240 100

120 5.0 4.6 6.8



236 23.1 19.8 29.8




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E




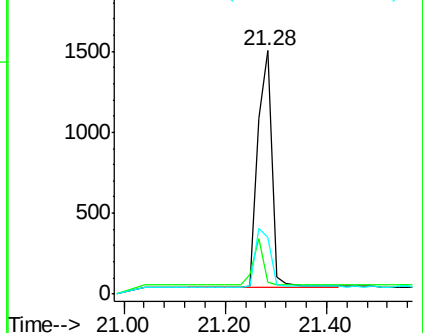




#27
Pvrene
Concen: 0.35 ng
RT: 19.53 min Scan# 1183
Delta R.T. 0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11




Instrument :
BNA_E
ClientSampleId :


Tot Ion:202 Resp: 12277
Ion Ratio Lower Upper
202 100
200 0.0 0.0 0.0
203 18.2 13.5 20.3

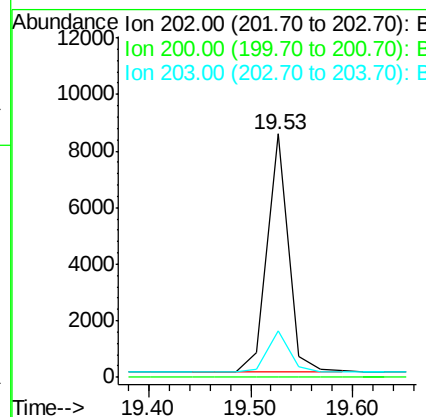

#28
Terphenyl-d14
Concen: 0.37 ng
RT: 19.74 min Scan# 1193
Delta R.T. 0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11

Tgt Ion:244 Resp: 1772
Ion Ratio Lower Upper
244 100
212 12.9 18.4 27.6#
122 16.5 23.3 34.9#



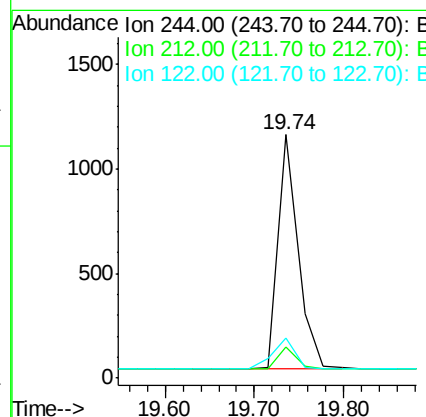





#29
Benzo(a)anthracene
Concen: 0.35 ng
RT: 21.25 min Scan# 1266
Delta R.T. 0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11




Instrument :
BNA_E
ClientSampled :


Tot Ion:228 Resp: 2259
Ion Ratio Lower Upper
228 100
226 35.0 32.0 48.0
229 18.3 21.4 32.0#

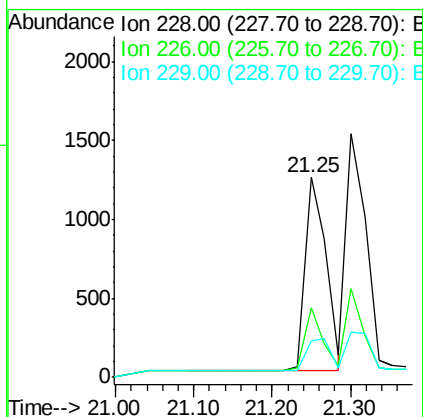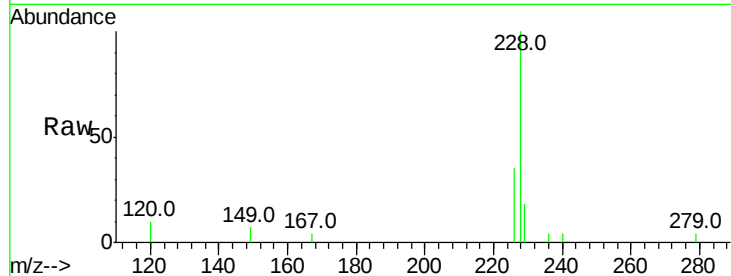

#30
Chrysene
Concen: 0.33 ng
RT: 21.30 min Scan# 1269
Delta R.T. 0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11

Tgt Ion:228 Resp: 2671
Ion Ratio Lower Upper
228 100
226 36.4 34.2 51.2
229 18.5 18.6 28.0#

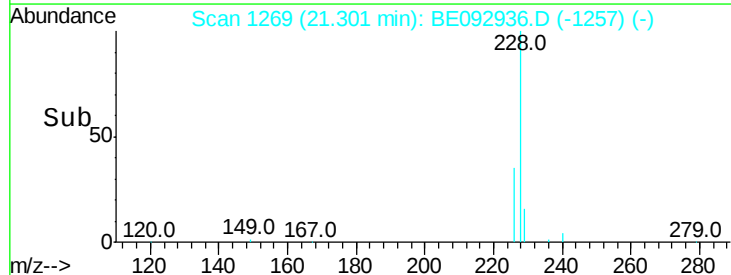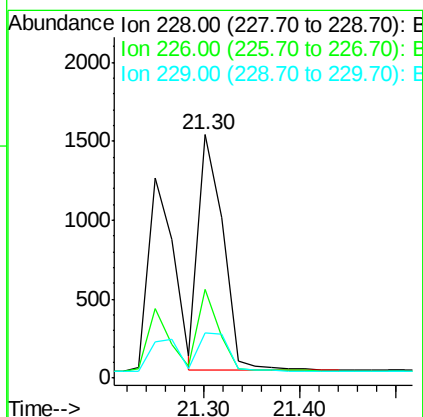







#31
 Bis(2-ethylhexyl)phthalate
 Concen: 0.34 ng
 RT: 21.20 min Scan# 1263
 Delta R.T. 0.00 min
 Lab File: BE092936.D
 Acq: 5 May 2017 19:11

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:149 Resp: 598
 Ion Ratio Lower Upper
 149 100
 167 23.2 20.9 31.3
 279 0.0 0.0 0.0

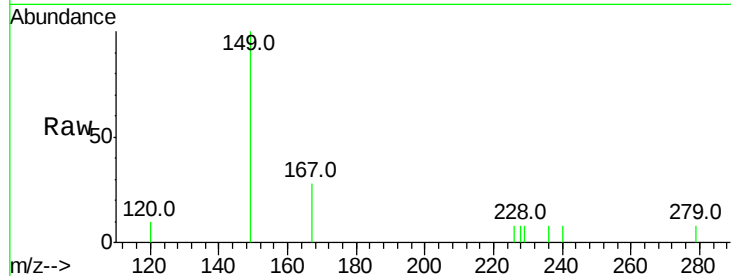


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E


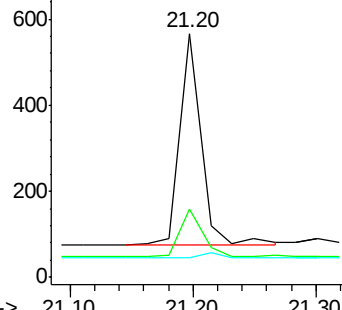



#32
 Indeno(1,2,3-cd)pyrene
 Concen: 0.36 ng
 RT: 26.22 min Scan# 1650
 Delta R.T. -0.00 min
 Lab File: BE092936.D
 Acq: 5 May 2017 19:11

Tgt Ion:276 Resp: 10677
 Ion Ratio Lower Upper
 276 100
 138 32.7 25.8 38.6
 277 25.2 20.2 30.4



Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E




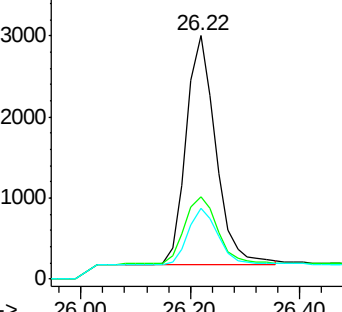


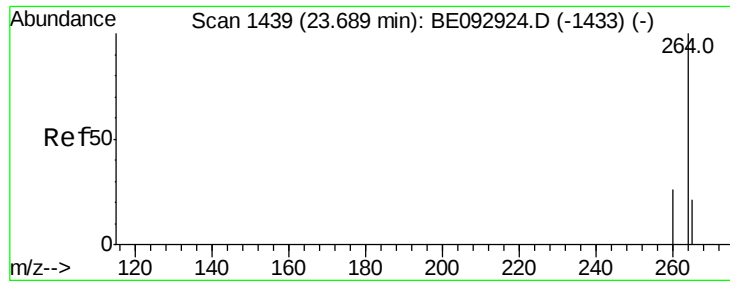

#33
 Pervlene-d12
 Concen: 0.40 ng
 RT: 23.69 min Scan# 1439
 Delta R.T. 0.00 min
 Lab File: BE092936.D
 Acq: 5 May 2017 19:11




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:264 Resp: 2297
 Ion Ratio Lower Upper
 264 100
 260 28.1 23.5 35.3
 265 30.8 27.2 40.8

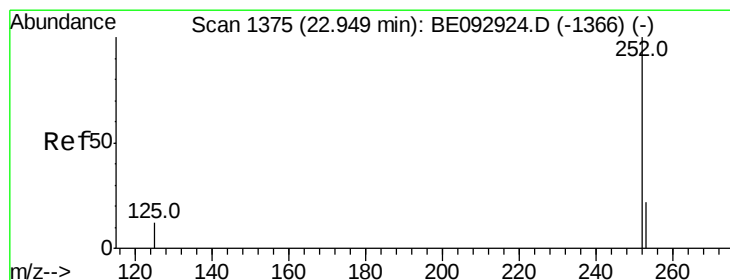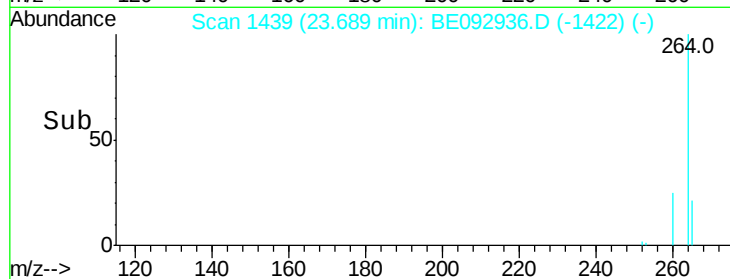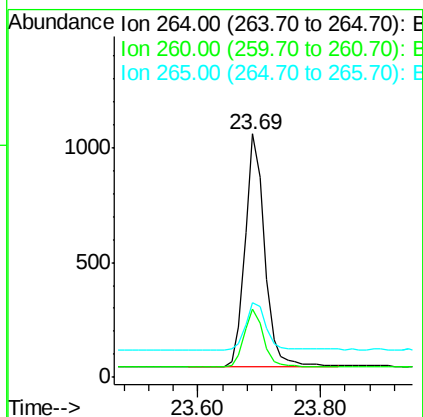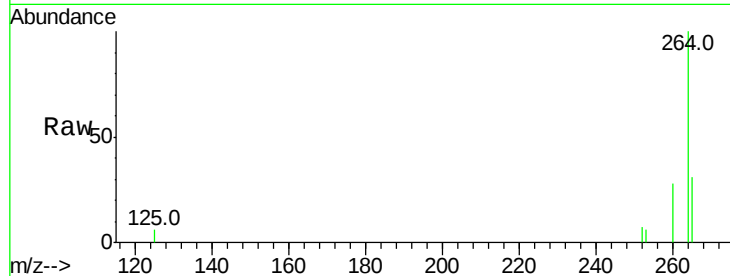

#34
 Benzo(b)fluoranthene
 Concen: 0.31 ng
 RT: 22.95 min Scan# 1375
 Delta R.T. 0.00 min
 Lab File: BE092936.D
 Acq: 5 May 2017 19:11

Tgt Ion:252 Resp: 2317
 Ion Ratio Lower Upper
 252 100
 253 25.1 24.7 37.1
 125 16.8 20.3 30.5#


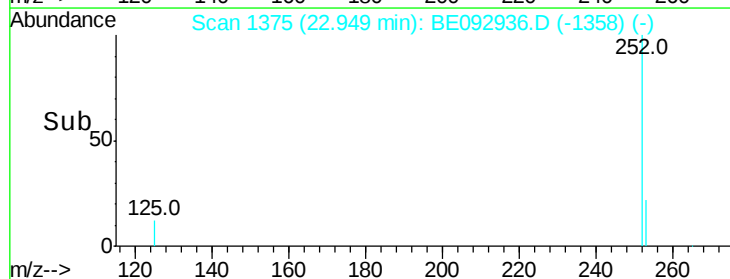
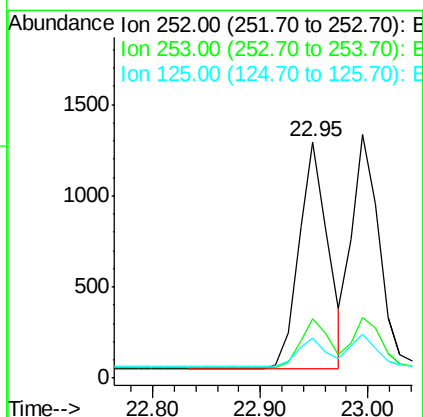
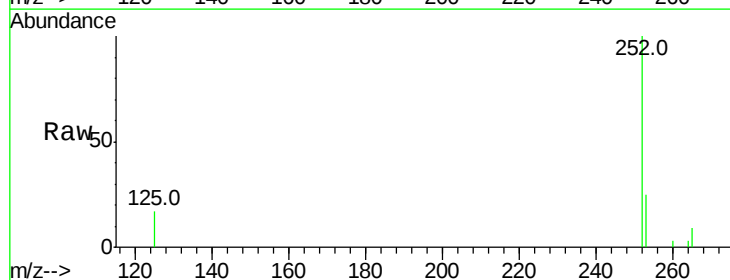




#35
Benzo(k)fluoranthene
Concen: 0.31 ng
RT: 23.00 min Scan# 1379
Delta R.T. 0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11




Instrument :
BNA_E
ClientSampleId :


Tot Ion:252 Resp: 2314
Ion Ratio Lower Upper
252 100
253 24.6 25.8 38.8#
125 18.0 22.9 34.3#

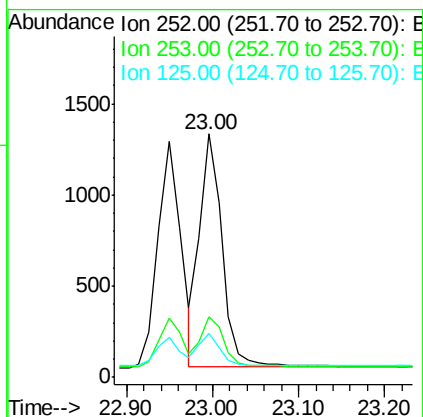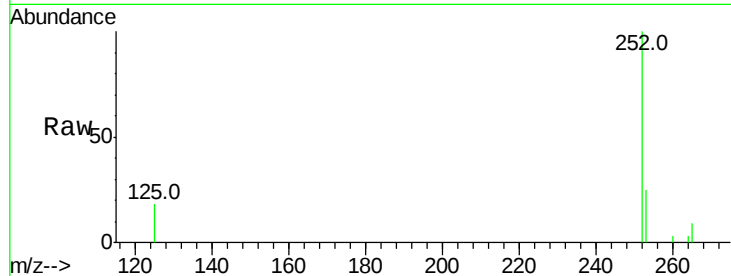

#36
Benzo(a)pyrene
Concen: 0.32 ng
RT: 23.57 min Scan# 1429
Delta R.T. -0.01 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11

Tgt Ion:252 Resp: 1995
Ion Ratio Lower Upper
252 100
253 25.3 31.3 46.9#
125 20.0 26.4 39.6#



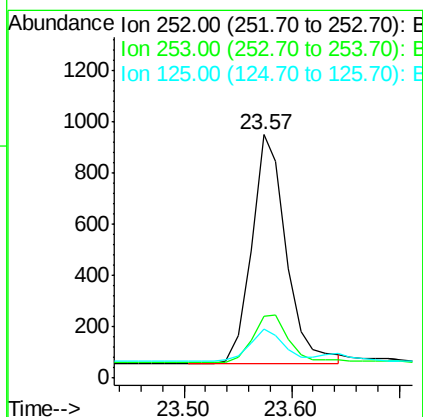





#37
Dibenzo(a,h)anthracene
Concen: 0.32 ng
RT: 26.25 min Scan# 1652
Delta R.T. -0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11

Instrument :
BNA_E
ClientSampleId :

Tot Ion:278 Resp: 2235
Ion Ratio Lower Upper
278 100
139 23.3 27.4 41.2#
279 29.3 33.3 49.9#

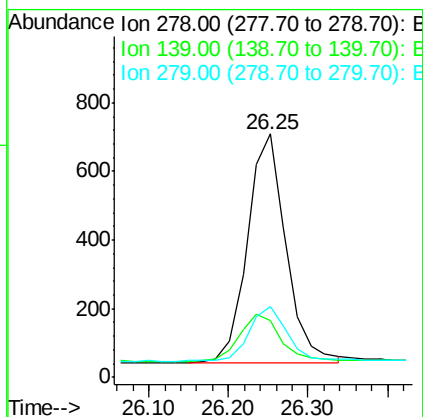

#38
Benzo(g,h,i)perylene
Concen: 0.32 ng
RT: 26.99 min Scan# 1695
Delta R.T. -0.00 min
Lab File: BE092936.D
Acq: 5 May 2017 19:11

Tgt Ion:276 Resp: 9442
Ion Ratio Lower Upper
276 100
277 27.6 29.9 44.9#
138 33.6 34.6 51.8#

