
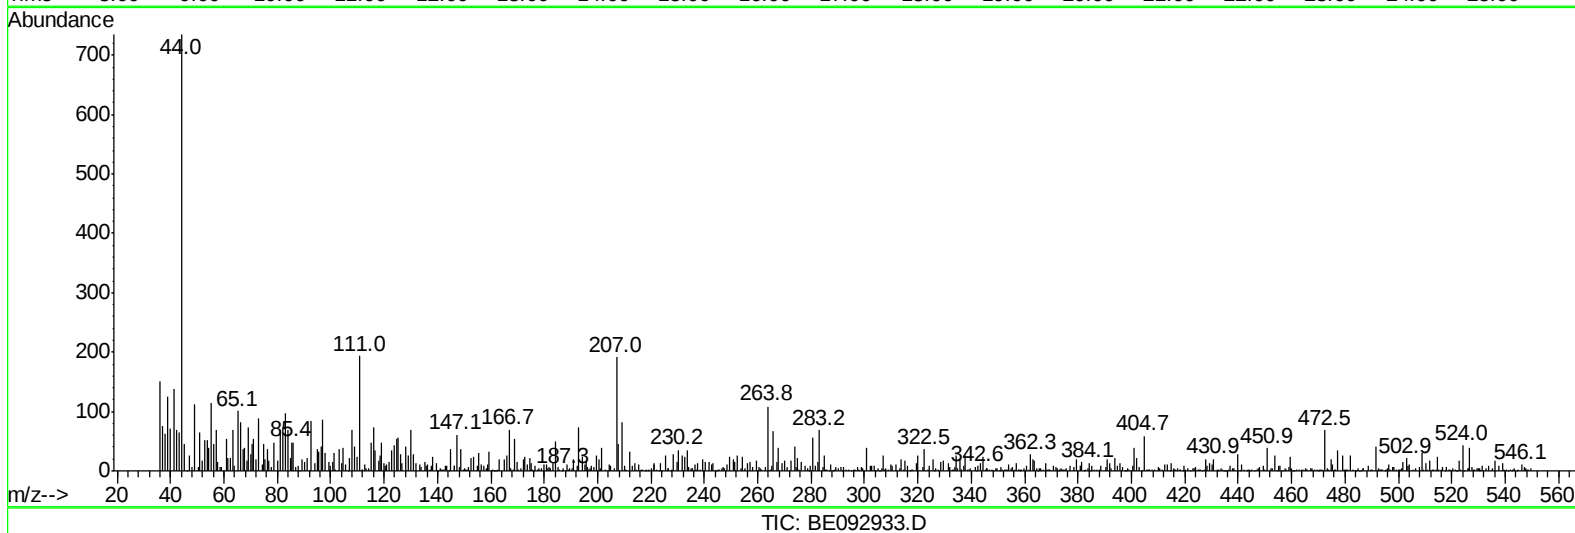


Data Path : Z:\HPCHEM1\BNA E\DATA\BE050517\
Data File : BE092933.D
Acq On : 5 May 2017 17:02
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 04:47:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

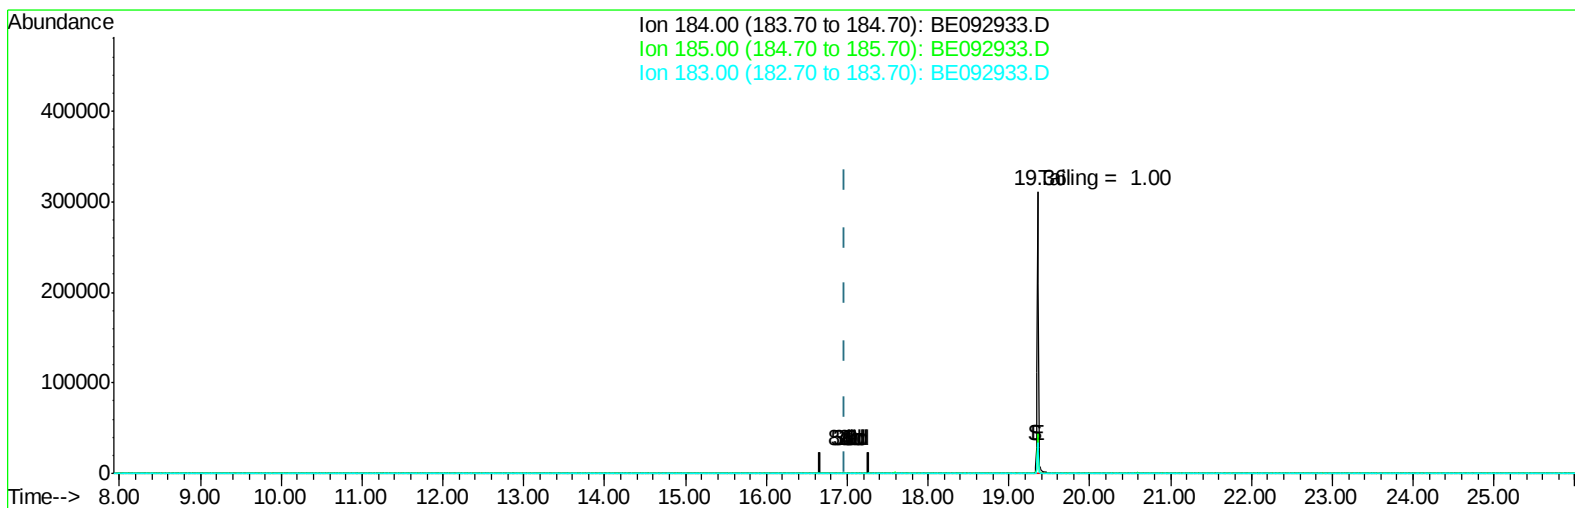

(76) Benzidine




17.006min (+0.029) 33.32ng

response 31

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	12.00#
183.00	12.20	26.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050517\
Data File : BE092933.D
Acq On : 5 May 2017 17:02
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 04:47:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

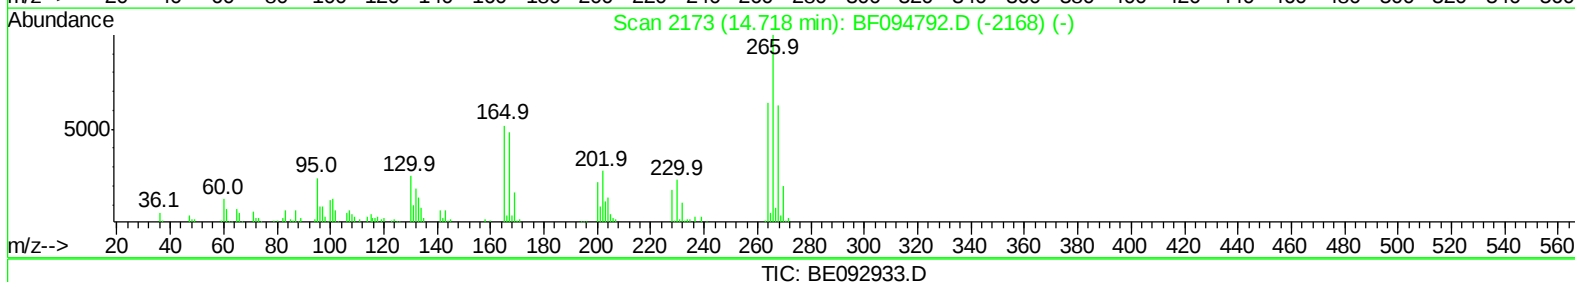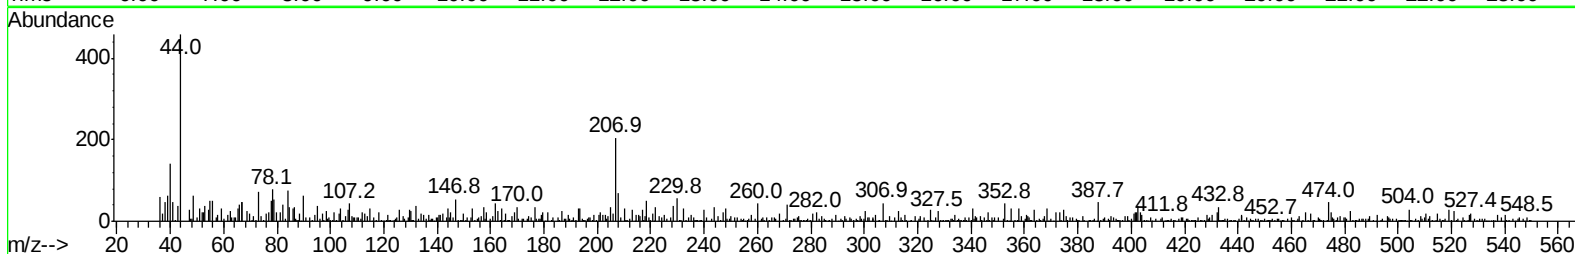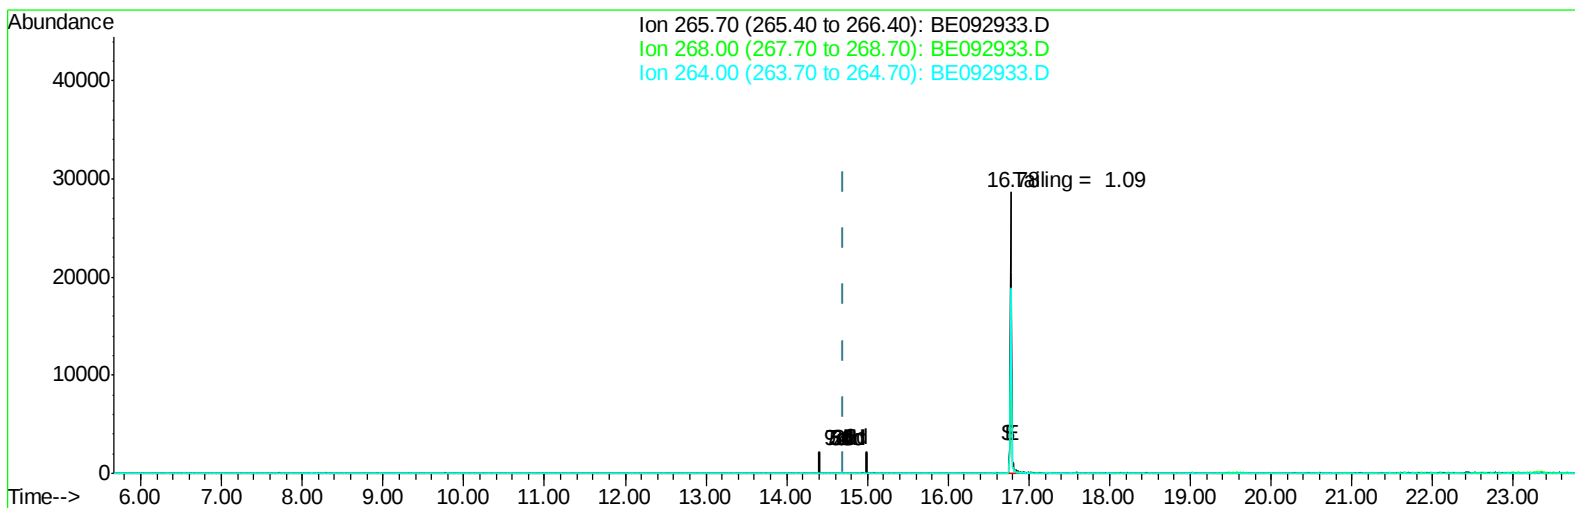

TIC: BE092933.D

(69) Pentachlorophenol (C)

14.762min (+0.043) 279.29ng

response 13

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	90.00#
264.00	64.60	15.00#
0.00	0.00	0.00