

Data Path : S:\HPCHEM1\BNA_E\DATA\BE050517\
 Data File : BE092938.D
 Acq On : 5 May 2017 20:25
 Operator : SJ/MA
 Sample : I2893-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 3060-PP1

Quant Time: May 06 02:14:10 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE050517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 05 14:05:07 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	760	0.40	ng	0.00
7) Naphthalene-d8	10.53	136	3181	0.40	ng	0.00
13) Acenaphthene-d10	14.39	164	1482	0.40	ng	0.00
19) Phenanthrene-d10	17.13	188	4075	0.40	ng	0.00
26) Chrysene-d12	21.28	240	4218	0.40	ng	0.00
33) Perylene-d12	23.69	264	3519	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.35	112	314	0.19	ng	0.00
5) Phenol-d6	6.94	99	282	0.12	ng	0.00
8) Nitrobenzene-d5	8.90	82	737	0.34	ng	0.00
11) 2-Methylnaphthalene-d10	12.13	152	1749	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.86	330	102	0.44	ng	0.00
15) 2-Fluorobiphenyl	13.01	172	3302	0.48	ng	0.00
24) Fluoranthene-d10	19.13	212	4074	0.43	ng	-0.02
28) Terphenyl-d14	19.74	244	5230	0.71	ng	0.00
Target Compounds						Qvalue
31) Bis(2-ethylhexyl)phthalate	21.20	149	3218	1.19	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : S:\HPCHEM1\BNA_E\DATA\BE050517\
Data File : BE092938.D
Acq On : 5 May 2017 20:25
Operator : SJ/MA
Sample : I2893-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
3060-PP1

Quant Time: May 06 02:14:10 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE050517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 14:05:07 2017
Response via : Initial Calibration

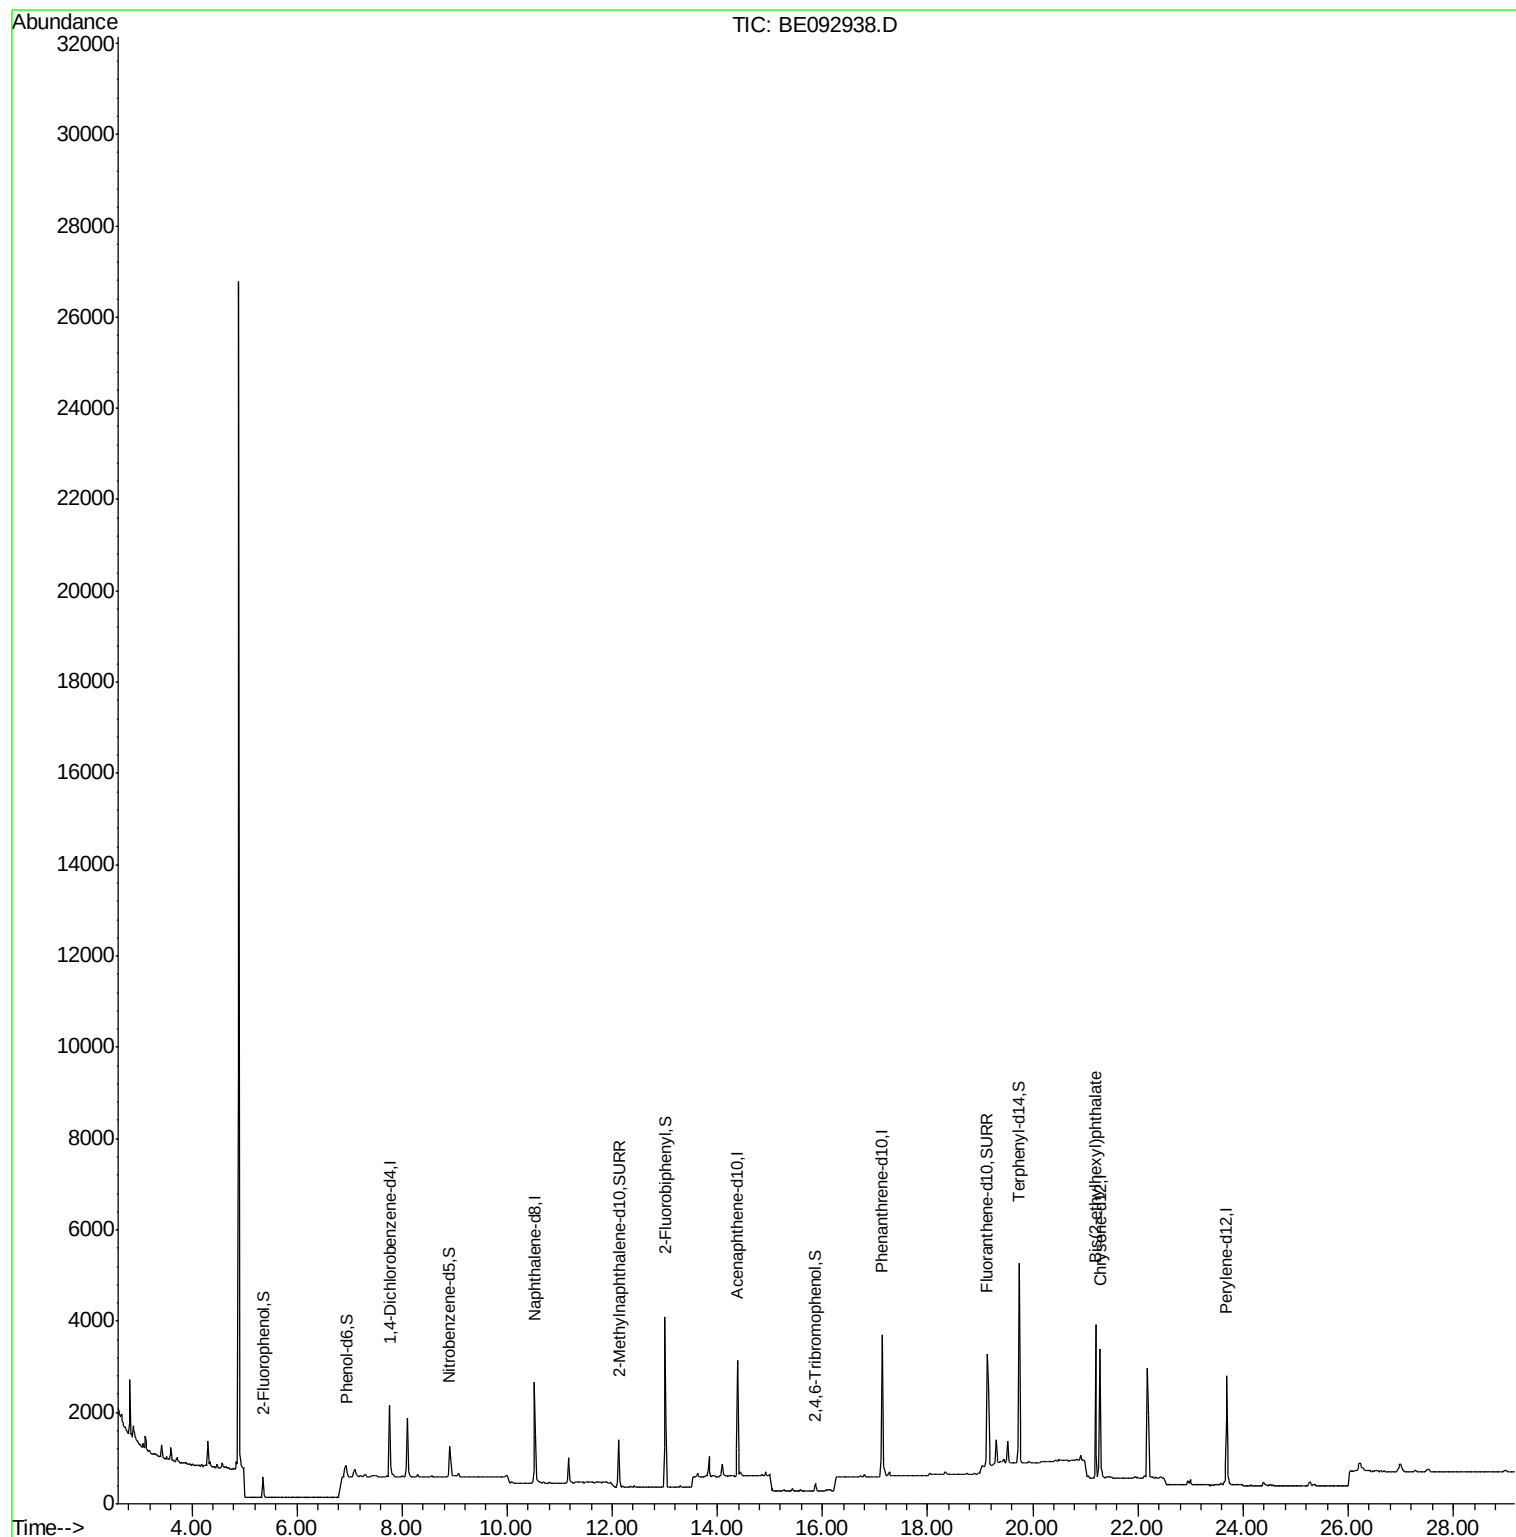




#1




1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.77 min Scan# 555
Delta R.T. -0.00 min
Lab File: BE092938.D
Acq: 5 May 2017 20:25

Instrument :
BNA_E
ClientSampleId :
3060-PP1

Tgt Ion:152 Resp: 760
Ion Ratio Lower Upper
152 100
150 163.7 129.9 194.9
115 76.6 62.6 93.8

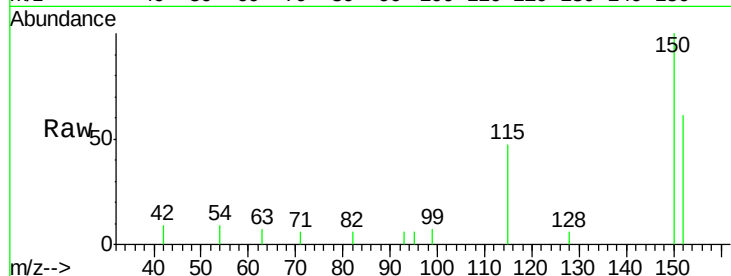


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

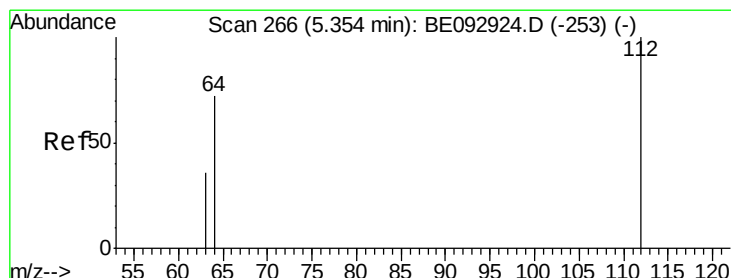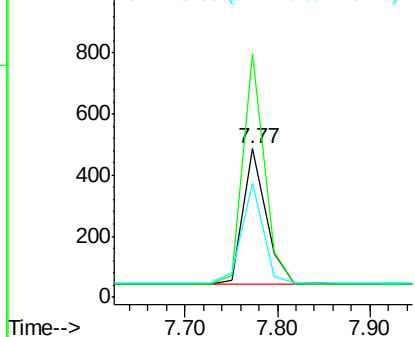



#4


2-Fluorophenol
Concen: 0.19 ng
RT: 5.35 min Scan# 266
Delta R.T. -0.00 min
Lab File: BE092938.D
Acq: 5 May 2017 20:25

Tgt Ion:112 Resp: 314
Ion Ratio Lower Upper
112 100
64 71.3 52.6 79.0
63 36.6 29.0 43.4

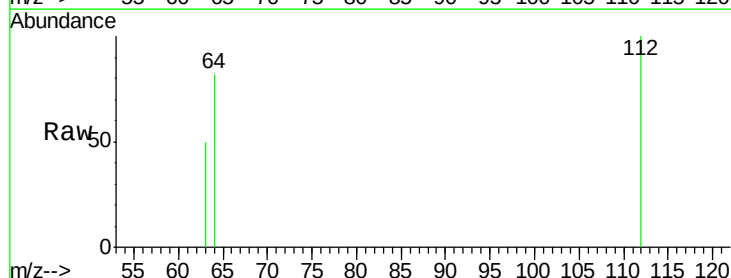

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

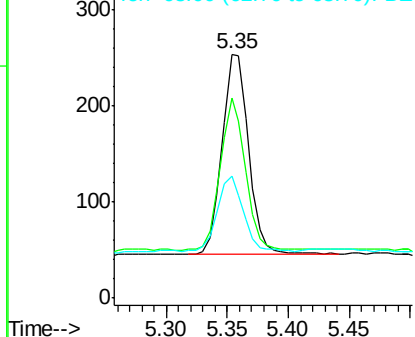

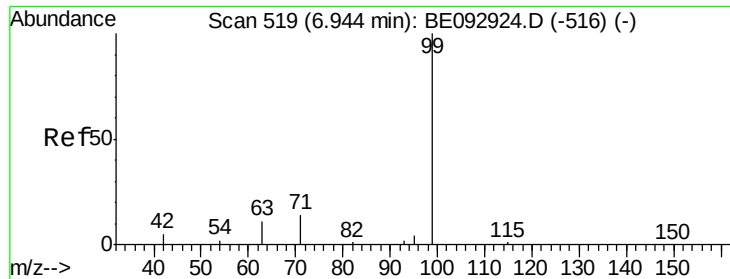

#5

Phenol-d6

Concen: 0.12 ng

RT: 6.94 min Scan# 519

Delta R.T. -0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25

Instrument :

BNA_E

ClientSampleId :

3060-PP1


Tgt Ion: 99 Resp: 282

Ion Ratio Lower Upper

99 100

42 0.0 0.0 0.0




71 0.0 0.0 0.0

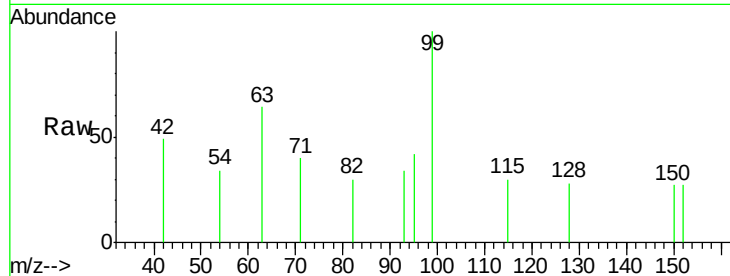

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

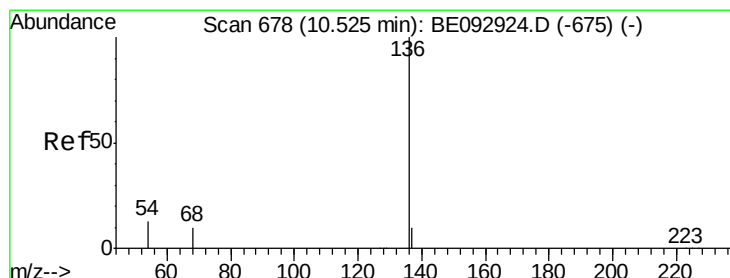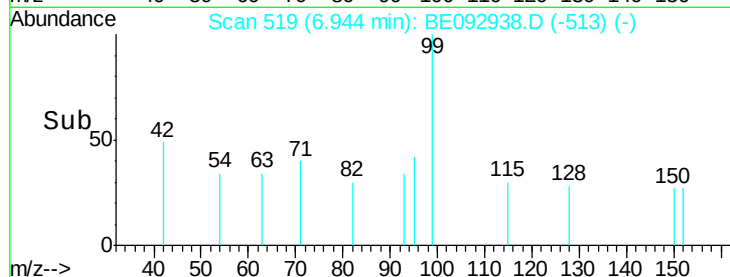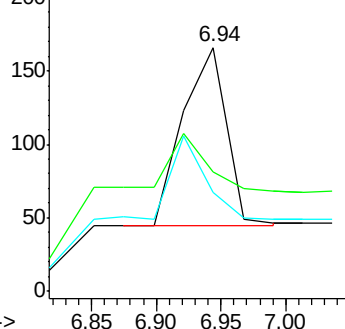

#7

Naphthalene-d8

Concen: 0.40 ng

RT: 10.53 min Scan# 678

Delta R.T. 0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25

Tgt Ion: 136 Resp: 3181


Ion Ratio Lower Upper

136 100

137 12.3 10.4 15.6

54 13.2 12.6 18.8

68 11.7 10.7 16.1


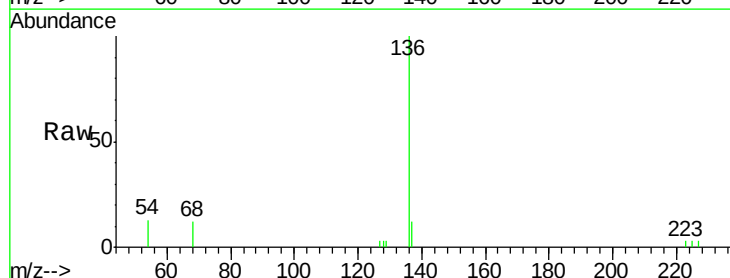



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

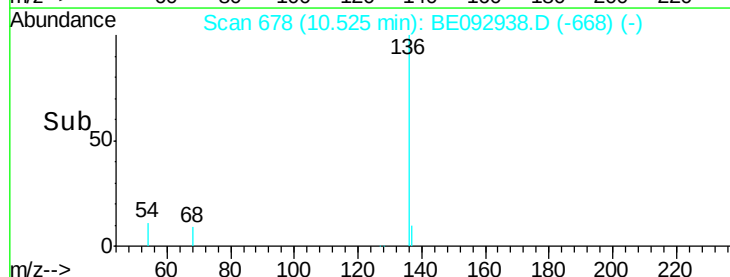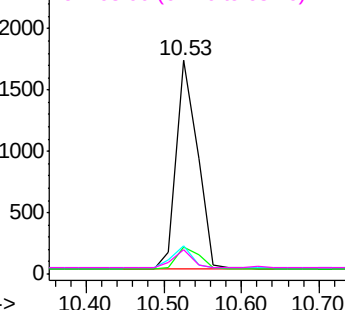

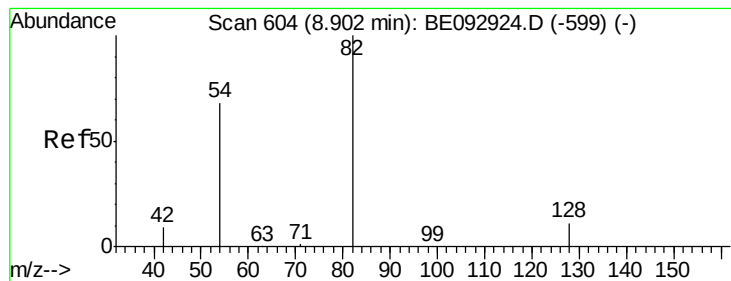

#8

Nitrobenzene-d5

Concen: 0.34 ng

RT: 8.90 min Scan# 604

Delta R.T. -0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25

Instrument :

BNA_E

ClientSampleId :

3060-PP1


Tgt Ion: 82 Resp: 737

Ion Ratio Lower Upper

82 100

128 21.7 35.3 52.9#




54 72.3 65.1 97.7

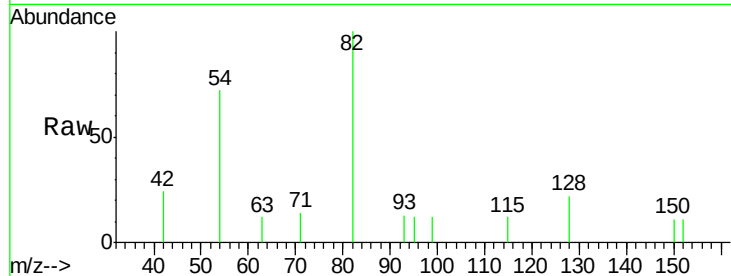

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

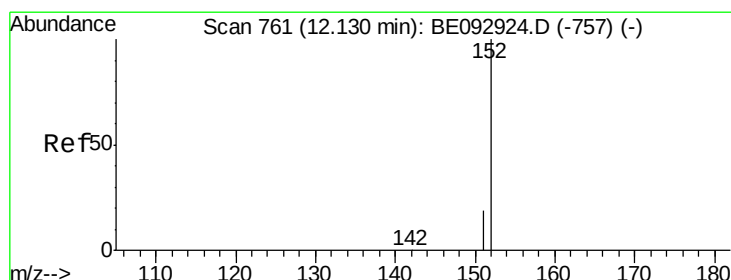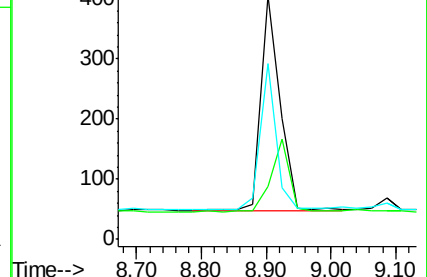

#11

2-Methylnaphthalene-d10

Concen: 0.37 ng

RT: 12.13 min Scan# 761

Delta R.T. 0.00 min

Lab File: BE092938.D


Acq: 5 May 2017 20:25

Tgt Ion: 152 Resp: 1749

Ion Ratio Lower Upper



152 100


151 19.4 15.7 23.5

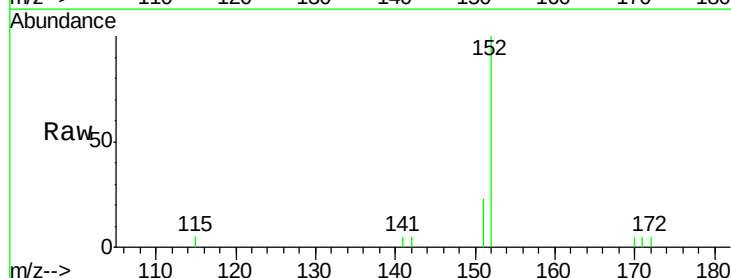

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

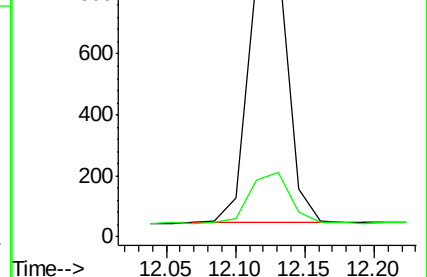

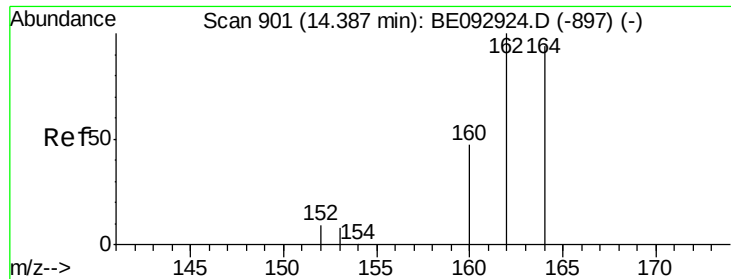

#13

Acenaphthene-d10

Concen: 0.40 ng

RT: 14.39 min Scan# 901

Delta R.T. -0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25

Instrument :

BNA_E

ClientSampleId :

3060-PP1


Tgt Ion:164 Resp: 1482

Ion Ratio Lower Upper

164 100

162 102.3 86.6 130.0




160 48.8 44.5 66.7

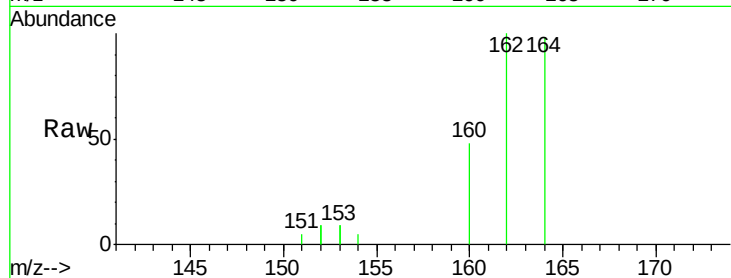

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

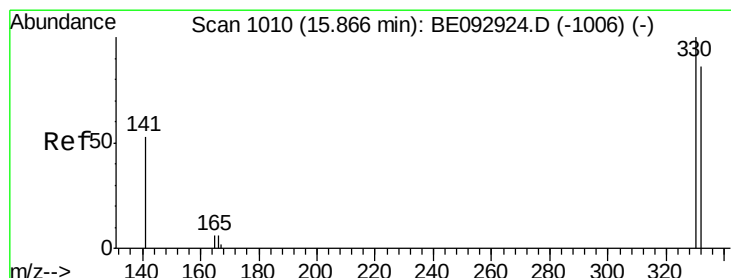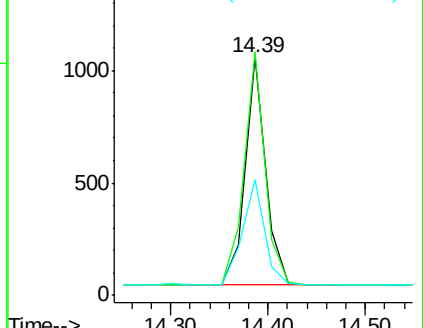

#14

2,4,6-Tribromophenol

Concen: 0.44 ng

RT: 15.86 min Scan# 1010

Delta R.T. -0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25


Tgt Ion:330 Resp: 102

Ion Ratio Lower Upper

330 100

332 96.1 69.1 103.7



141 84.3 54.6 81.8#

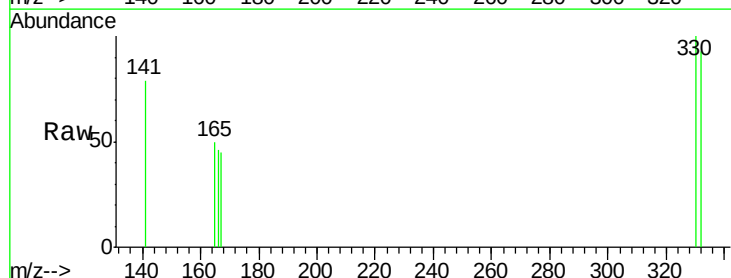


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

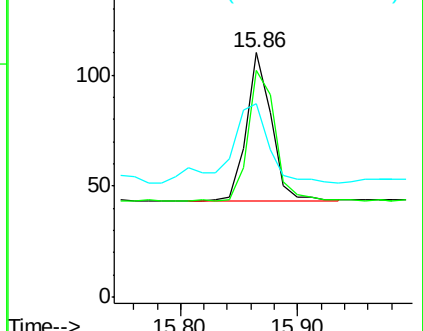

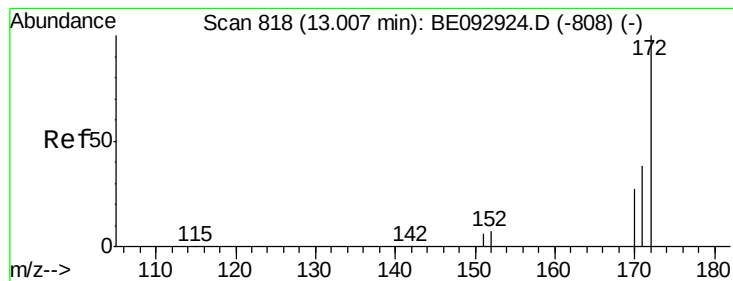

#15

2-Fluorobiphenyl

Concen: 0.48 ng

RT: 13.01 min Scan# 818

Delta R.T. 0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25

Instrument :

BNA_E

ClientSampleId :

3060-PP1


Tgt Ion:172 Resp: 3302

Ion Ratio Lower Upper

172 100

171 36.9 35.8 53.6




170 25.3 28.5 42.7#

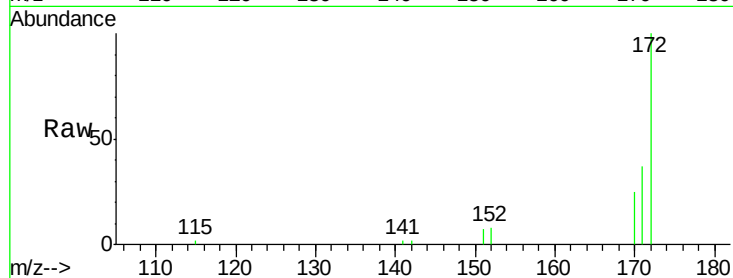

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

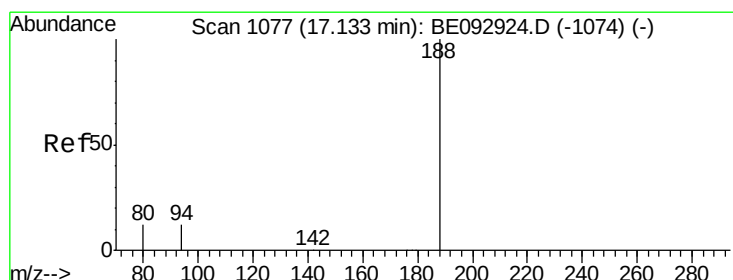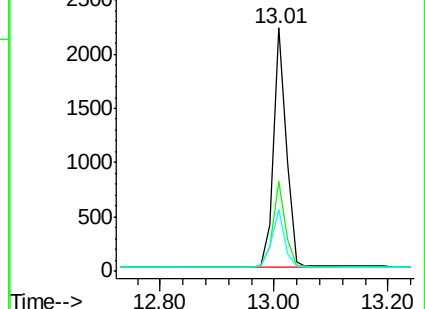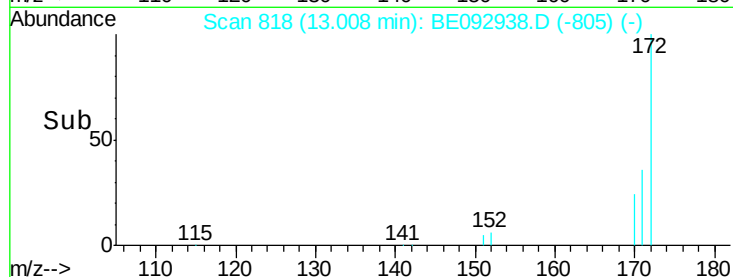

#19

Phenanthrene-d10

Concen: 0.40 ng

RT: 17.13 min Scan# 1078

Delta R.T. 0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25


Tgt Ion:188 Resp: 4075

Ion Ratio Lower Upper

188 100

94 9.8 10.2 15.4#



80 9.5 10.6 15.8#

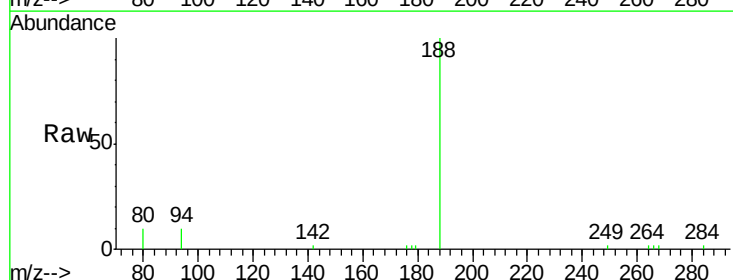


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

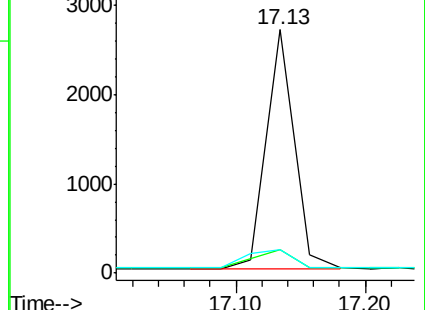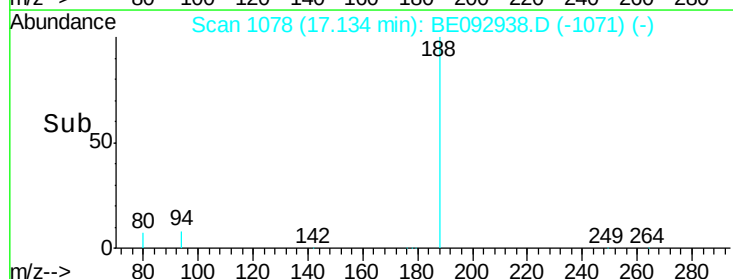



#24

Fluoranthene-d10

Concen: 0.43 ng

RT: 19.13 min Scan# 1164

Delta R.T. -0.02 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25

Instrument :

BNA_E

ClientSampled :

3060-PP1


Tgt Ion:212 Resp: 4074

Ion Ratio Lower Upper

212 100

106 18.9 0.0 0.0#




104 10.1 0.0 0.0#

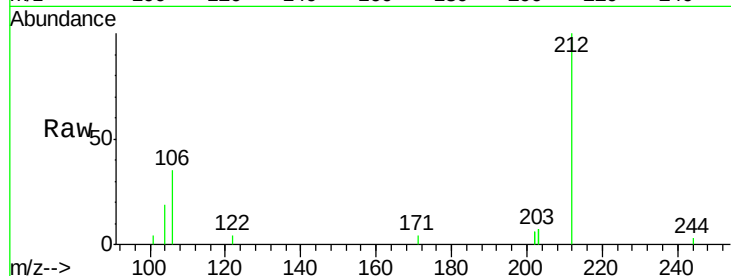

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

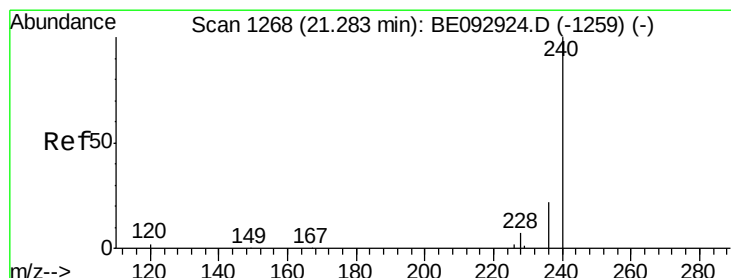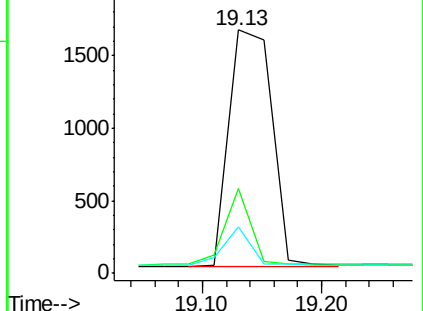

#26

Chrysene-d12

Concen: 0.40 ng

RT: 21.28 min Scan# 1268

Delta R.T. 0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25


Tgt Ion:240 Resp: 4218

Ion Ratio Lower Upper

240 100

120 4.3 4.6 6.8#



236 23.4 19.8 29.8

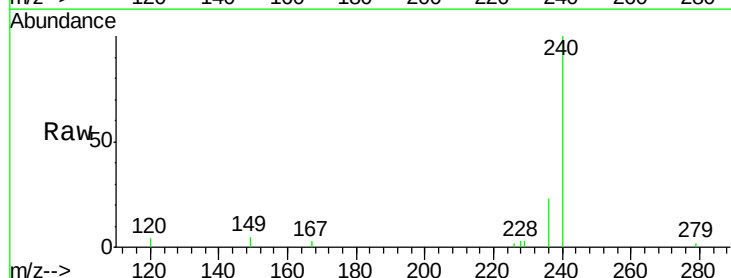


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

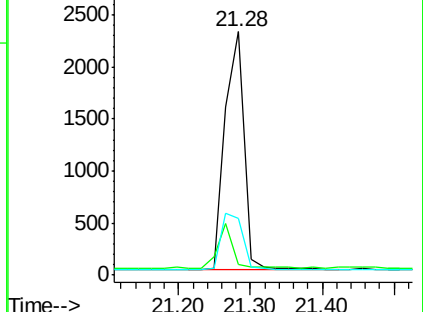

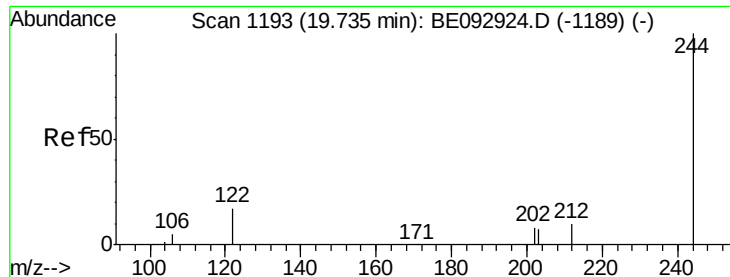

#28

Terphenyl-d14

Concen: 0.71 ng

RT: 19.74 min Scan# 1193

Delta R.T. 0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25

Instrument :

BNA_E

ClientSampleId :

3060-PP1


Tgt Ion:244 Resp: 5230

Ion Ratio Lower Upper

244 100

212 10.7 18.4 27.6#




122 13.3 23.3 34.9#

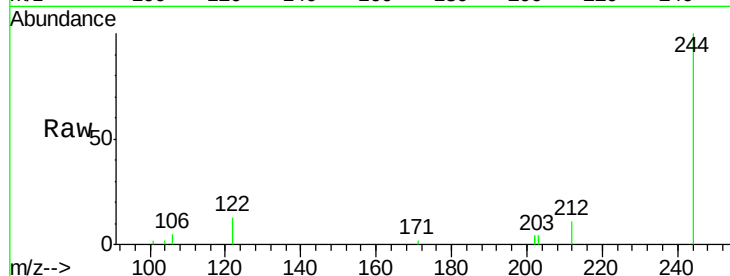

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

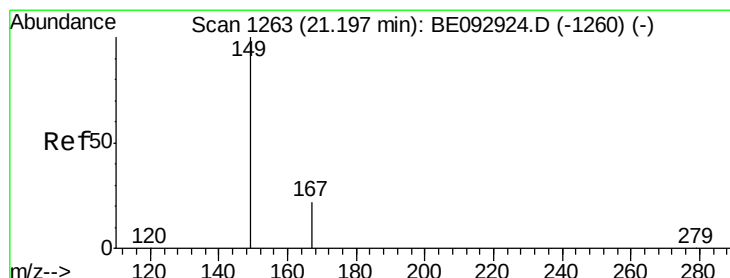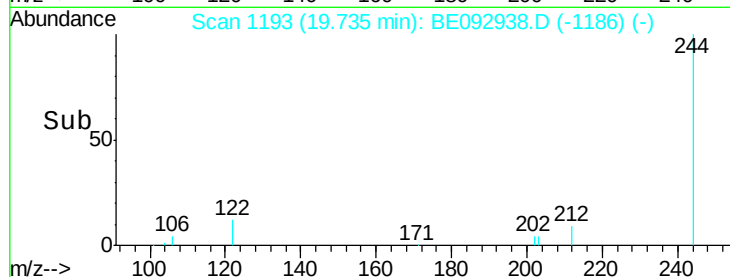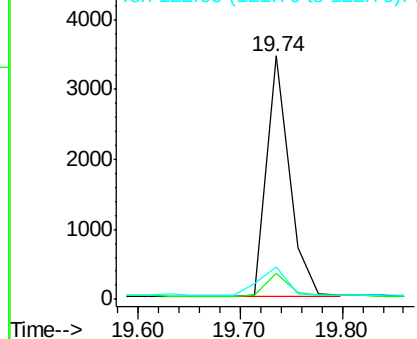

#31

Bis(2-ethylhexyl)phthalate

Concen: 1.19 ng

RT: 21.20 min Scan# 1263

Delta R.T. 0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25


Tgt Ion:149 Resp: 3218

Ion Ratio Lower Upper

149 100

167 25.1 20.9 31.3



279 2.6 0.0 0.0#



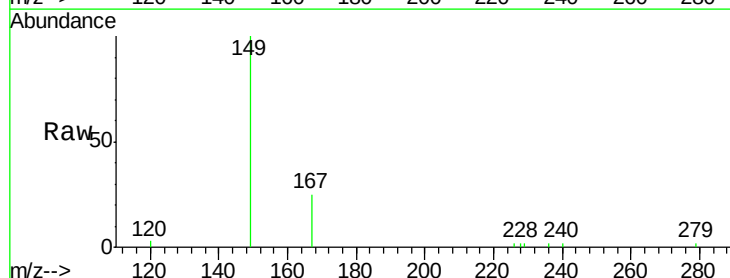


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

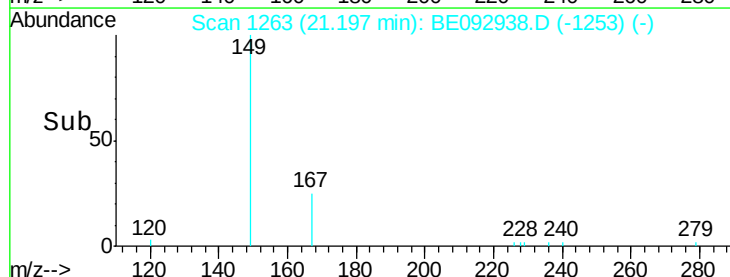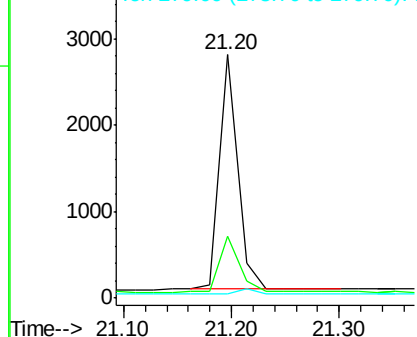

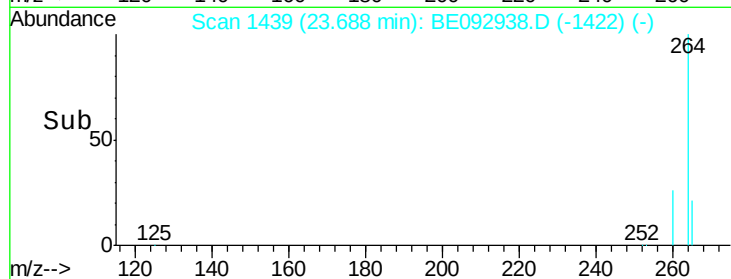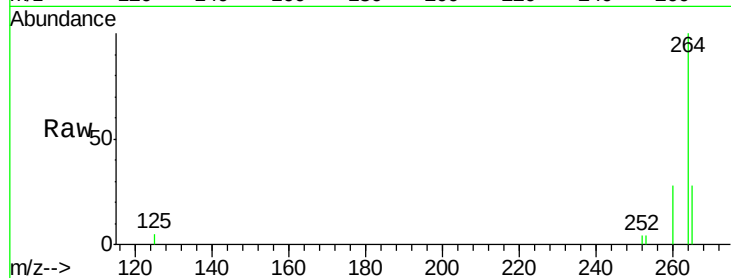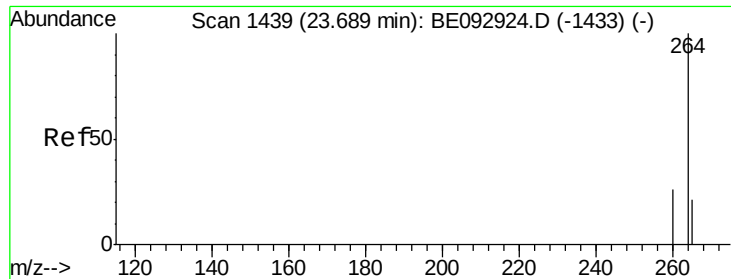

#33

Perylene-d12

Concen: 0.40 ng

RT: 23.69 min Scan# 1439

Delta R.T. -0.00 min

Lab File: BE092938.D

Acq: 5 May 2017 20:25

Instrument :

BNA_E

ClientSampleId :

3060-PP1

Tgt Ion: 264 Resp: 3519

Ion Ratio Lower Upper

264 100

260 27.9 23.5 35.3

265 27.6 27.2 40.8

