

Data Path : S:\HPCHEM1\BNA_E\DATA\BE050517\
 Data File : BE092955.D
 Acq On : 6 May 2017 6:58
 Operator : SJ/MA
 Sample : I2893-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 3072-PA3

Quant Time: May 08 04:42:24 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE050517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 05 14:05:07 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	903	0.40	ng	0.00
7) Naphthalene-d8	10.53	136	4024	0.40	ng	0.00
13) Acenaphthene-d10	14.39	164	2184	0.40	ng	0.00
19) Phenanthrene-d10	17.13	188	5179	0.40	ng	0.00
26) Chrysene-d12	21.28	240	6189	0.40	ng	0.00
33) Perylene-d12	23.70	264	5261	0.40	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.36	112	411	0.20	ng	0.00
5) Phenol-d6	6.94	99	347	0.12	ng	0.00
8) Nitrobenzene-d5	8.90	82	1215	0.45	ng	0.00
11) 2-Methylnaphthalene-d10	12.13	152	2213	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.88	330	264	0.77	ng	0.01
15) 2-Fluorobiphenyl	13.01	172	3616	0.36	ng	0.00
24) Fluoranthene-d10	19.15	212	5646	0.47	ng	0.00
28) Terphenyl-d14	19.74	244	3890	0.36	ng	0.00
Target Compounds						Qvalue
31) Bis(2-ethylhexyl)phthalate	21.20	149	2905	0.73	ng	# 49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : S:\HPCHEM1\BNA_E\DATA\BE050517\
Data File : BE092955.D
Acq On : 6 May 2017 6:58
Operator : SJ/MA
Sample : I2893-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
3072-PA3

Quant Time: May 08 04:42:24 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE050517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 05 14:05:07 2017
Response via : Initial Calibration

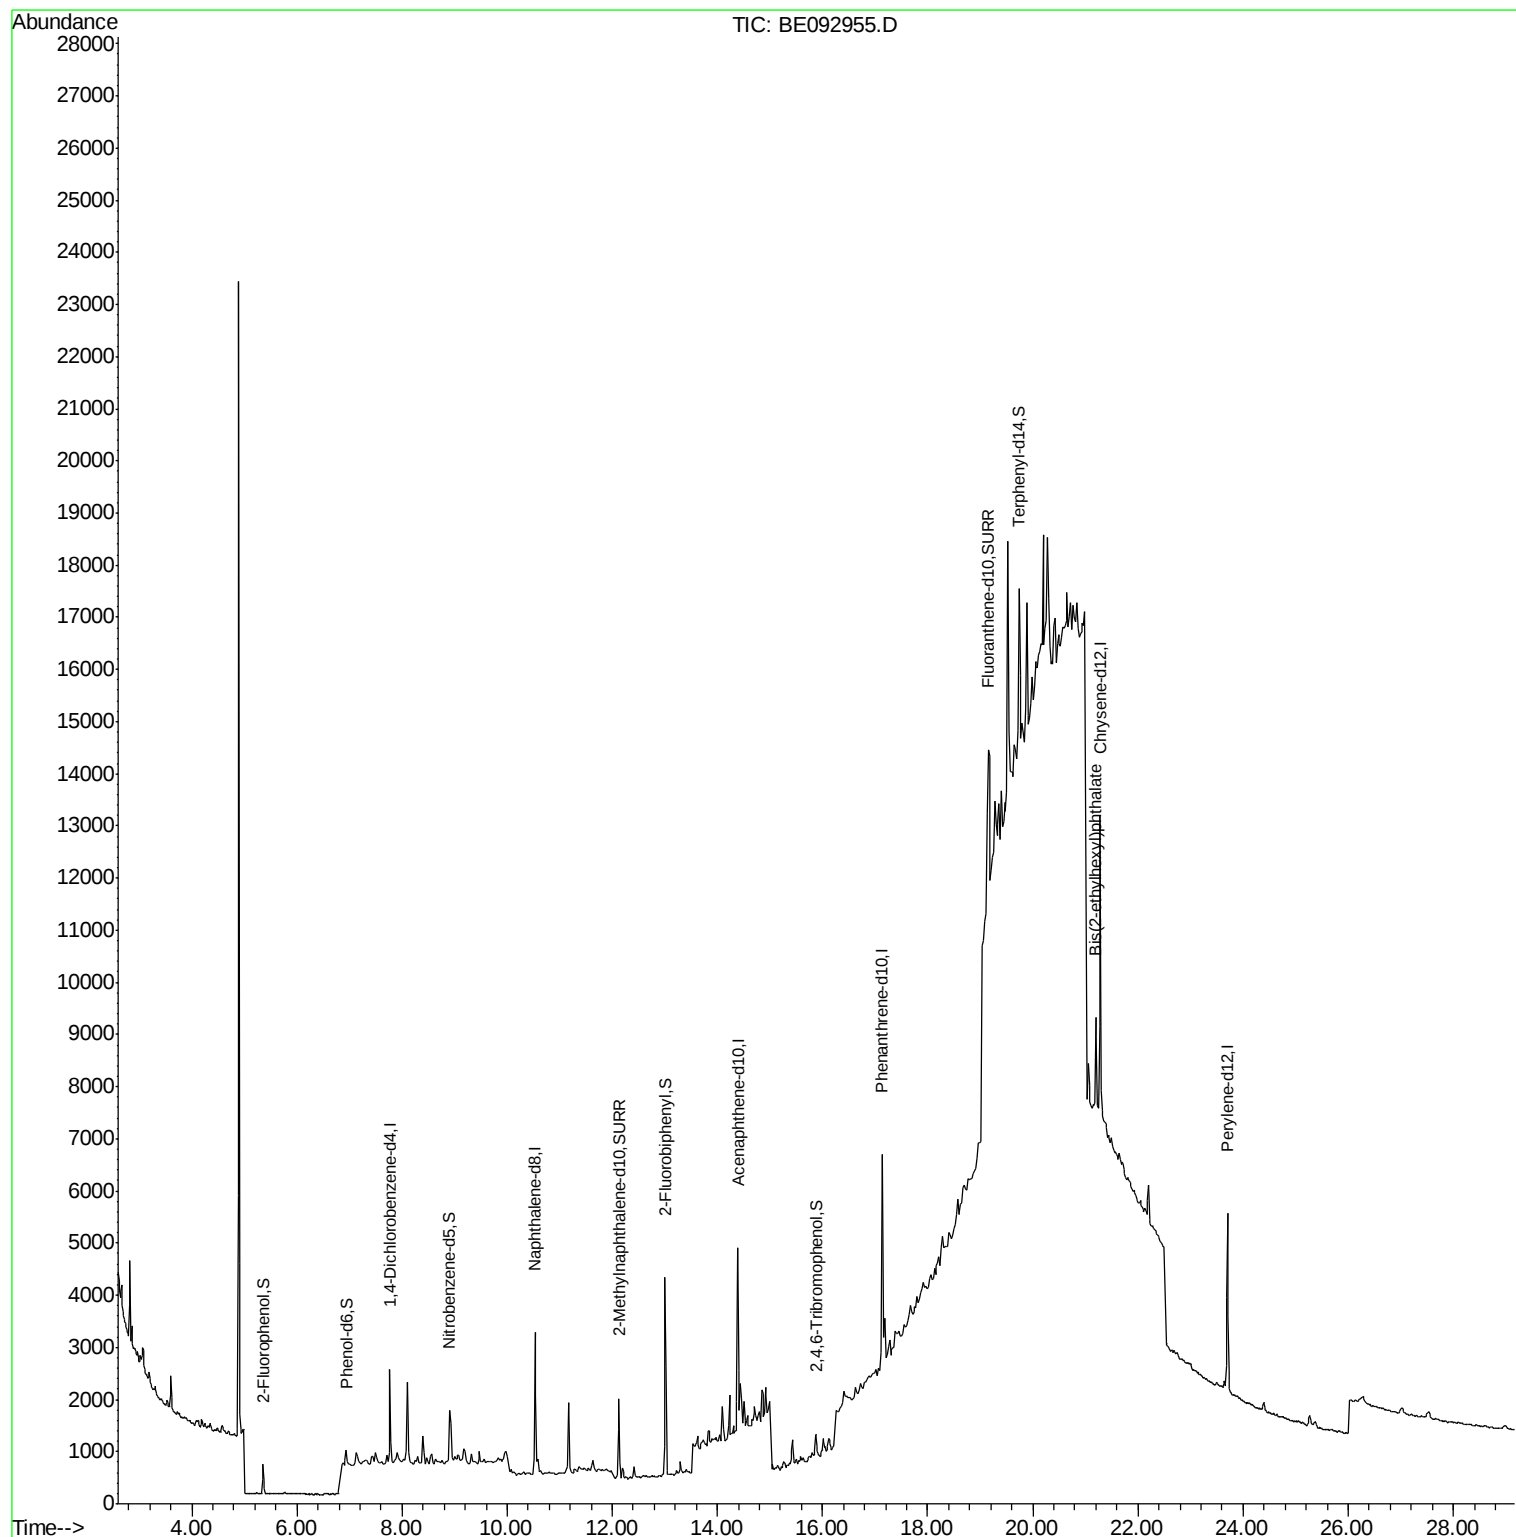

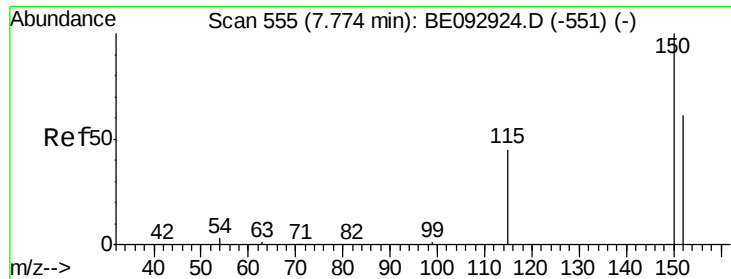

#1

1,4-Dichlorobenzene-d4

Concen: 0.40 ng

RT: 7.77 min Scan# 555

Delta R.T. -0.00 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58

Instrument :

BNA_E

ClientSampleId :

3072-PA3


Tgt Ion:152 Resp: 903

Ion Ratio Lower Upper

152 100

150 164.5 129.9 194.9




115 83.2 62.6 93.8

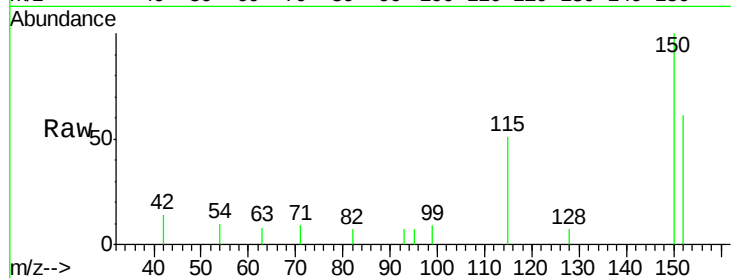

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

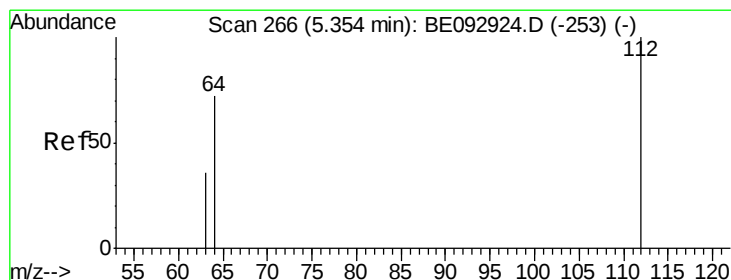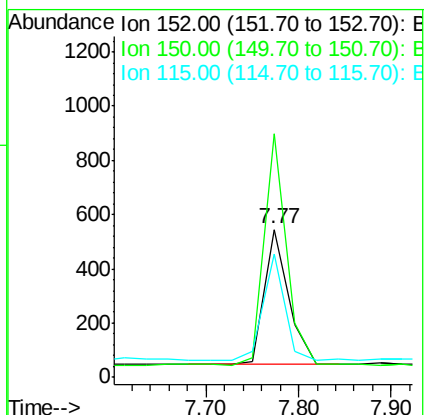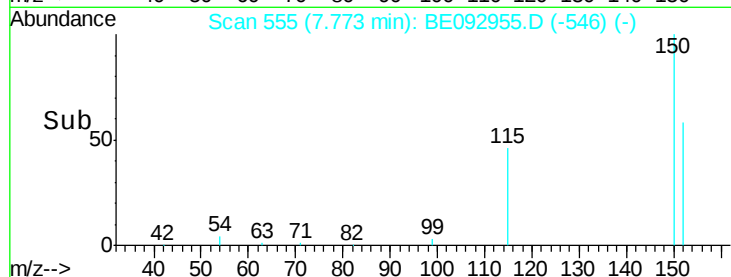

#4

2-Fluorophenol

Concen: 0.20 ng

RT: 5.36 min Scan# 267

Delta R.T. 0.01 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58


Tgt Ion:112 Resp: 411

Ion Ratio Lower Upper

112 100

64 68.4 52.6 79.0



63 34.8 29.0 43.4

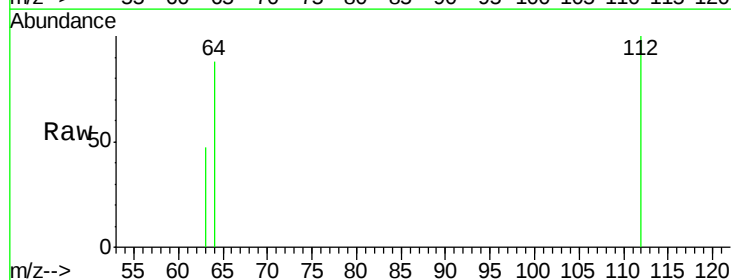


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

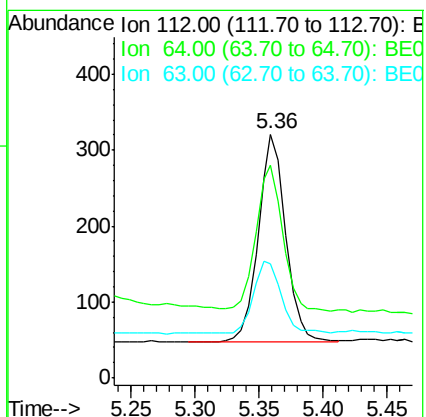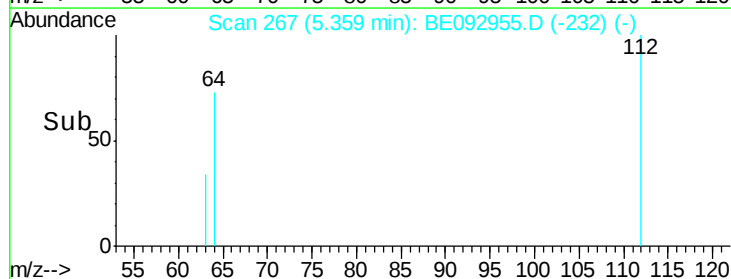

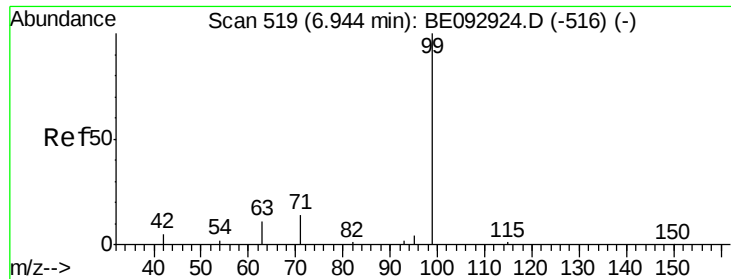

#5

Phenol-d6

Concen: 0.12 ng

RT: 6.94 min Scan# 519

Delta R.T. -0.00 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58

Instrument :

BNA_E

ClientSampleId :

3072-PA3


Tgt Ion: 99 Resp: 347

Ion Ratio Lower Upper

99 100

42 0.0 0.0 0.0




71 23.1 0.0 0.0#

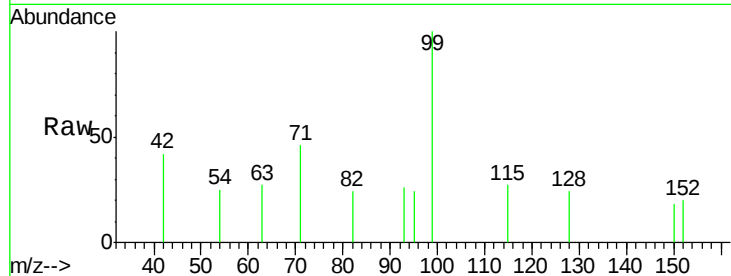

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

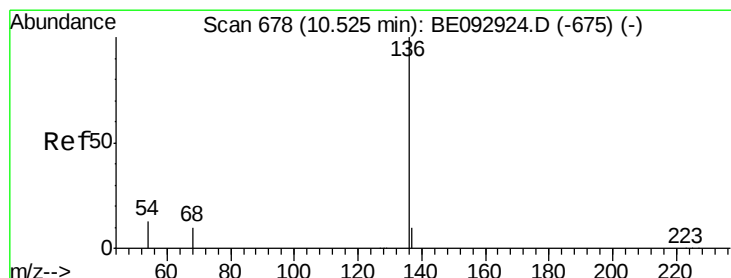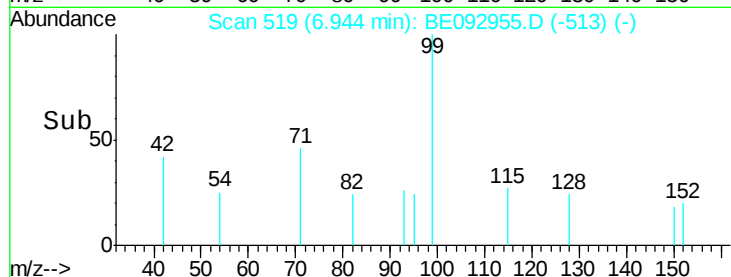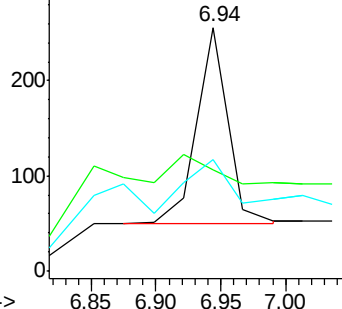

#7

Naphthalene-d8

Concen: 0.40 ng

RT: 10.53 min Scan# 678

Delta R.T. 0.00 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58

Tgt Ion: 136 Resp: 4024


Ion Ratio Lower Upper

136 100

137 12.3 10.4 15.6

54 15.5 12.6 18.8

68 13.7 10.7 16.1


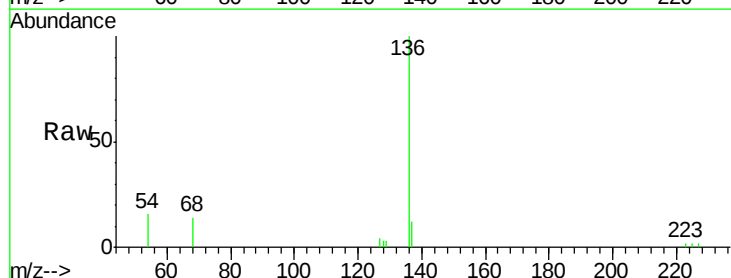



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

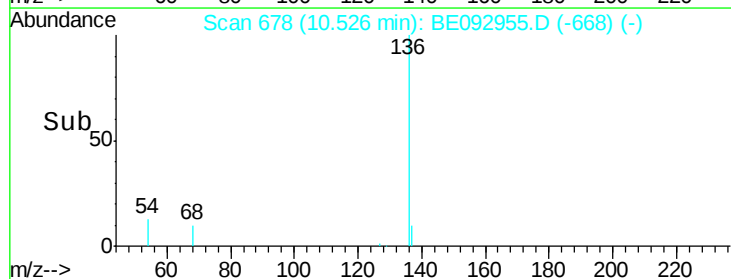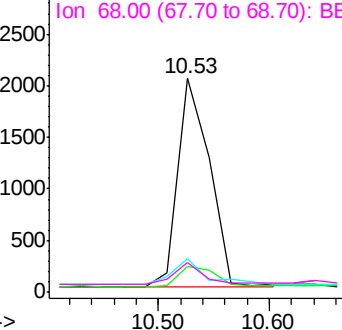

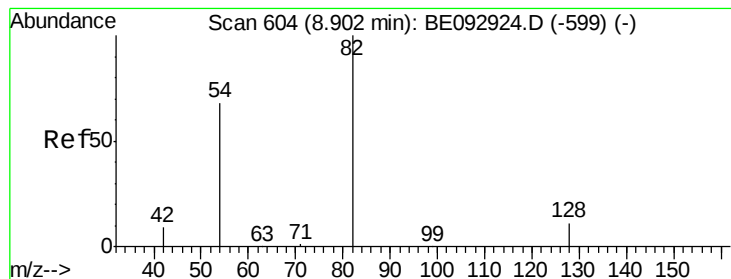

#8

Nitrobenzene-d5

Concen: 0.45 ng

RT: 8.90 min Scan# 604

Delta R.T. -0.00 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58


Instrument :

BNA_E

ClientSampleId :

3072-PA3




Tgt Ion:	82	Resp:	1215
Ion	Ratio	Lower	Upper
82	100		
128	19.1	35.3	52.9#
54	73.6	65.1	97.7

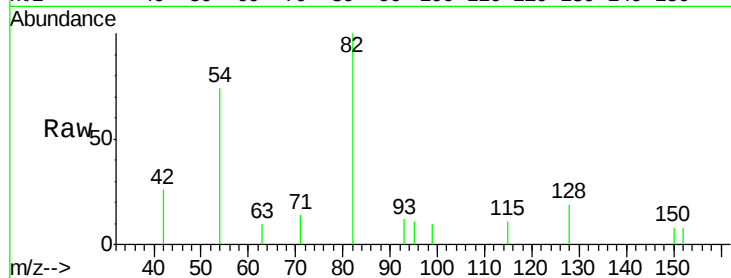

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

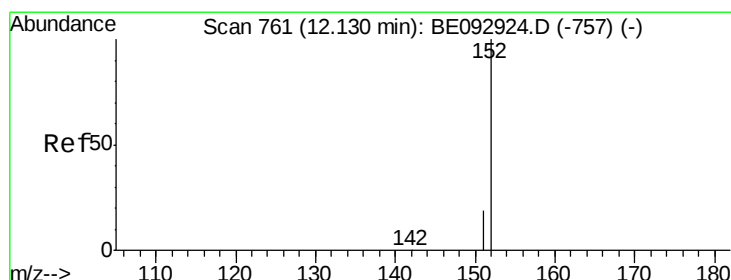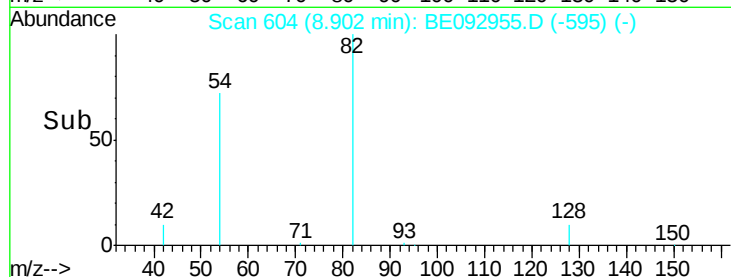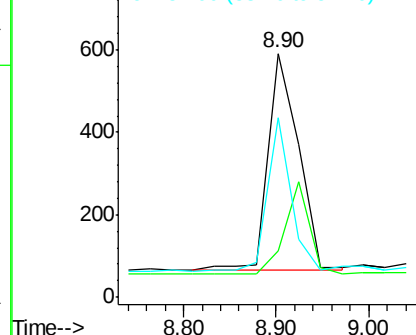

#11

2-Methylnaphthalene-d10

Concen: 0.37 ng


RT: 12.13 min Scan# 761

Delta R.T. -0.00 min

Lab File: BE092955.D



Acq: 6 May 2017 6:58


Tgt Ion:	152	Resp:	2213
Ion	Ratio	Lower	Upper
152	100		
151	20.4	15.7	23.5

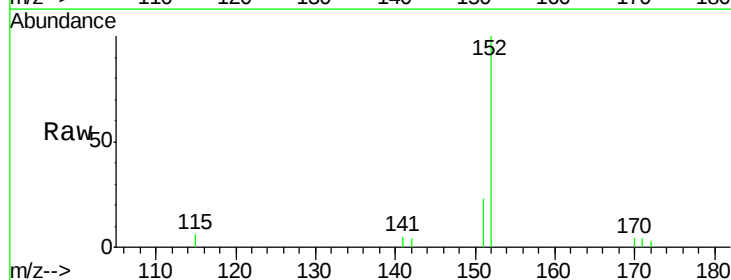

Abundance Ion 152.00 (151.70 to 152.70): BE0

Ion 151.00 (150.70 to 151.70): BE0

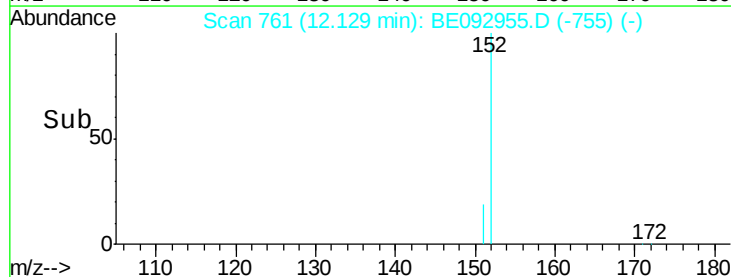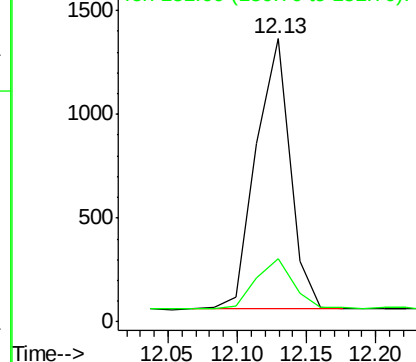

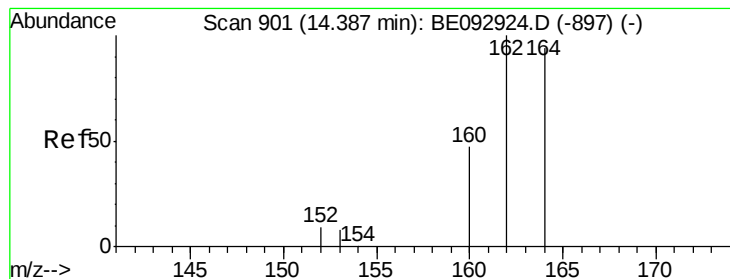

#13

Acenaphthene-d10

Concen: 0.40 ng

RT: 14.39 min Scan# 901

Delta R.T. -0.00 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58

Instrument :

BNA_E

ClientSampleId :

3072-PA3


Tgt Ion:164 Resp: 2184

Ion Ratio Lower Upper

164 100

162 105.2 86.6 130.0




160 53.1 44.5 66.7

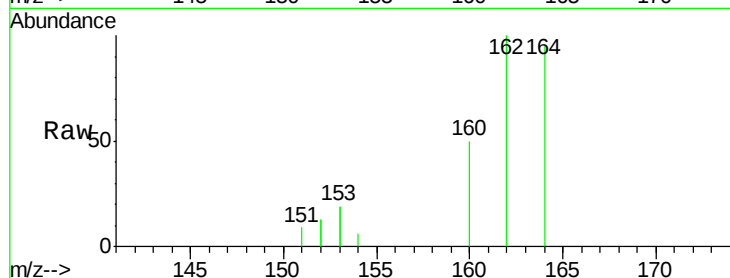

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

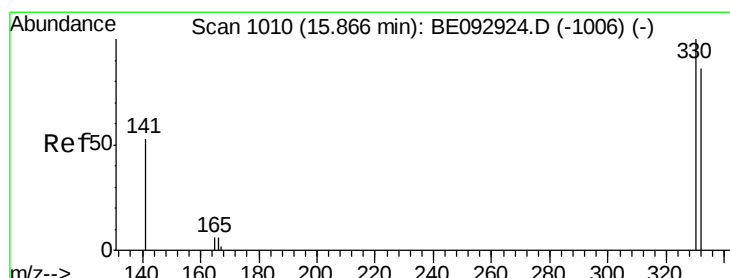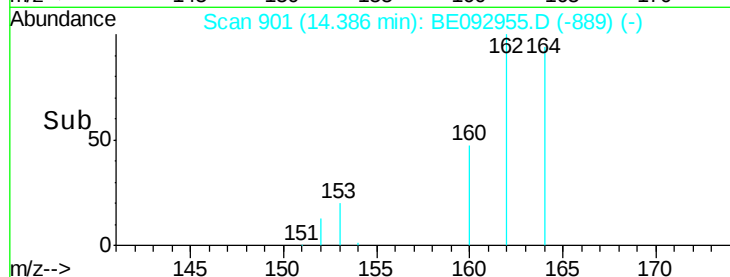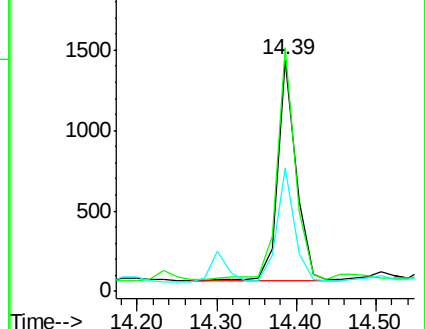

#14

2,4,6-Tribromophenol

Concen: 0.77 ng

RT: 15.88 min Scan# 1011

Delta R.T. 0.01 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58


Tgt Ion:330 Resp: 264

Ion Ratio Lower Upper

330 100

332 99.6 69.1 103.7



141 100.4 54.6 81.8#

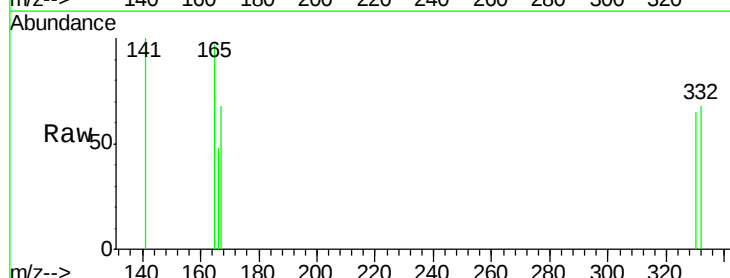


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

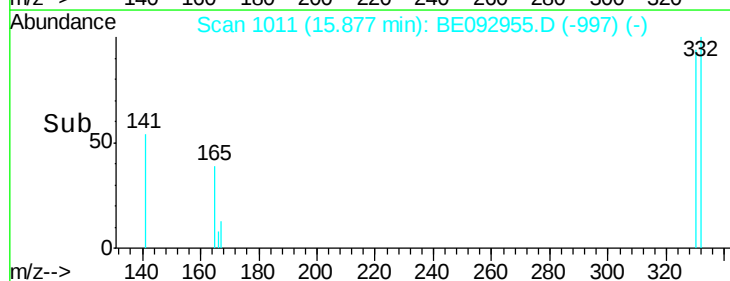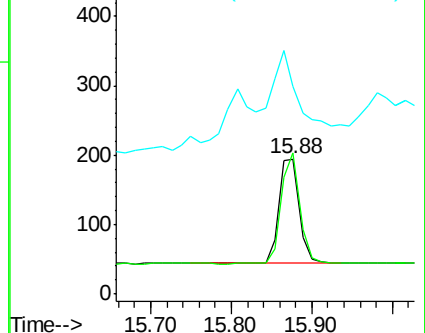

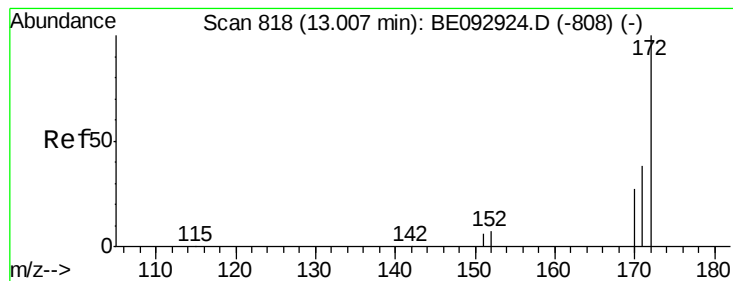

#15

2-Fluorobiphenyl

Concen: 0.36 ng

RT: 13.01 min Scan# 818

Delta R.T. -0.00 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58

Instrument :

BNA_E

ClientSampleId :

3072-PA3


Tgt Ion:172 Resp: 3616

Ion Ratio Lower Upper

172 100

171 39.4 35.8 53.6




170 29.1 28.5 42.7

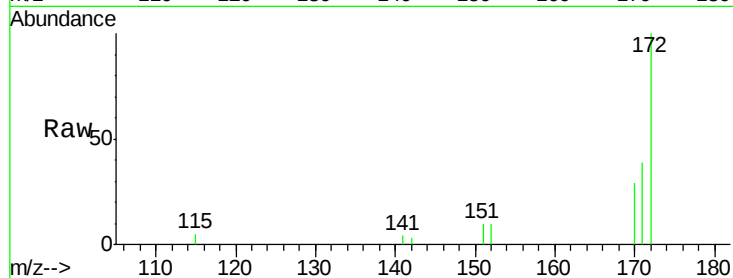

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

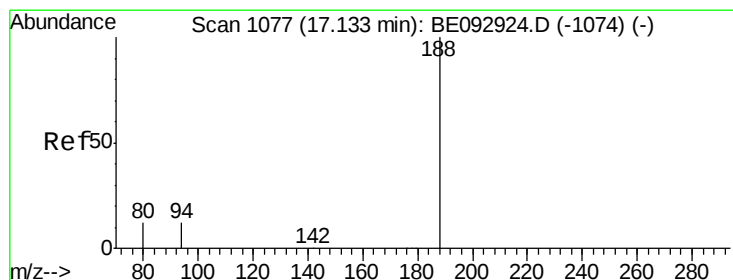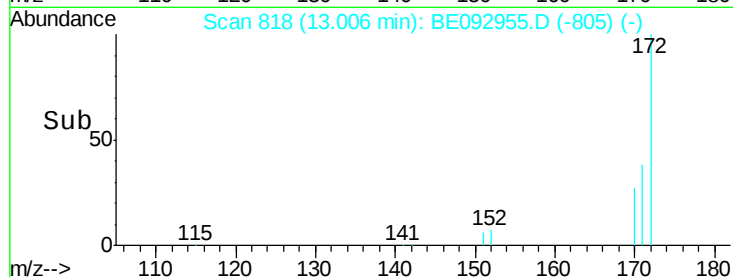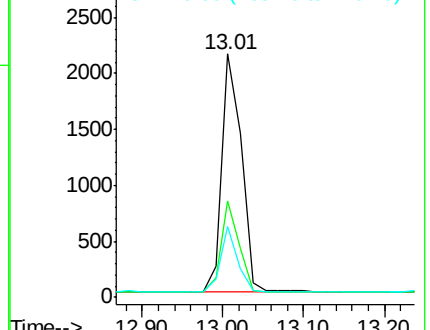

#19

Phenanthrene-d10

Concen: 0.40 ng

RT: 17.13 min Scan# 1078

Delta R.T. 0.00 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58


Tgt Ion:188 Resp: 5179

Ion Ratio Lower Upper

188 100

94 25.6 10.2 15.4#



80 23.9 10.6 15.8#

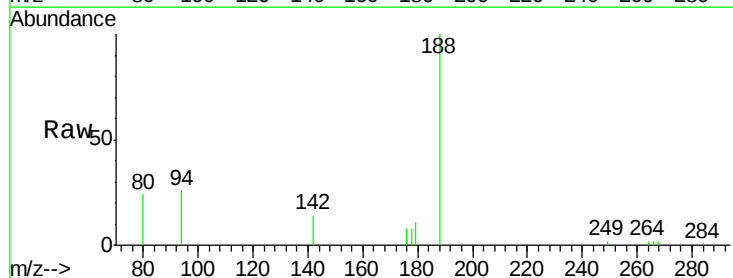


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

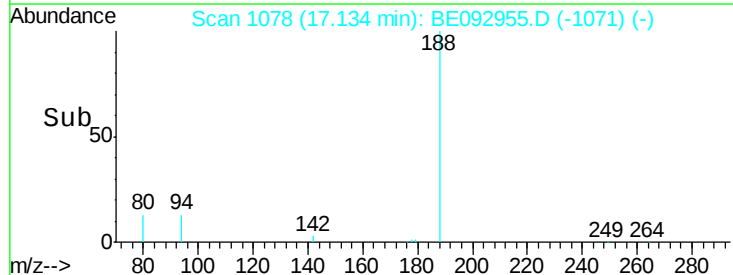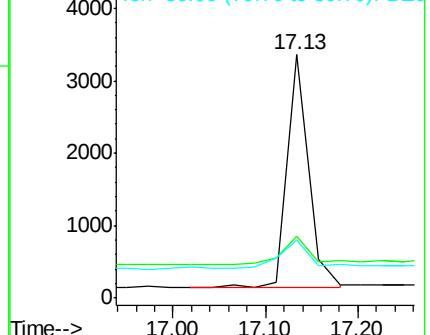


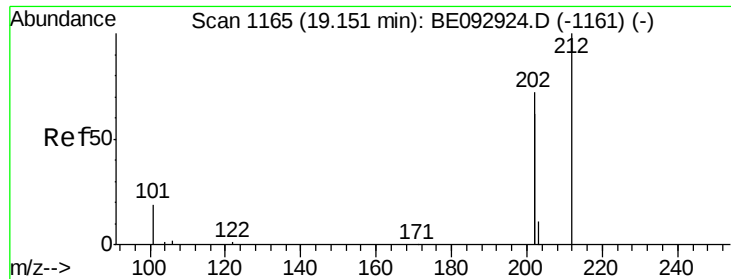




#24
 Fluoranthene-d10
 Concen: 0.47 ng
 RT: 19.15 min Scan# 1165
 Delta R.T. 0.00 min
 Lab File: BE092955.D
 Acq: 6 May 2017 6:58

Instrument :
 BNA_E
 ClientSampleId :
 3072-PA3

Tgt Ion: 212 Resp: 5646
 Ion Ratio Lower Upper
 212 100
 106 0.0 0.0 0.0
 104 0.0 0.0 0.0

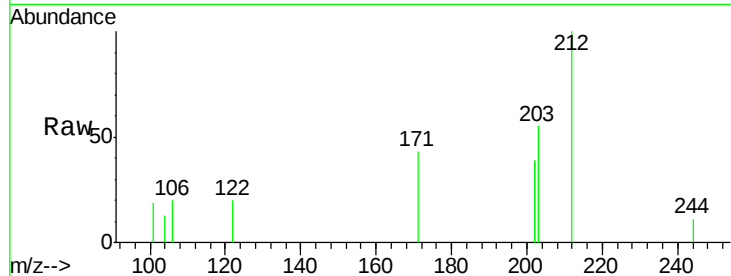


Abundance Ion 212.00 (211.70 to 212.70): E
 Ion 106.00 (105.70 to 106.70): E
 Ion 104.00 (103.70 to 104.70): E

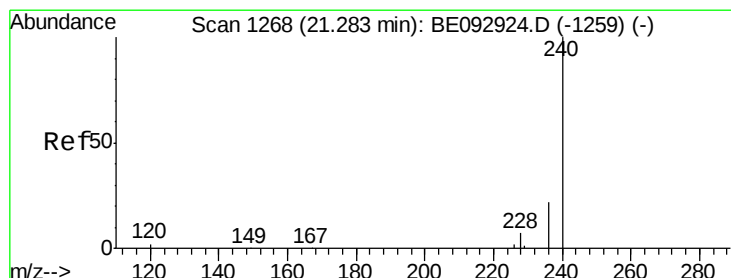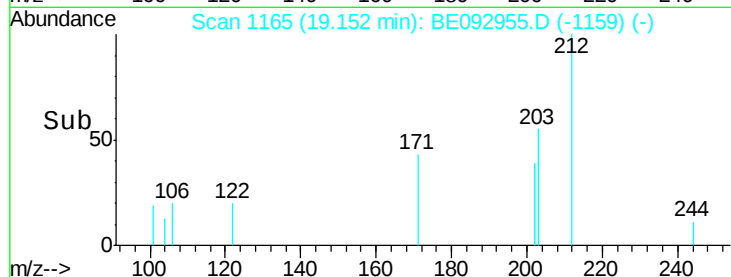
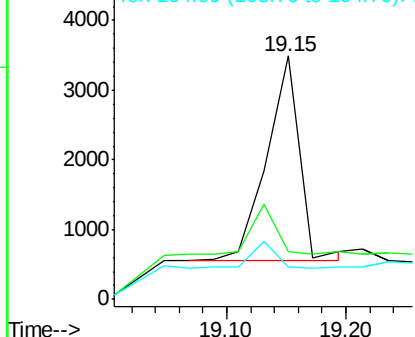



#26
 Chrysene-d12
 Concen: 0.40 ng
 RT: 21.28 min Scan# 1268
 Delta R.T. -0.00 min
 Lab File: BE092955.D
 Acq: 6 May 2017 6:58

Tgt Ion: 240 Resp: 6189
 Ion Ratio Lower Upper
 240 100
 120 16.2 4.6 6.8#
 236 34.4 19.8 29.8#

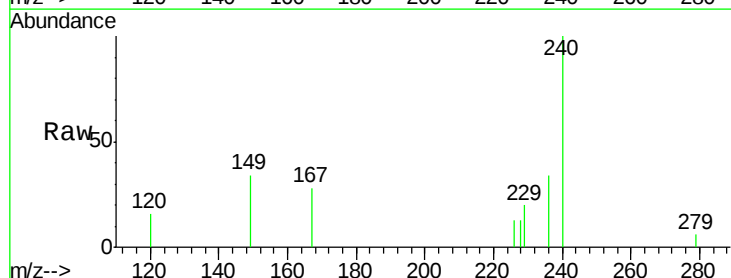

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

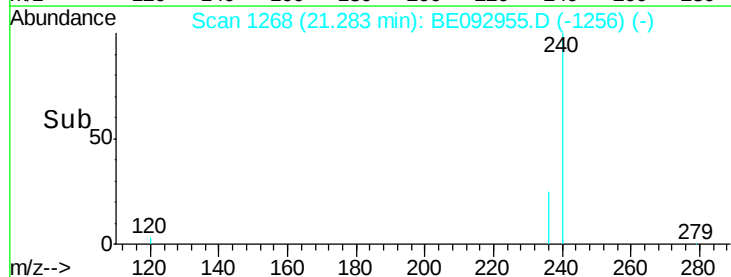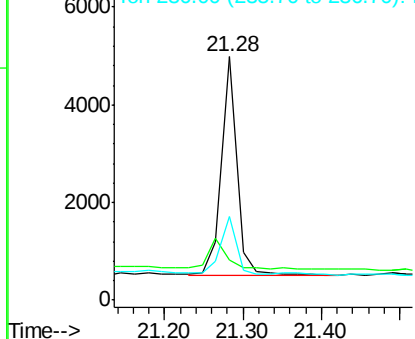

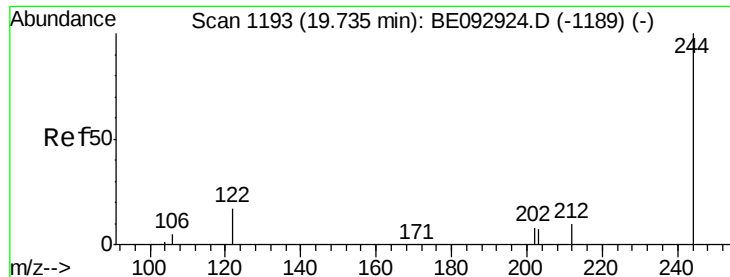

#28

Terphenyl-d14

Concen: 0.36 ng

RT: 19.74 min Scan# 1193

Delta R.T. 0.00 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58

Instrument :

BNA_E

ClientSampleId :

3072-PA3


Tgt Ion:244 Resp: 3890

Ion Ratio Lower Upper

244 100

212 32.6 18.4 27.6#




122 49.4 23.3 34.9#

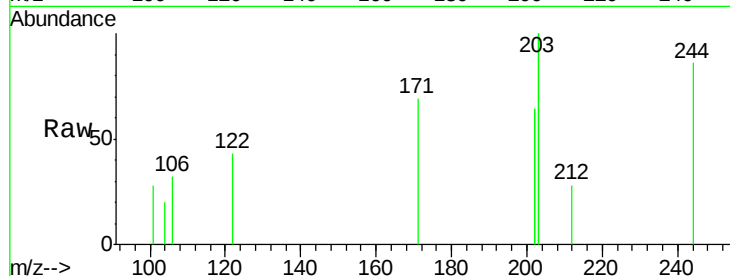

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

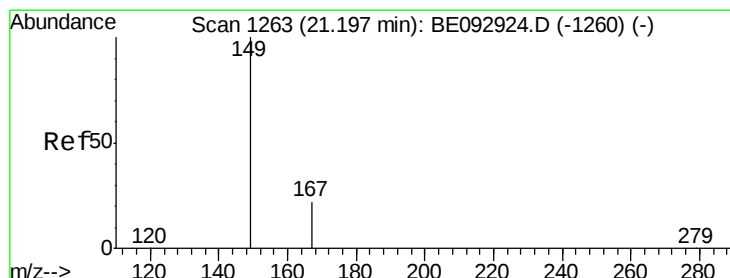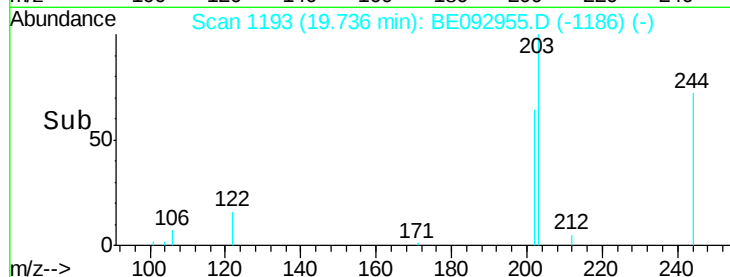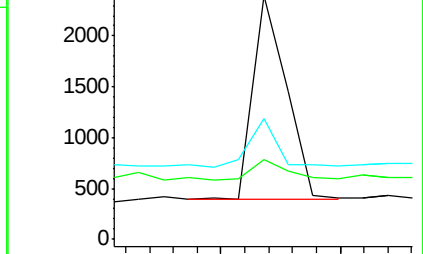

#31

Bis(2-ethylhexyl)phthalate

Concen: 0.73 ng

RT: 21.20 min Scan# 1263

Delta R.T. -0.00 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58


Tgt Ion:149 Resp: 2905

Ion Ratio Lower Upper

149 100

167 0.0 20.9 31.3#



279 0.0 0.0 0.0



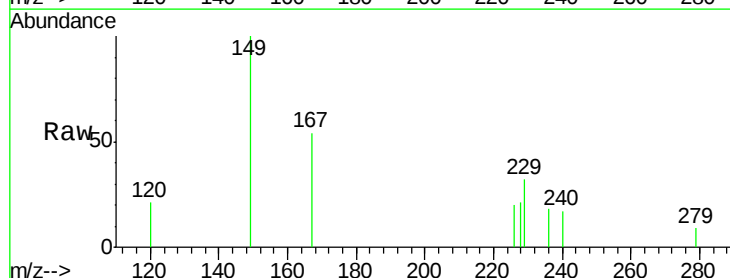


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

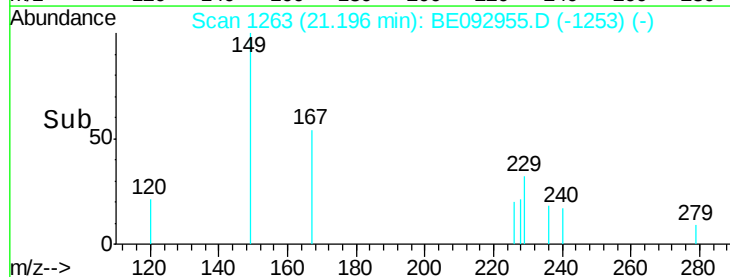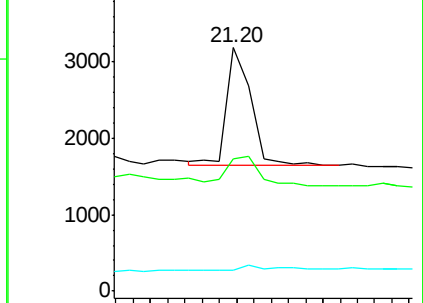

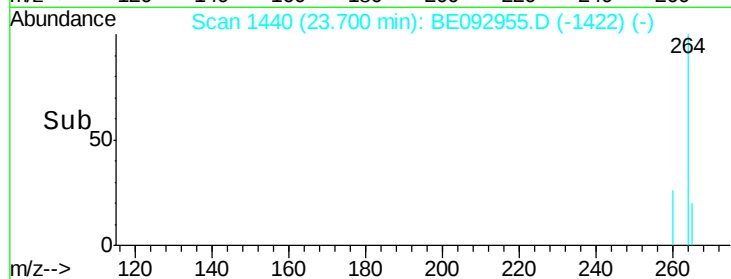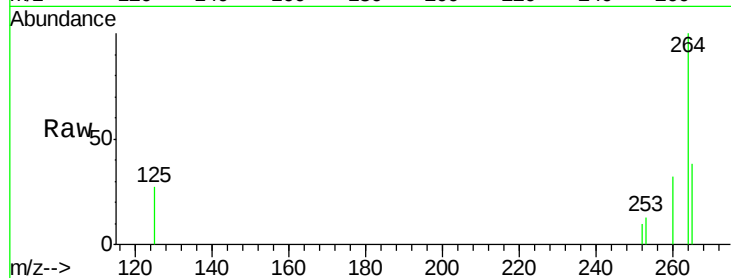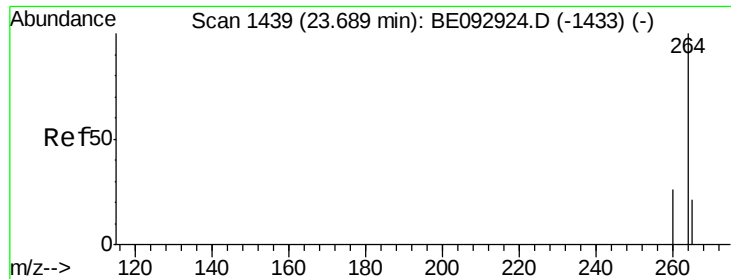

#33

Perylene-d12

Concen: 0.40 ng

RT: 23.70 min Scan# 1440

Delta R.T. 0.01 min

Lab File: BE092955.D

Acq: 6 May 2017 6:58

Instrument :

BNA_E

ClientSampleId :

3072-PA3

Tgt Ion: 264 Resp: 5261

Ion Ratio Lower Upper

264 100

260 31.6 23.5 35.3

265 38.1 27.2 40.8

