


Data Path : S:\HPCHEM1\BNA_E\Data\BE050517\
Data File : BE092921.D
Acq On : 5 May 2017 9:08
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE050517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 05 14:05:07 2017

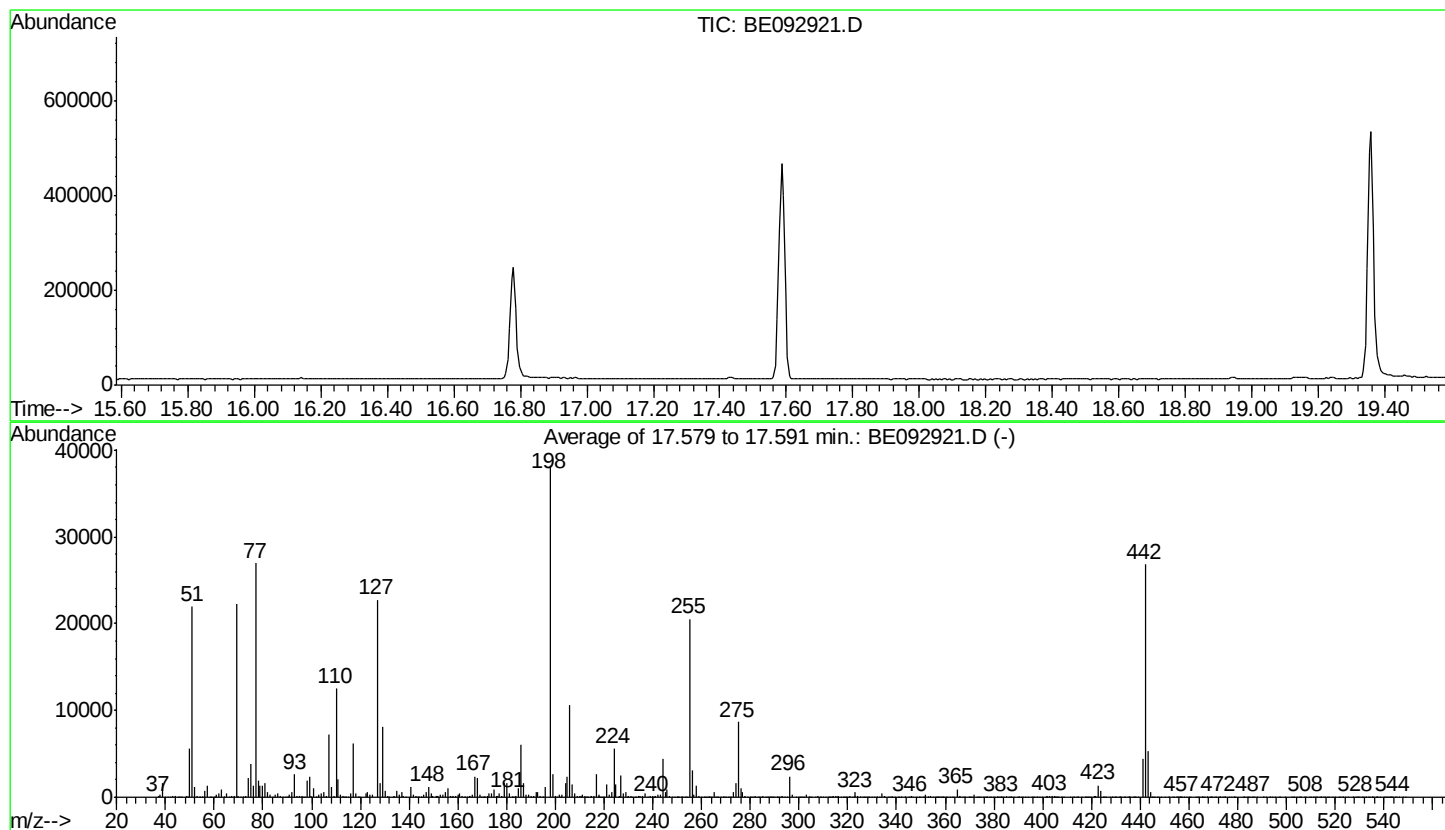

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.4	21949	PASS
68	69	0.00	2	0.6	131	PASS
69	198	0.00	100	58.4	22326	PASS
70	69	0.00	2	0.6	132	PASS
127	198	10	80	59.6	22768	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38221	PASS
199	198	5	9	7.0	2683	PASS
275	198	10	60	22.6	8650	PASS
365	198	1	100	2.5	937	PASS
441	442	0.01	24	16.7	4466	PASS
442	198	50	100	70.1	26790	PASS
443	442	15	24	19.8	5311	PASS