


Data Path : S:\HPCHEM1\BNA_E\Data\BE050517\
 Data File : BE092933.D
 Acq On : 5 May 2017 17:02
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE050517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 05 14:05:07 2017

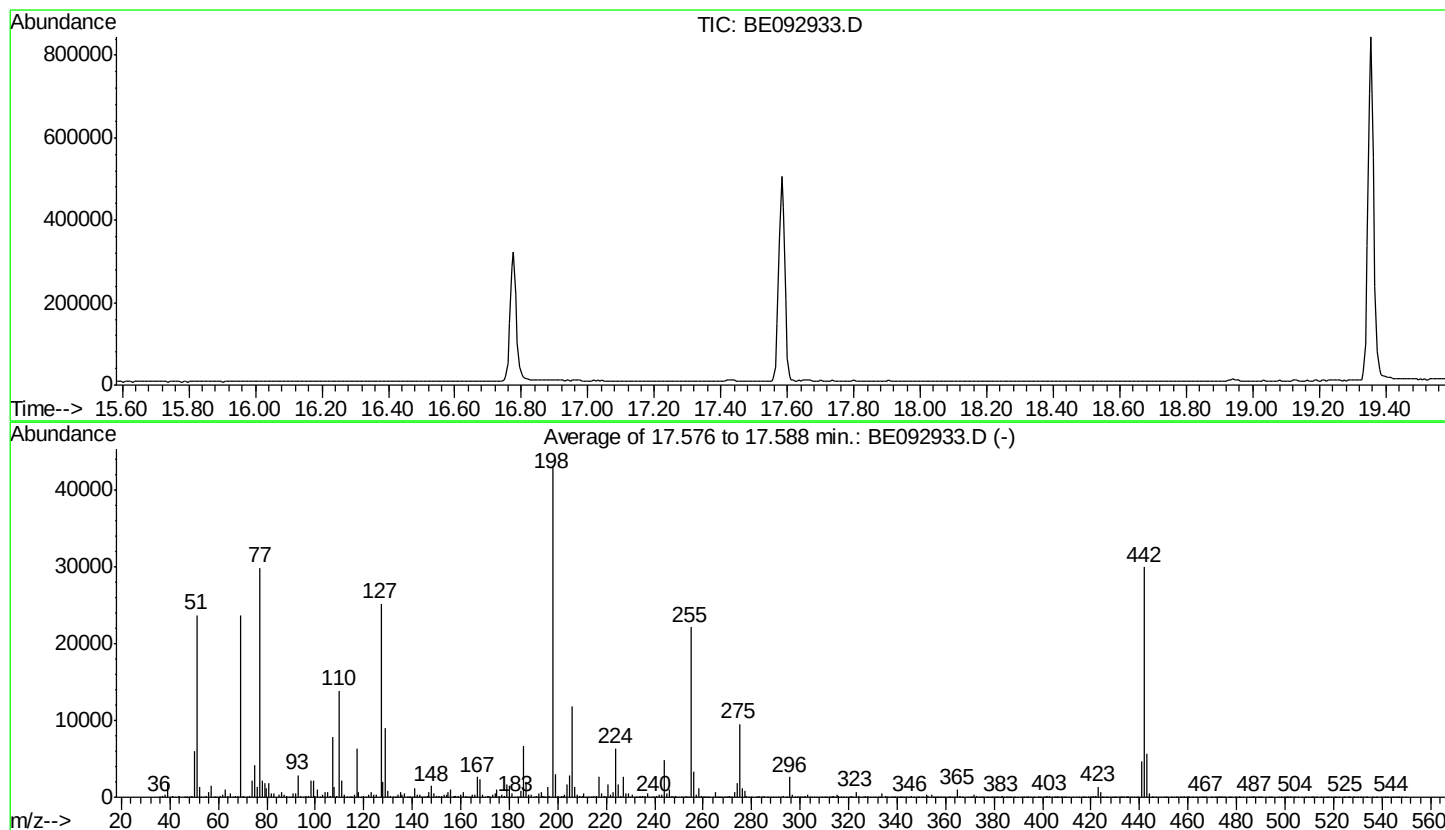

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	23722	PASS
68	69	0.00	2	0.5	125	PASS
69	198	0.00	100	54.9	23715	PASS
70	69	0.00	2	0.5	121	PASS
127	198	10	80	58.5	25232	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43168	PASS
199	198	5	9	7.1	3073	PASS
275	198	10	60	22.1	9560	PASS
365	198	1	100	2.2	946	PASS
441	442	0.01	24	15.3	4598	PASS
442	198	50	100	69.5	29984	PASS
443	442	15	24	18.9	5678	PASS