


Data Path : S:\HPCHEM1\BNA\_E\Data\BE050517\  
 Data File : BE092951.D  
 Acq On : 6 May 2017 4:25  
 Operator : SJ/MA  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE050517.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri May 05 14:05:07 2017

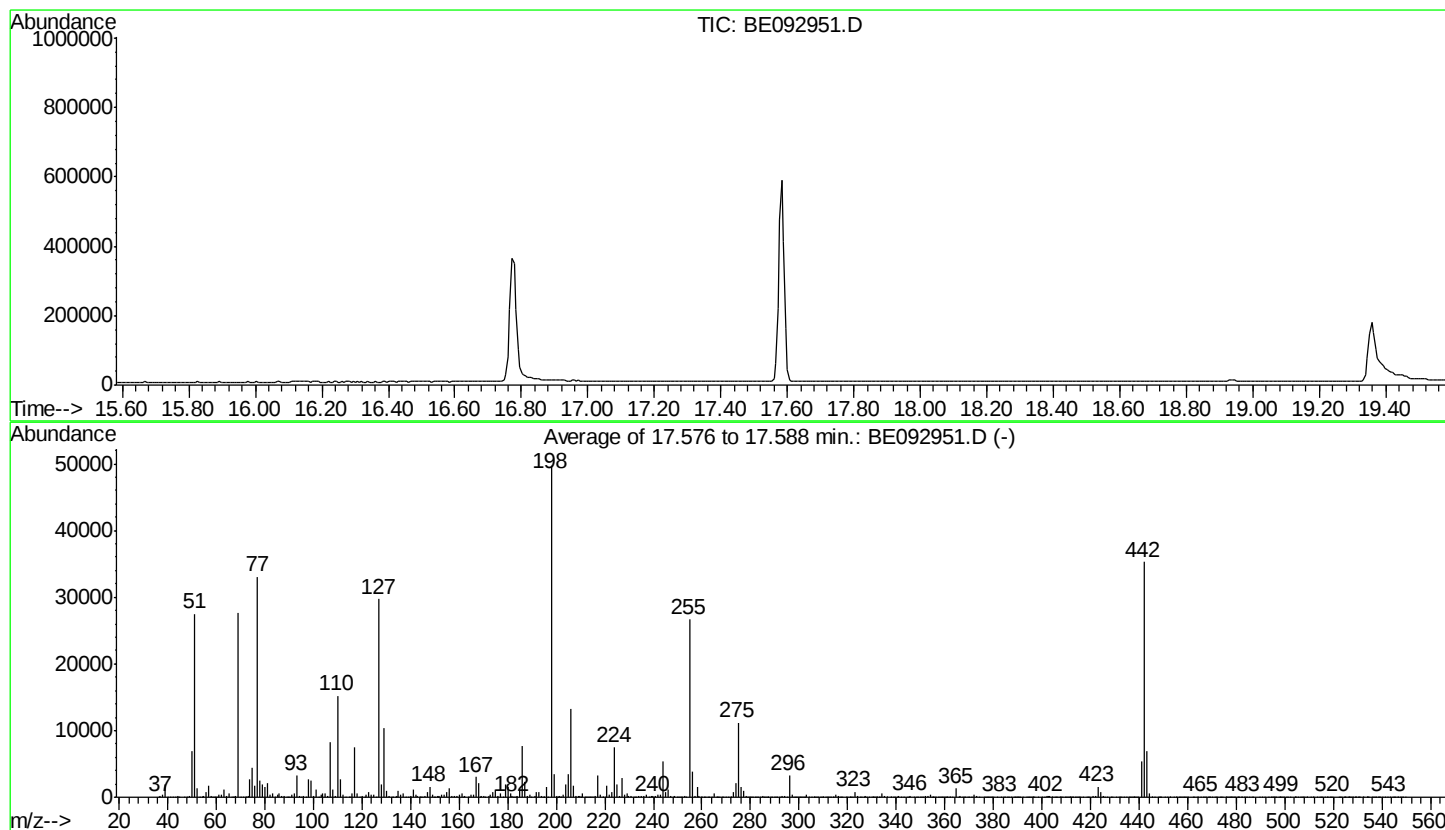

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2543

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 55.4      | 27543   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.6       | 172     | PASS             |
| 69          | 198          | 0.00         | 100          | 55.6      | 27645   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 95      | PASS             |
| 127         | 198          | 10           | 80           | 59.7      | 29688   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 49725   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 3391    | PASS             |
| 275         | 198          | 10           | 60           | 22.6      | 11230   | PASS             |
| 365         | 198          | 1            | 100          | 2.6       | 1285    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.4      | 5420    | PASS             |
| 442         | 198          | 50           | 100          | 71.0      | 35307   | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 6929    | PASS             |