


Data Path : Z:\HPCHEM1\BNA_E\Data\BE050917\
 Data File : BE092958.D
 Acq On : 9 May 2017 10:18
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE050517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 09 15:34:16 2017

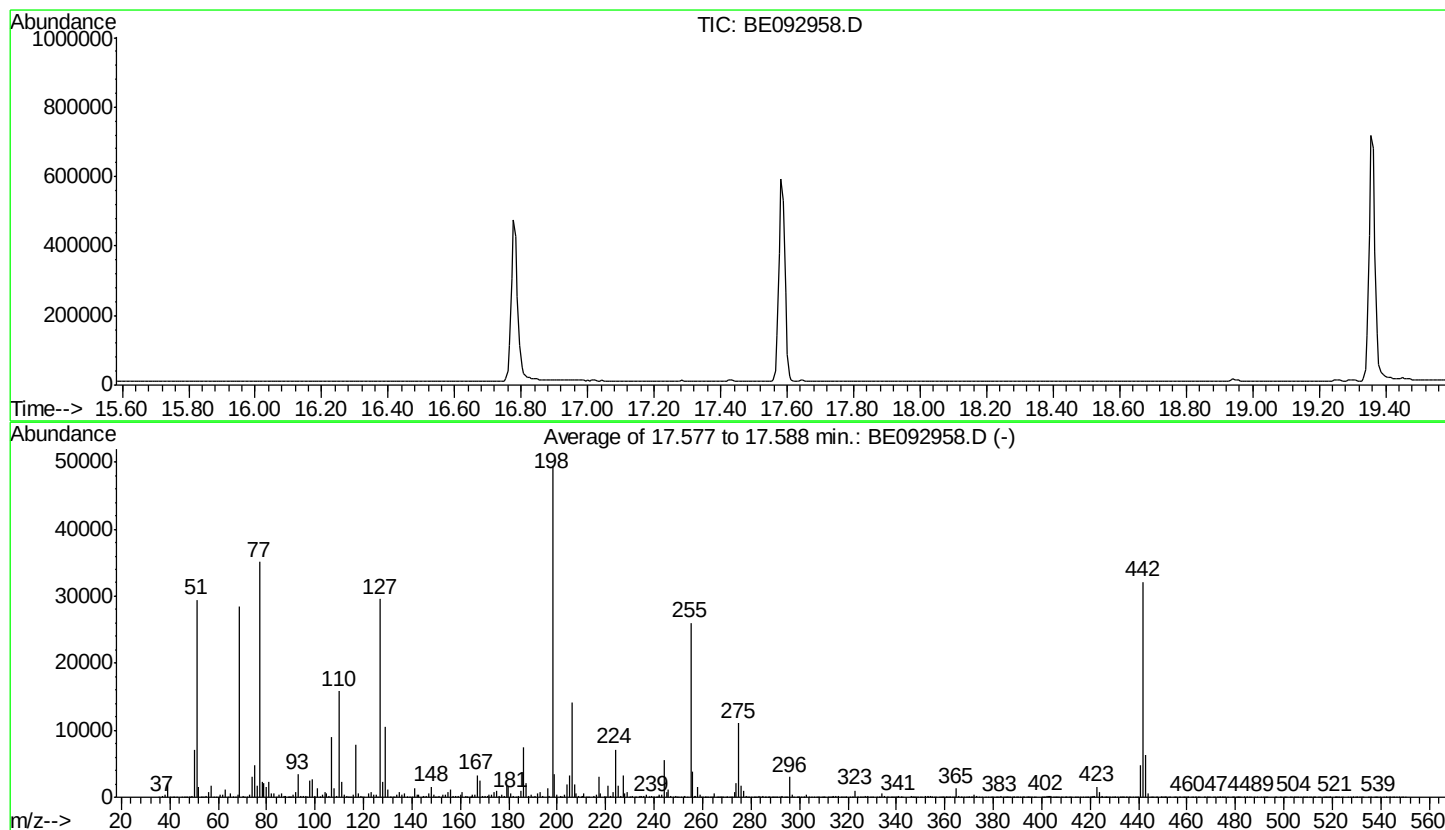

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.6	29484	PASS
68	69	0.00	2	1.3	375	PASS
69	198	0.00	100	57.6	28514	PASS
70	69	0.00	2	0.6	166	PASS
127	198	10	80	59.8	29582	PASS
197	198	0.00	2	0.4	219	PASS
198	198	100	100	100.0	49470	PASS
199	198	5	9	6.9	3434	PASS
275	198	10	60	22.4	11070	PASS
365	198	1	100	2.5	1258	PASS
441	442	0.01	24	15.0	4826	PASS
442	198	50	100	65.0	32176	PASS
443	442	15	24	19.7	6348	PASS