
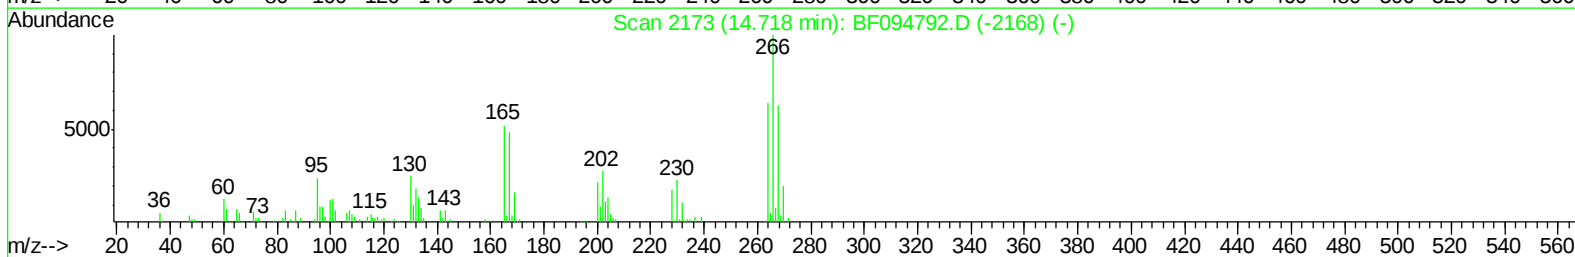
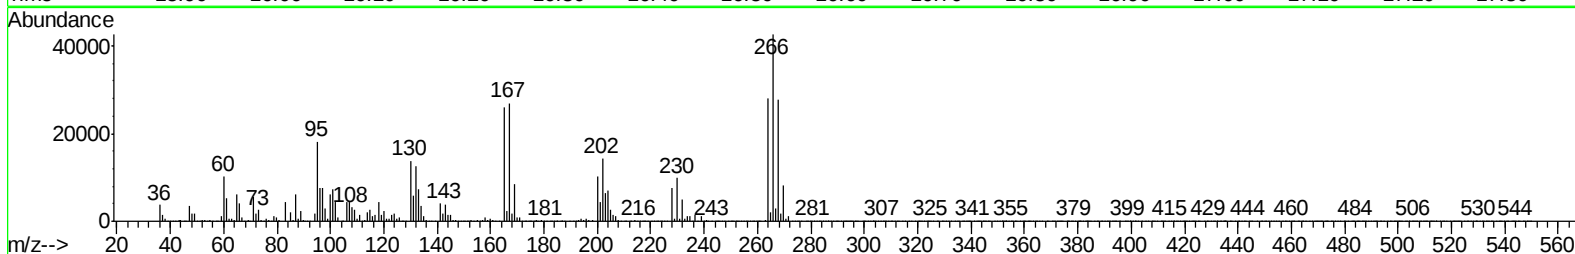


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051017\
Data File : BE092974.D
Acq On : 10 May 2017 9:10
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 06:49:32 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

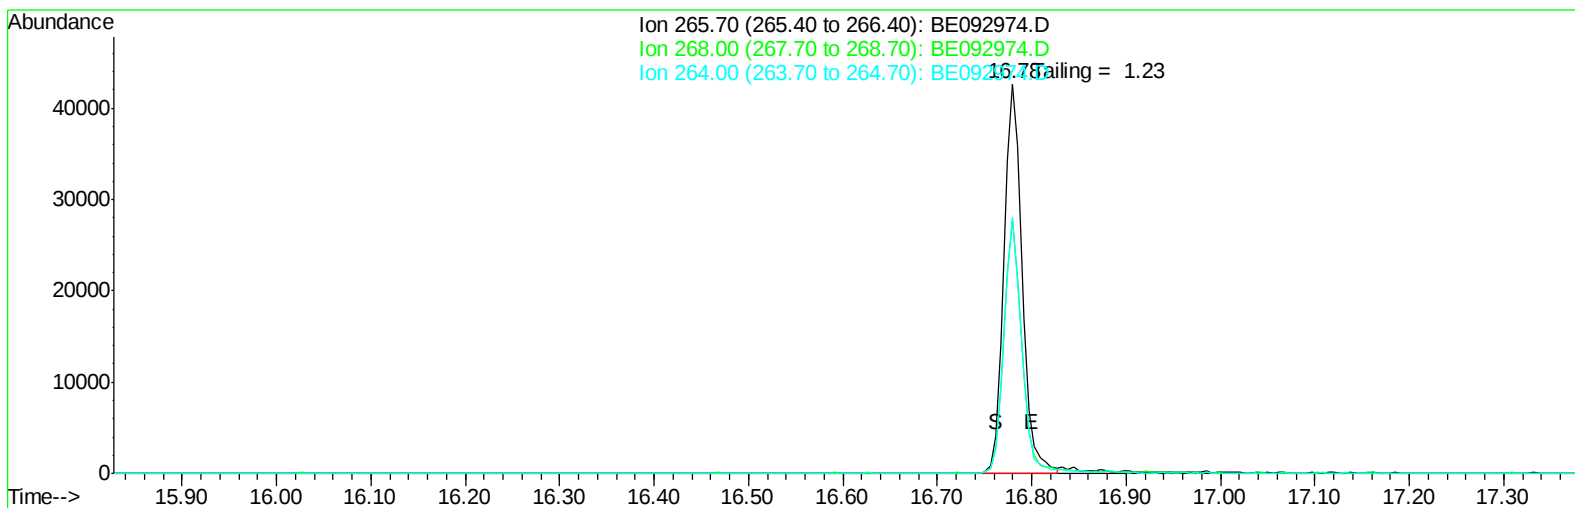

TIC: BE092974.D

(69) Pentachlorophenol (C)




14.770min (+0.052) 294.31ng

response 32

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	71.88
264.00	64.60	62.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051017\
Data File : BE092974.D
Acq On : 10 May 2017 9:10
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 06:49:32 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

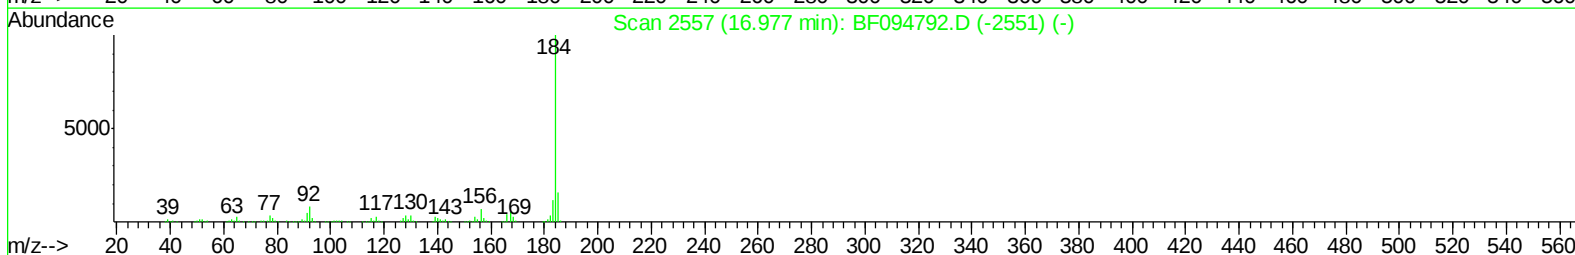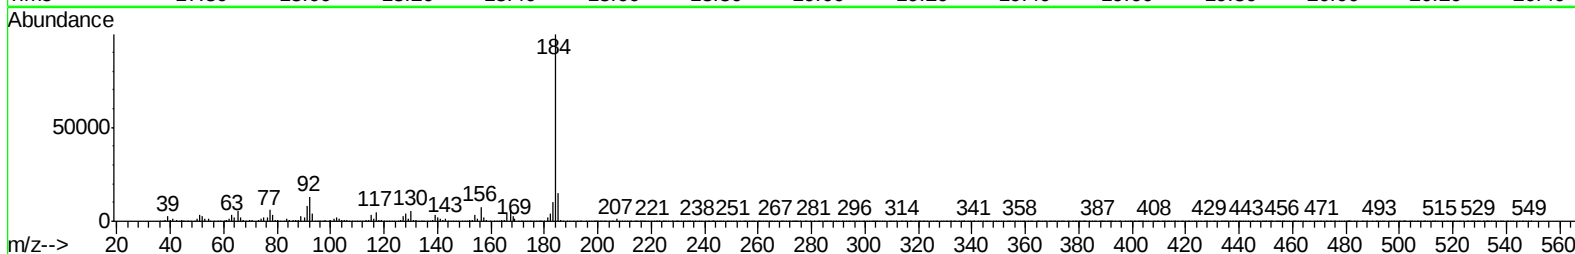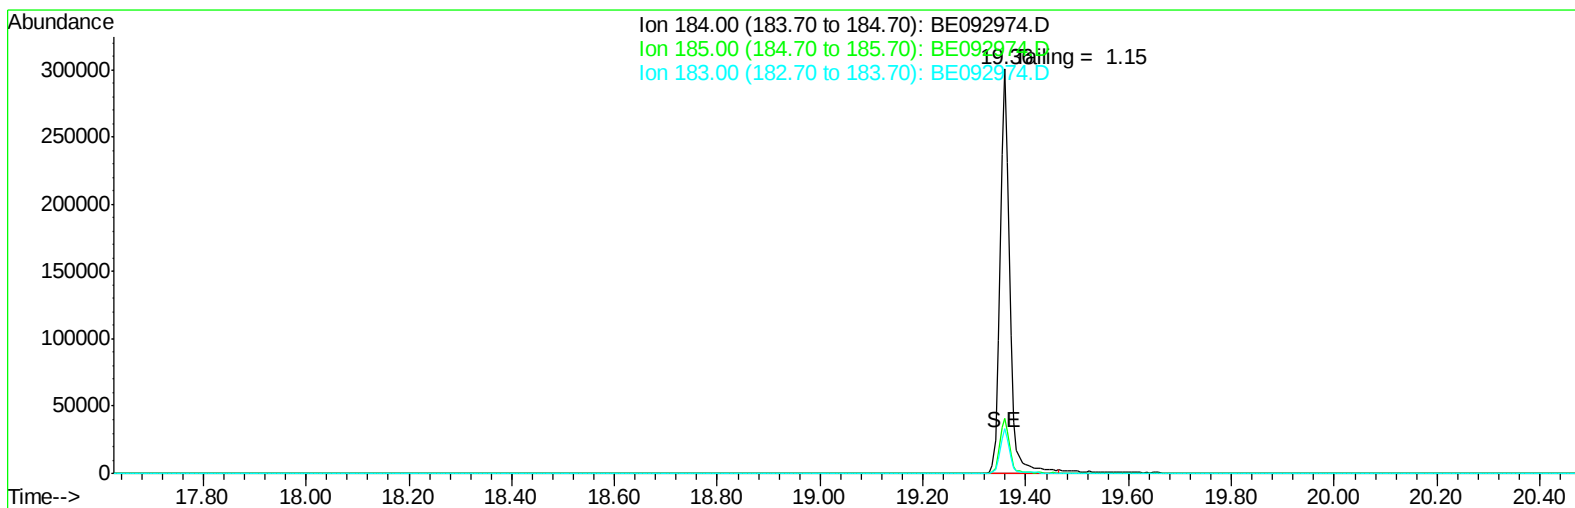

TIC: BE092974.D

(76) Benzidine

16.915min (-0.062) 205.96ng

response 50

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	60.98#
183.00	12.20	34.15#
0.00	0.00	0.00