
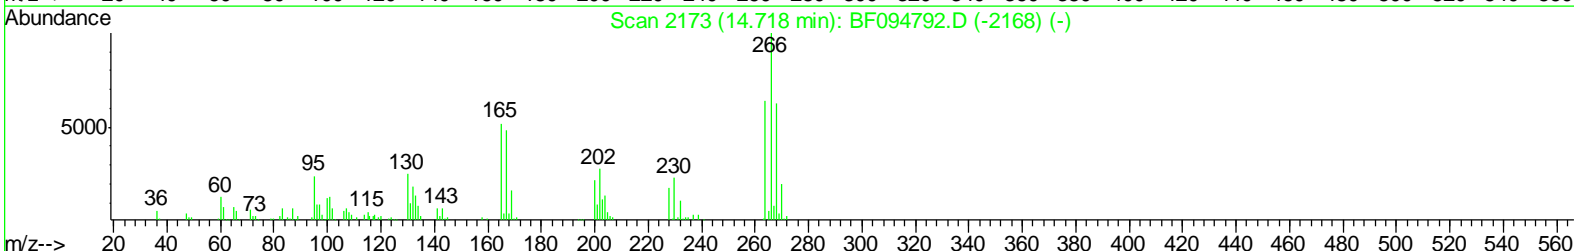
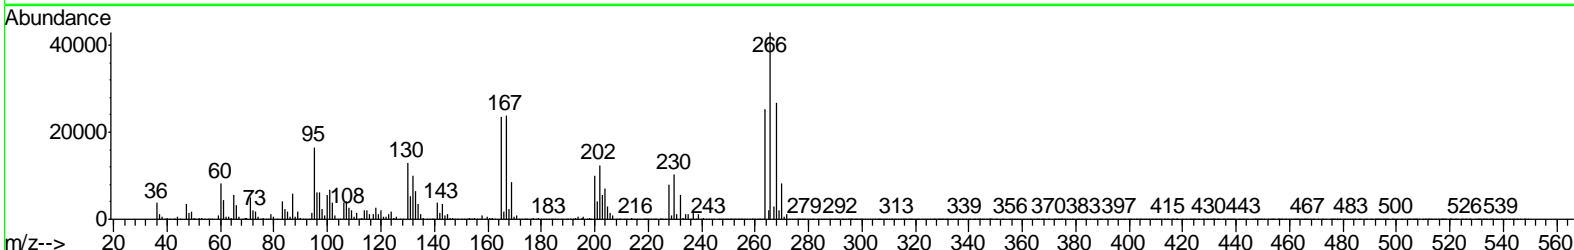


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051017\
 Data File : BE092980.D
 Acq On : 10 May 2017 13:56
 Operator : SJ/MA
 Sample : DF7TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 06:51:09 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration

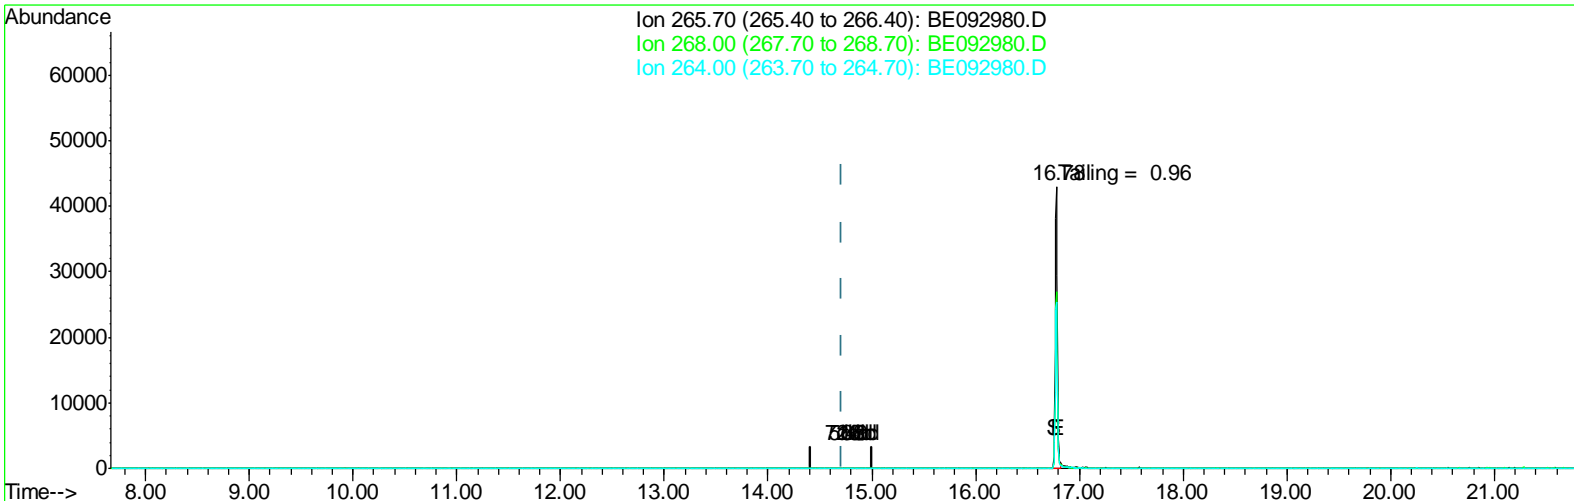




TIC: BE092980.D

(69) Pentachlorophenol (C)
 14.728min (+0.009) 678.91ng
 response 32

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	73.53
264.00	64.60	76.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051017\
 Data File : BE092980.D
 Acq On : 10 May 2017 13:56
 Operator : SJ/MA
 Sample : DF7PP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 06:51:09 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration

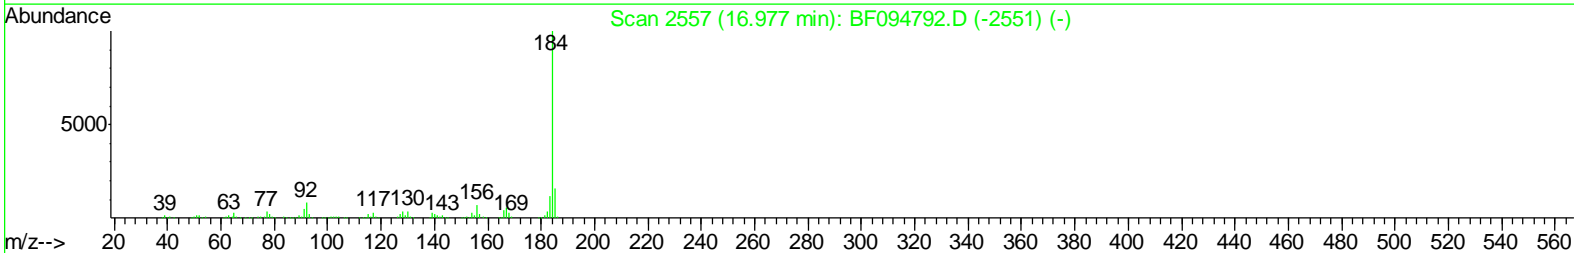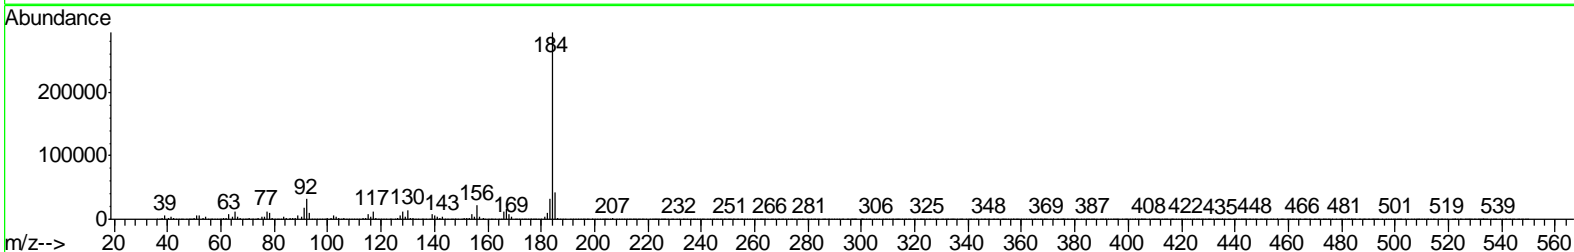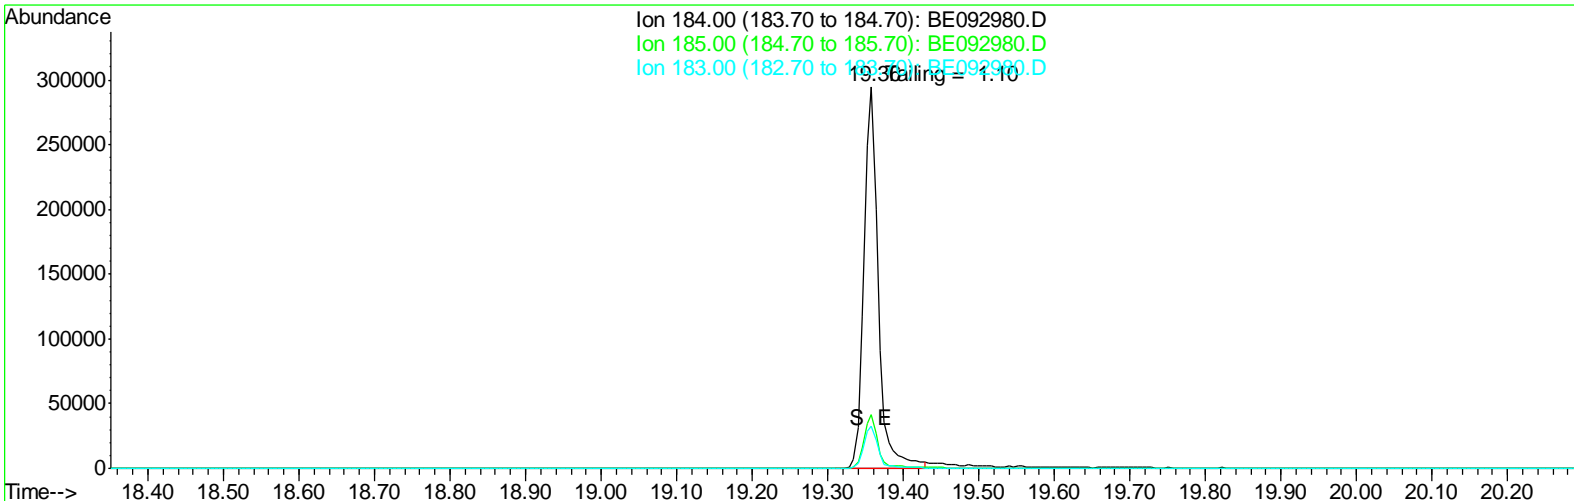

TIC: BE092980.D

(76) Benzidine

17.066min (+0.089) 54.44ng

response 36

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	39.02#
183.00	12.20	2.44#
0.00	0.00	0.00