


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051017\
 Data File : BE092966.D
 Acq On : 9 May 2017 16:42
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 10 03:43:15 2017

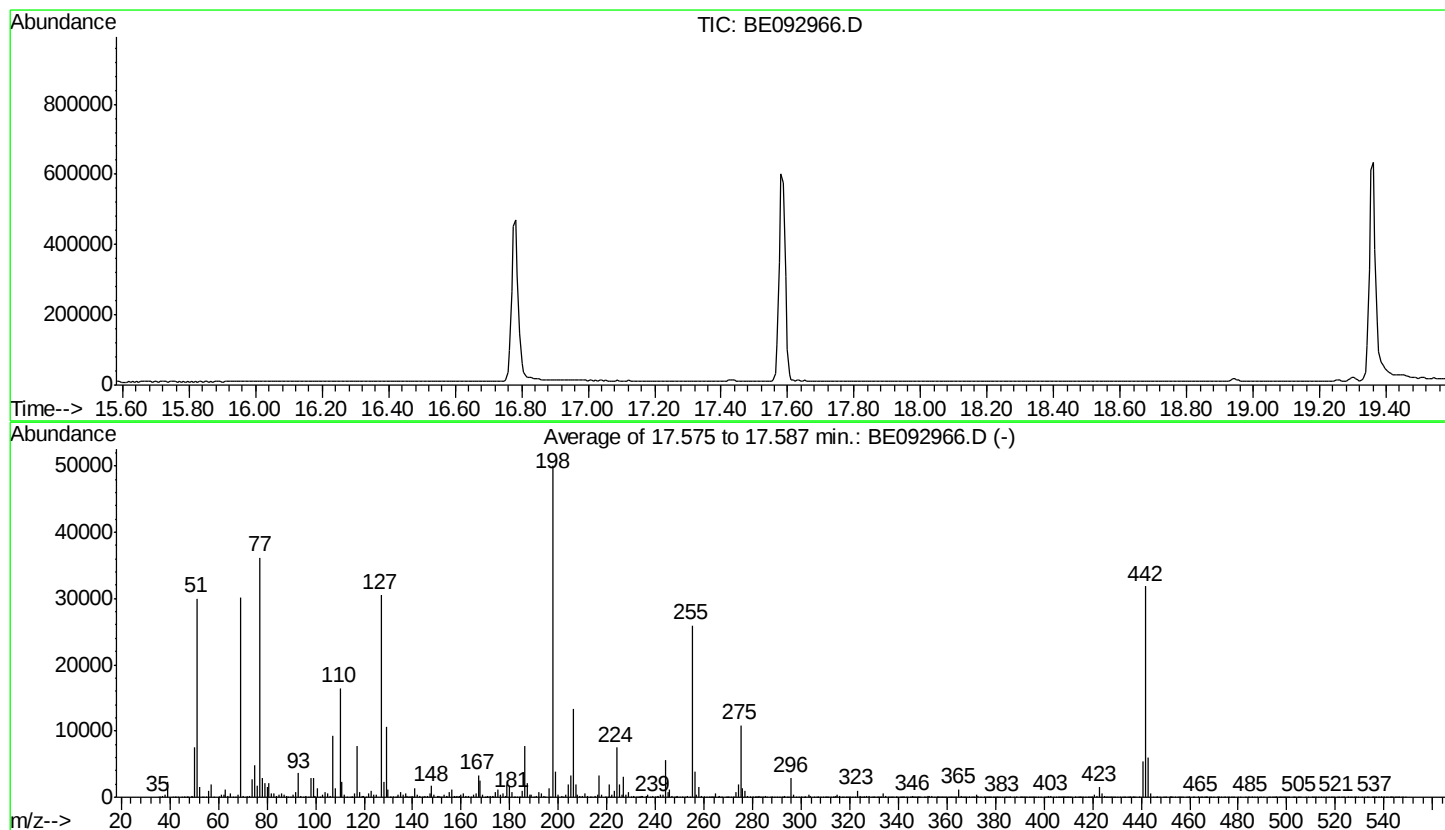

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.8	29954	PASS
68	69	0.00	2	1.1	331	PASS
69	198	0.00	100	60.1	30084	PASS
70	69	0.00	2	0.4	125	PASS
127	198	10	80	61.1	30570	PASS
197	198	0.00	2	0.1	32	PASS
198	198	100	100	100.0	50061	PASS
199	198	5	9	7.6	3788	PASS
275	198	10	60	21.7	10839	PASS
365	198	1	100	2.4	1216	PASS
441	442	0.01	24	16.7	5324	PASS
442	198	50	100	63.7	31874	PASS
443	442	15	24	19.0	6055	PASS