


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051017\
 Data File : BE092974.D
 Acq On : 10 May 2017 9:10
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 10 03:43:15 2017

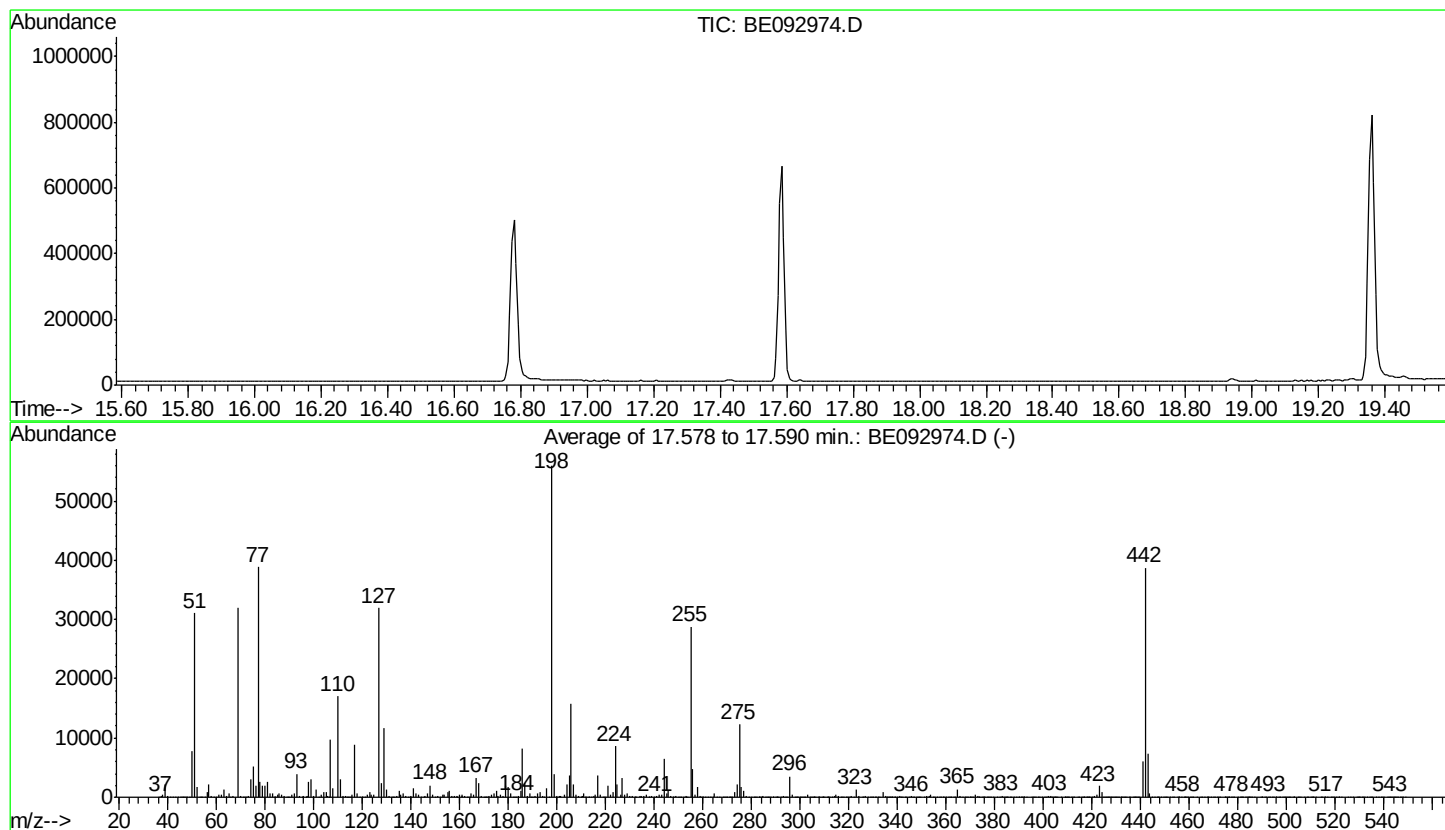

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2543

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.5	31058	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	57.1	31953	PASS
70	69	0.00	2	0.4	139	PASS
127	198	10	80	57.0	31898	PASS
197	198	0.00	2	0.2	93	PASS
198	198	100	100	100.0	55959	PASS
199	198	5	9	6.9	3883	PASS
275	198	10	60	22.0	12311	PASS
365	198	1	100	2.5	1383	PASS
441	442	0.01	24	15.6	6038	PASS
442	198	50	100	69.2	38717	PASS
443	442	15	24	18.7	7254	PASS