
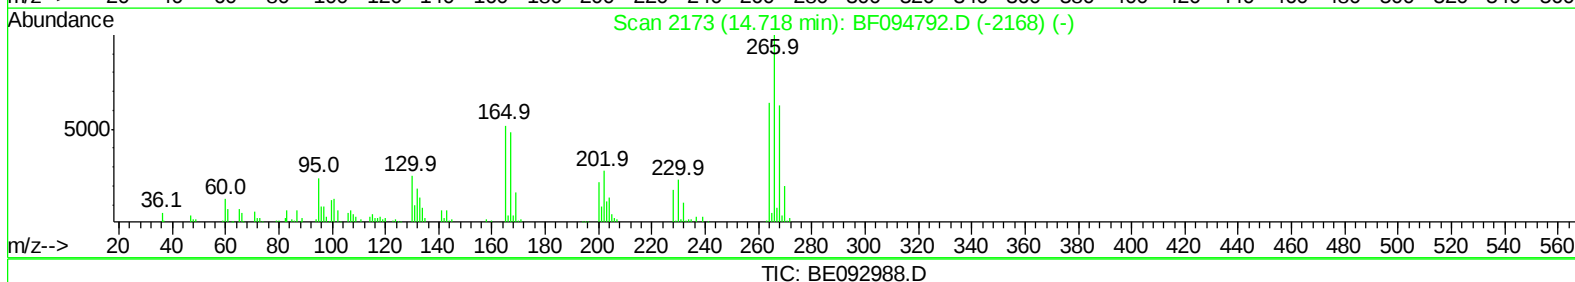
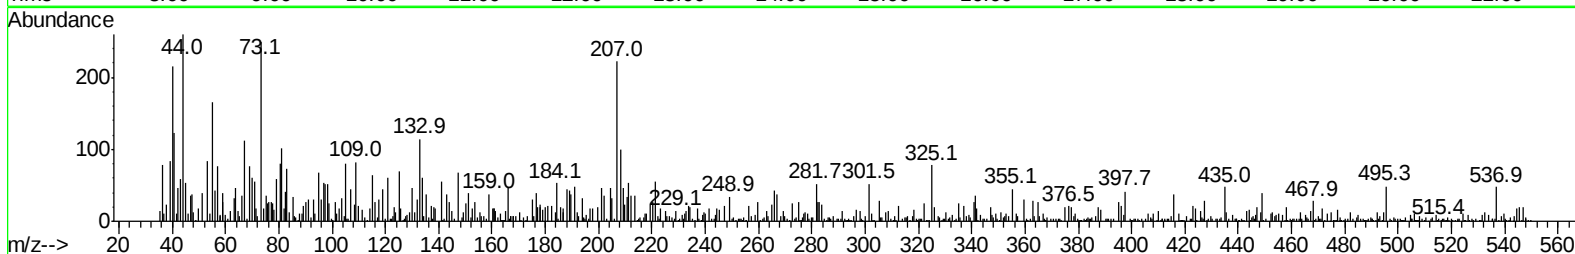


Data Path : Z:\HPCHEM1\BNA E\DATA\BE051117\
Data File : BE092988.D
Acq On : 11 May 2017 10:05
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 17:09:03 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

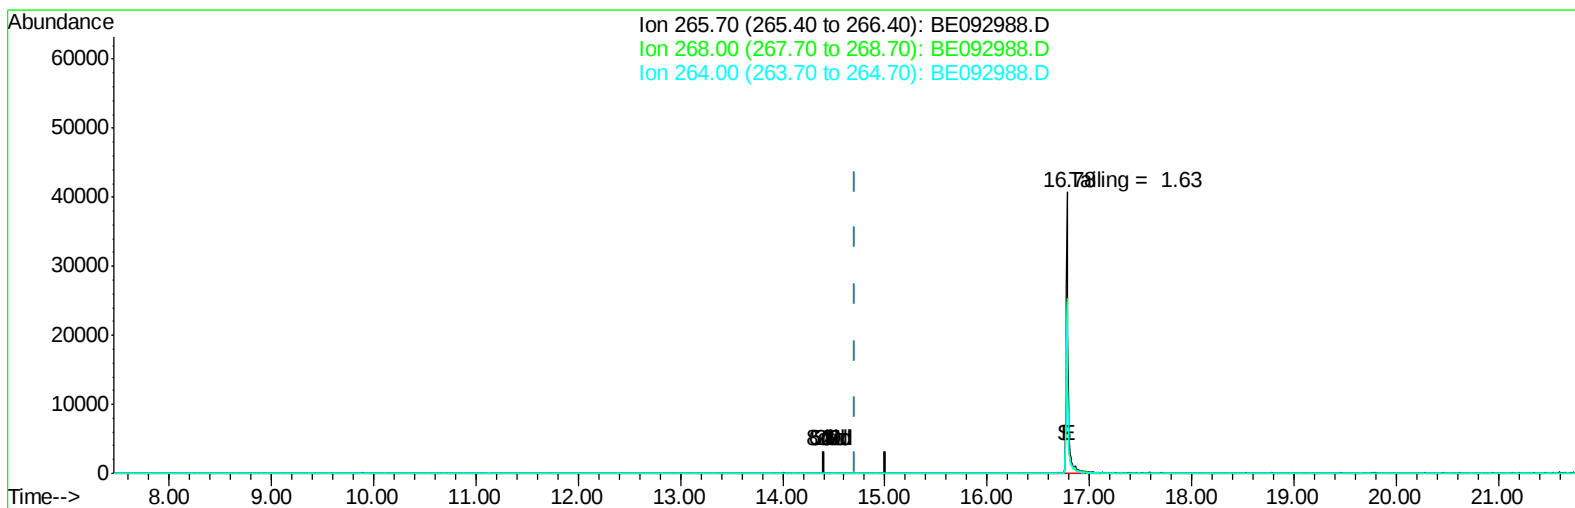

TIC: BE092988.D

(69) Pentachlorophenol (C)




14.469min (-0.250) 206.63ng

response 35

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	16.28#
264.00	64.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE051117\
Data File : BE092988.D
Acq On : 11 May 2017 10:05
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 17:09:03 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

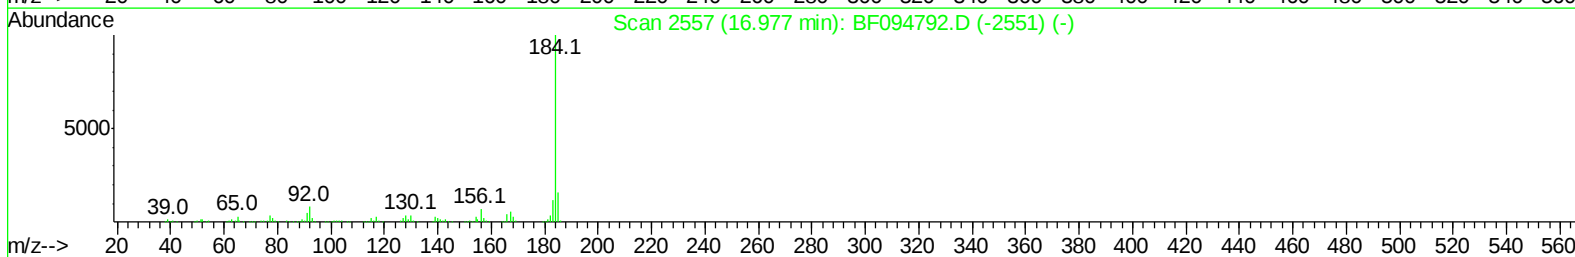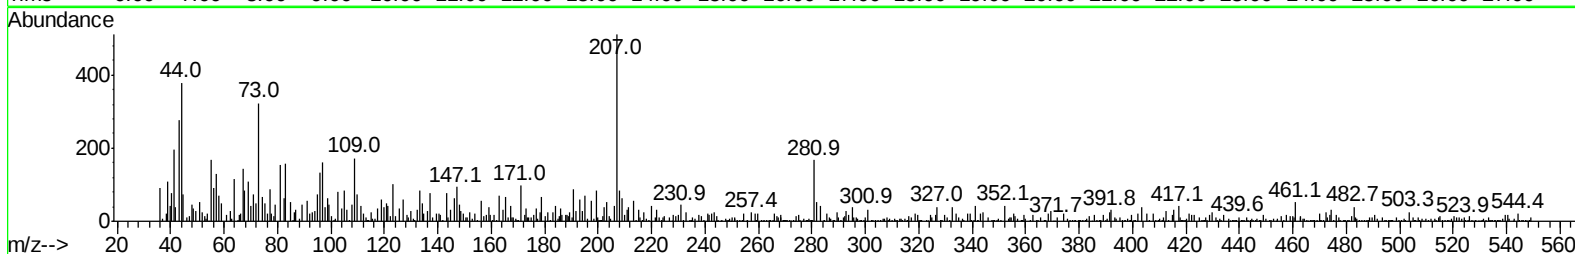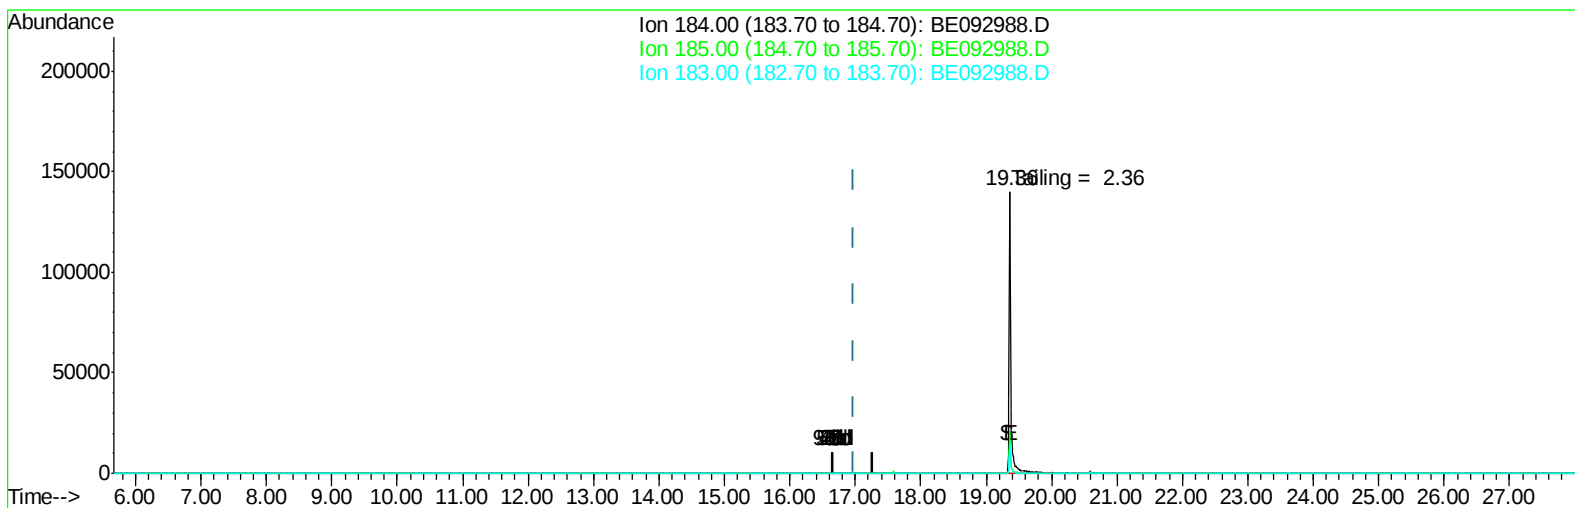

TIC: BE092988.D

(76) Benzidine

16.672min (-0.305) 39.76ng

response 26

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	51.22#
183.00	12.20	63.41#
0.00	0.00	0.00