

Data Path : Z:\HPCHEM1\BNA E\DATA\BE051117\
 Data File : BE093000.D
 Acq On : 11 May 2017 17:32
 Operator : SJ/MA
 Sample : I3058-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 LF001MW003-170508

Quant Time: May 11 18:54:44 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE051117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 11 14:48:08 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	844	0.40	ng	-0.02
7) Naphthalene-d8	10.52	136	3383	0.40	ng	0.00
13) Acenaphthene-d10	14.39	164	1692	0.40	ng	0.00
19) Phenanthrene-d10	17.13	188	4935	0.40	ng	0.00
27) Chrysene-d12	21.28	240	5070	0.40	ng	0.00
34) Perylene-d12	23.69	264	4137	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.35	112	456	0.20	ng	0.00
5) Phenol-d6	6.92	99	445	0.15	ng	-0.02
8) Nitrobenzene-d5	8.88	82	927	0.35	ng	-0.02
11) 2-Methylnaphthalene-d10	12.11	152	1867	0.39	ng	-0.02
14) 2,4,6-Tribromophenol	15.87	330	202	0.44	ng	-0.01
15) 2-Fluorobiphenyl	13.01	172	3479	0.52	ng	0.00
25) Fluoranthene-d10	19.14	212	4916	0.38	ng	-0.02
29) Terphenyl-d14	19.74	244	6697	0.74	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.31	88	21336	12.60	ng	Qvalue 96
6) bis(2-Chloroethyl)ether	7.18	93	502	0.18	ng	# 96
22) Pentachlorophenol	16.82	266	83	0.21	ng	92
32) Bis(2-ethylhexyl)phthalate	21.20	149	321	0.16	ng	# 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE051117\
Data File : BE093000.D
Acq On : 11 May 2017 17:32
Operator : SJ/MA
Sample : I3058-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
LF001MW003-170508

Quant Time: May 11 18:54:44 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE051117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 14:48:08 2017
Response via : Initial Calibration

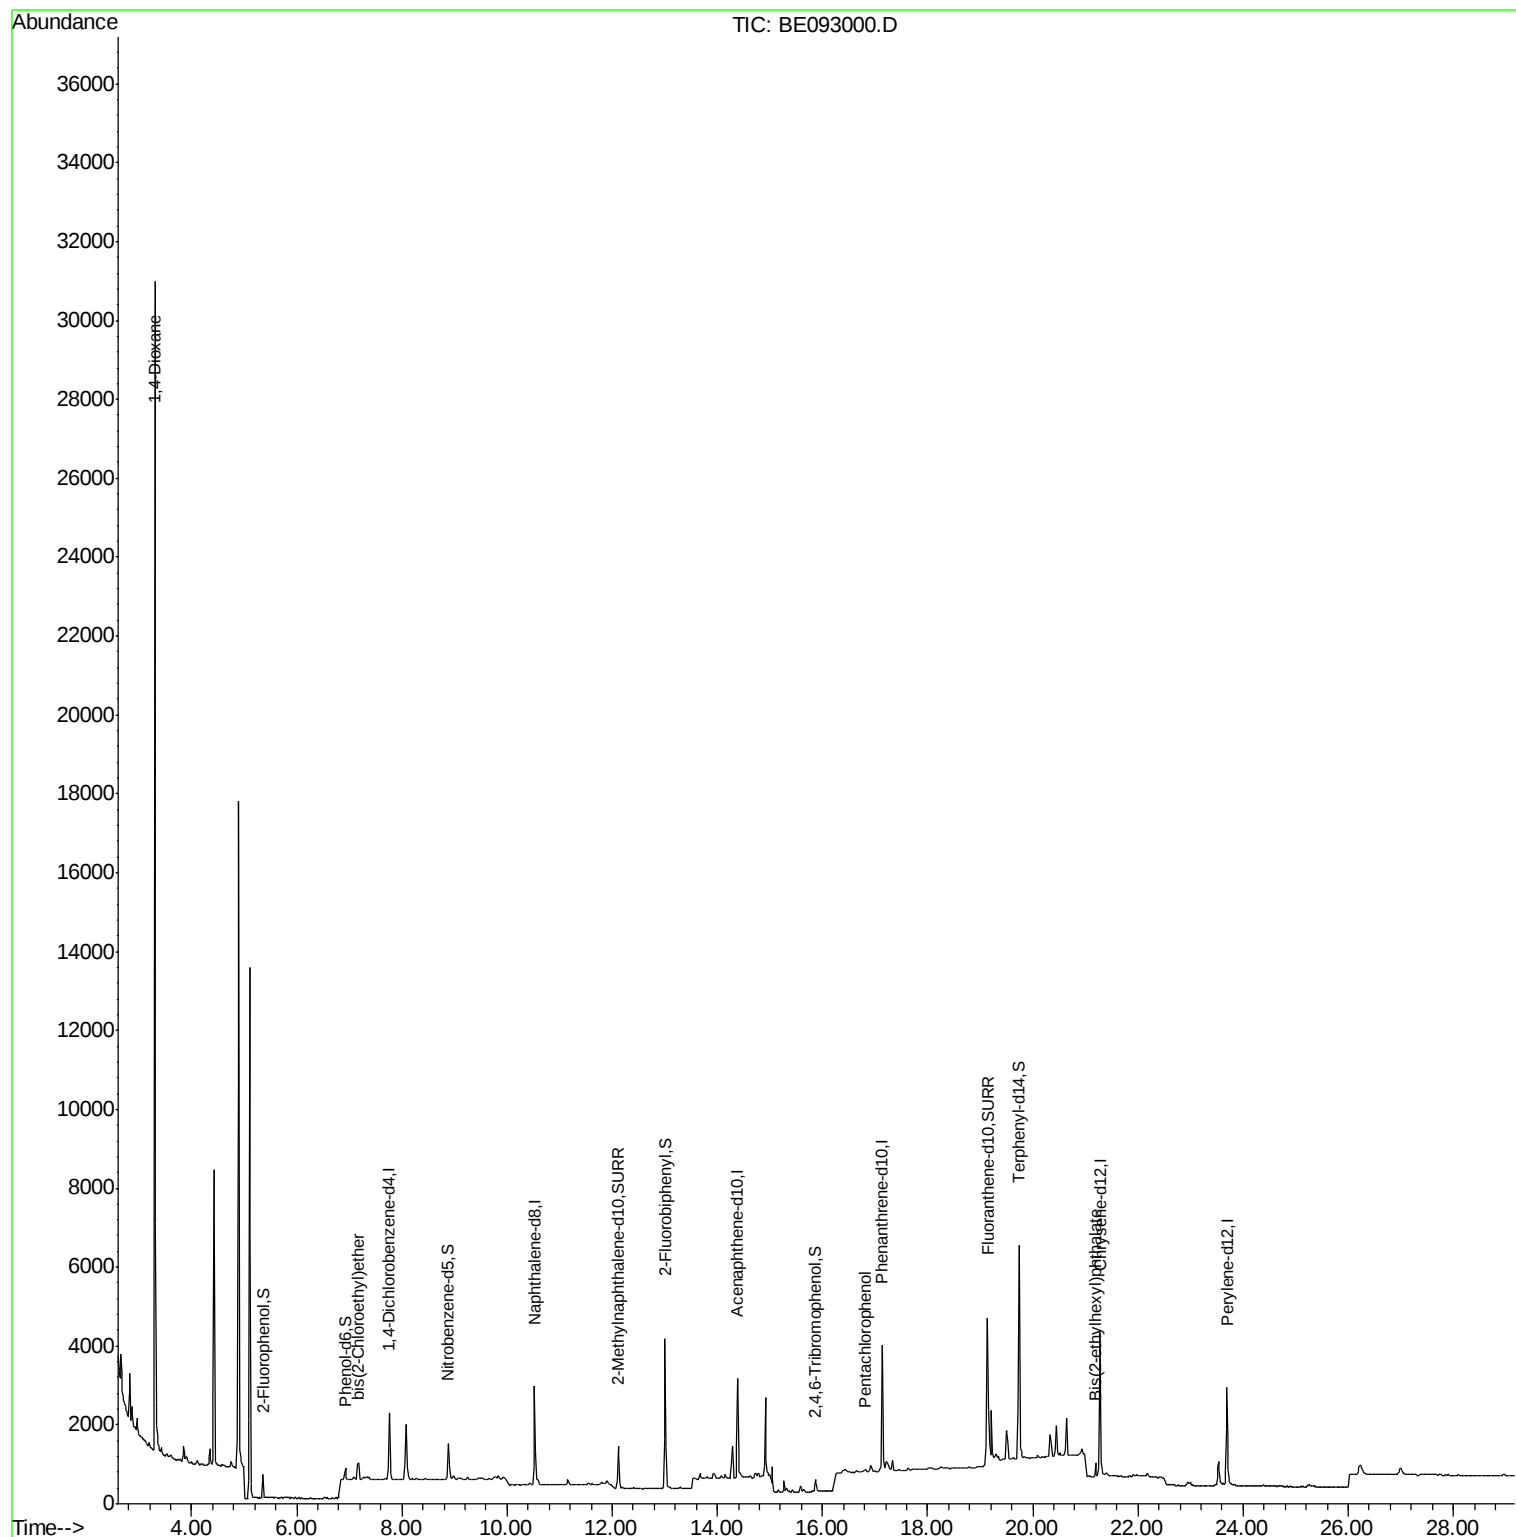



#1

1,4-Dichlorobenzene-d4

Concen: 0.40 ng

RT: 7.75 min Scan# 555

Delta R.T. -0.02 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32

Instrument :

BNA_E

ClientSampleId :

LF001MW003-170508


Tot Ion:152 Resp: 844

Ion Ratio Lower Upper

152 100

150 149.7 125.1 187.7




115 61.7 55.7 83.5

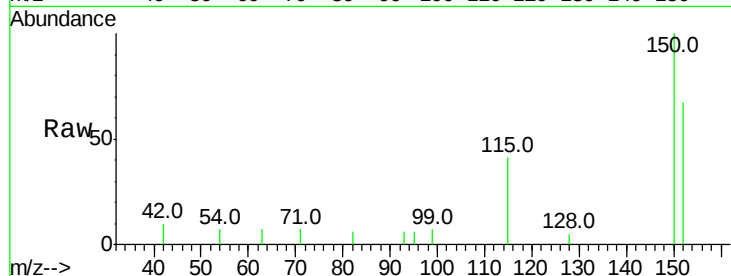

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

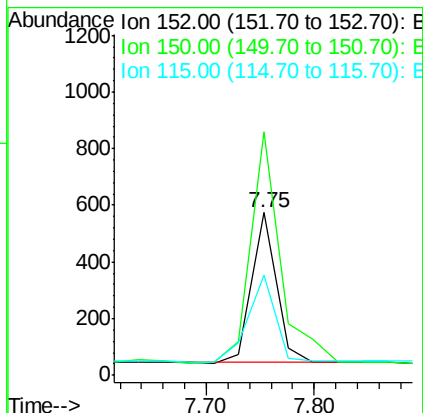

#2

1,4-Dioxane

Concen: 12.60 ng

RT: 3.31 min Scan# 62

Delta R.T. 0.00 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32


Tgt Ion: 88 Resp: 21336

Ion Ratio Lower Upper

88 100

58 80.7 62.2 93.4



43 31.9 23.2 34.8




Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

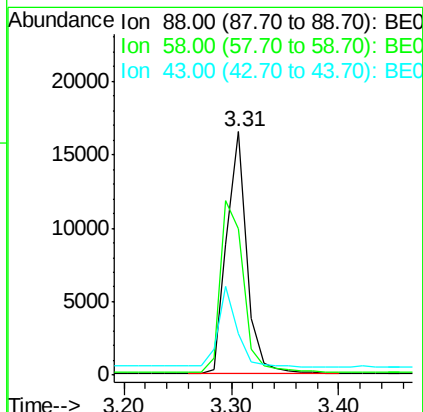

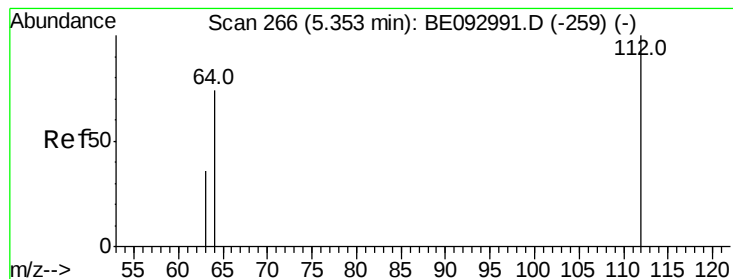

#4

2-Fluorophenol

Concen: 0.20 ng

RT: 5.35 min Scan# 266

Delta R.T. -0.00 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32

Instrument :

BNA_E

ClientSampleId :

LF001MW003-170508


Tot Ion:112 Resp: 456

Ion Ratio Lower Upper

112 100

64 69.7 56.4 84.6


63 36.0 29.3 43.9

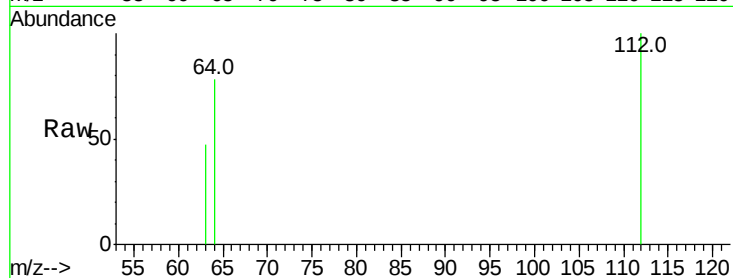



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

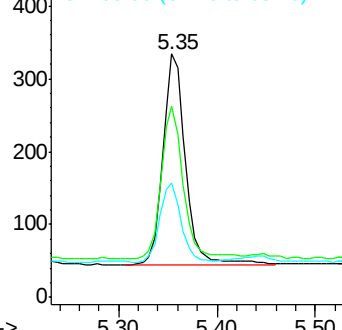

Time-->

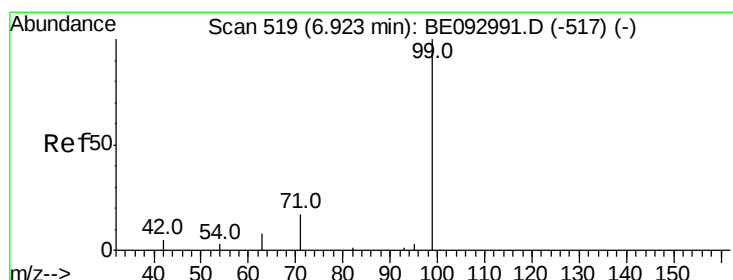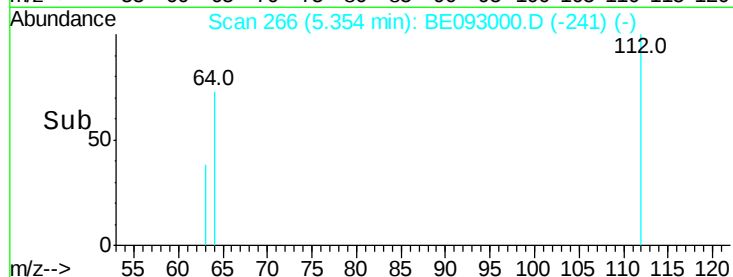

#5

Phenol-d6

Concen: 0.15 ng

RT: 6.92 min Scan# 519

Delta R.T. -0.02 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32


Tgt Ion: 99 Resp: 445

Ion Ratio Lower Upper

99 100

42 0.0 0.0 0.0


71 0.0 0.0 0.0

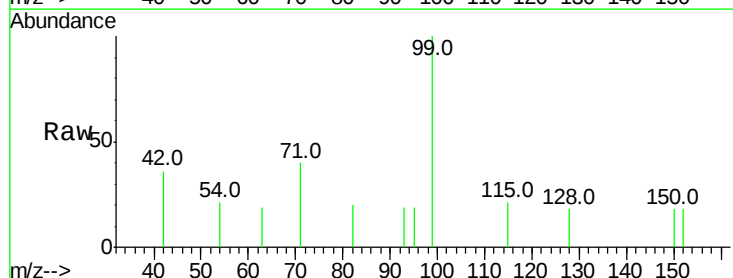


Abundance Ion 99.00 (98.70 to 99.70): BE0


Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

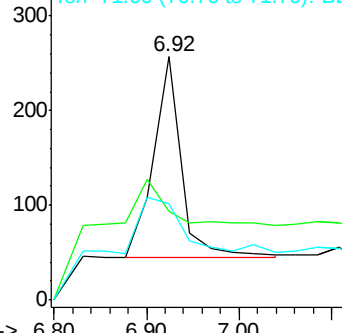

Time-->

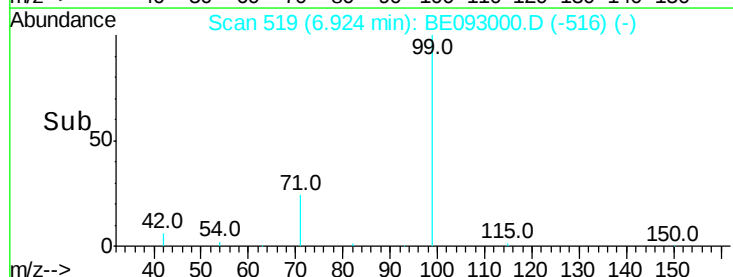



#6

bis(2-Chloroethyl)ether

Concen: 0.18 ng

RT: 7.18 min Scan# 530

Delta R.T. -0.02 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32

Instrument :

BNA_E

ClientSampleId :

LF001MW003-170508


Tot Ion: 93 Resp: 502

Ion Ratio Lower Upper

93 100

63 0.0 0.0 0.0




95 33.7 25.4 38.0

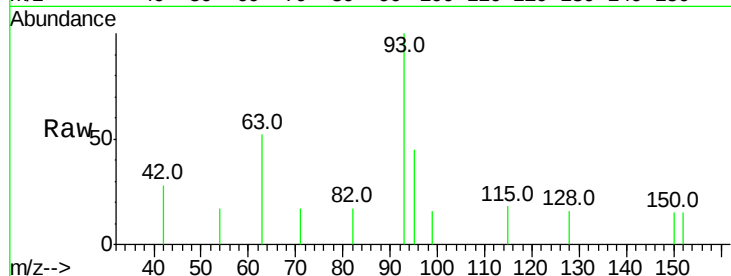

Abundance Ion 93.00 (92.70 to 93.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Ion 95.00 (94.70 to 95.70): BE0

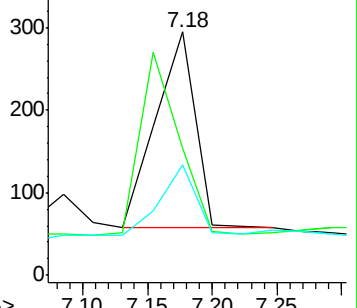

#7

Naphthalene-d8

Concen: 0.40 ng

RT: 10.52 min Scan# 678

Delta R.T. -0.00 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32

Tgt Ion: 136 Resp: 3383


Ion Ratio Lower Upper

136 100

137 12.3 9.8 14.8

54 11.9 10.3 15.5

68 11.0 9.0 13.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

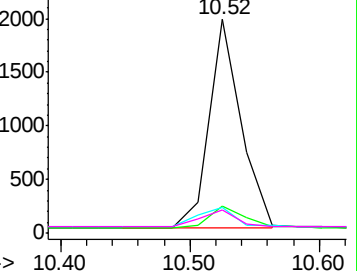

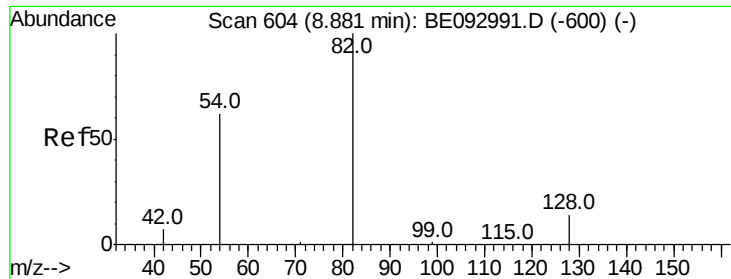

#8

Nitrobenzene-d5

Concen: 0.35 ng

RT: 8.88 min Scan# 604

Delta R.T. -0.02 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32

Instrument :

BNA_E

ClientSampleId :

LF001MW003-170508


Tot Ion: 82 Resp: 927

Ion Ratio Lower Upper

82 100

128 21.4 17.0 25.4




54 63.1 53.8 80.6

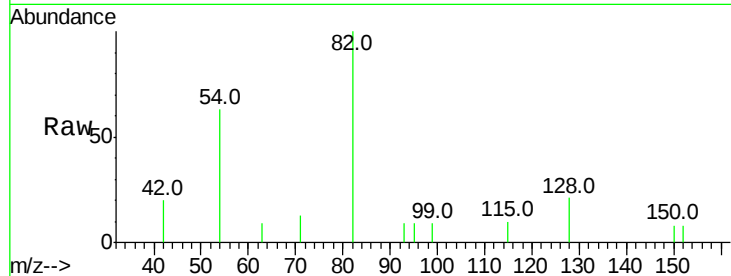

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

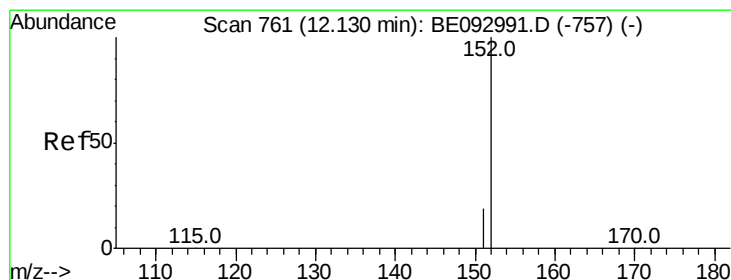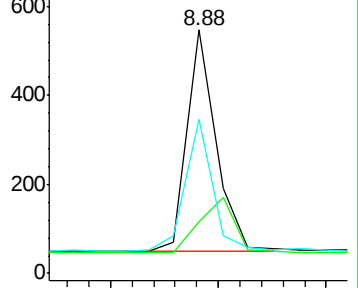

#11

2-Methylnaphthalene-d10

Concen: 0.39 ng

RT: 12.11 min Scan# 760

Delta R.T. -0.02 min

Lab File: BE093000.D


Acq: 11 May 2017 17:32

Tgt Ion: 152 Resp: 1867

Ion Ratio Lower Upper



152 100


151 19.6 15.1 22.7



Abundance Ion 152.00 (151.70 to 152.70): BE0

Ion 151.00 (150.70 to 151.70): BE0

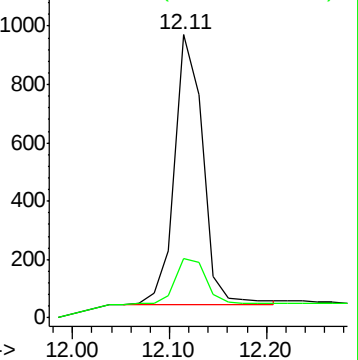

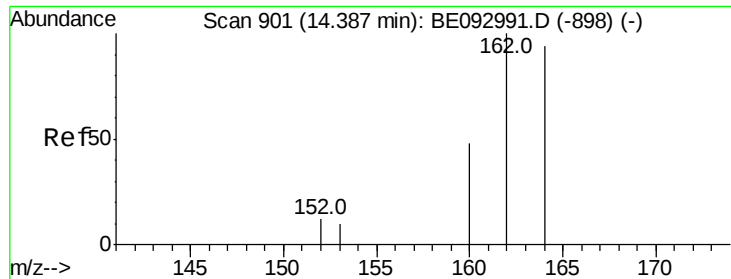

#13

Acenaphthene-d10

Concen: 0.40 ng

RT: 14.39 min Scan# 901

Delta R.T. -0.00 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32

Instrument :

BNA_E

ClientSampleId :

LF001MW003-170508


Tot Ion:164 Resp: 1692

Ion Ratio Lower Upper

164 100

162 103.9 84.6 127.0




160 49.7 41.8 62.6



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

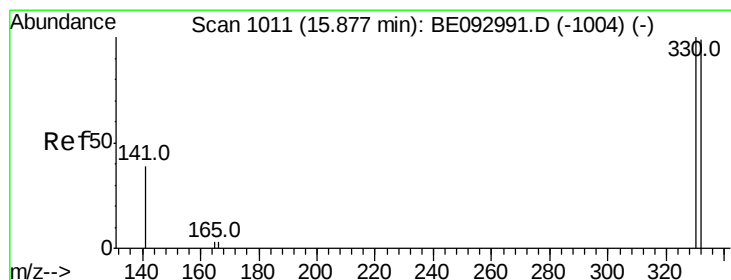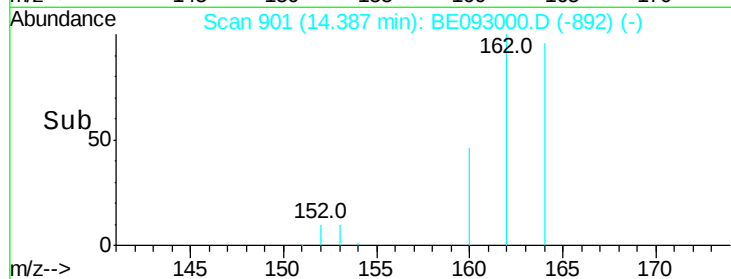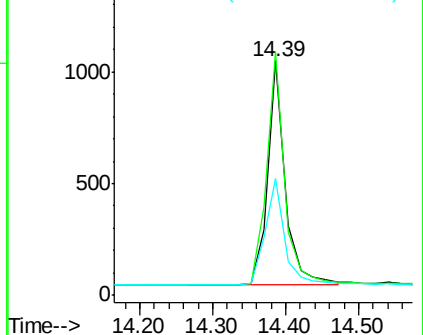

#14

2,4,6-Tribromophenol

Concen: 0.44 ng

RT: 15.87 min Scan# 1010

Delta R.T. -0.01 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32


Tgt Ion:330 Resp: 202

Ion Ratio Lower Upper

330 100

332 97.5 77.7 116.5



141 85.1 56.2 84.4#

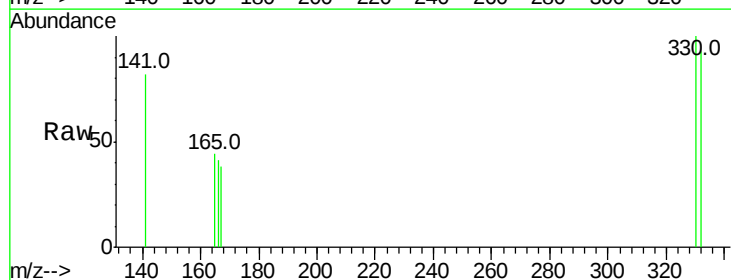


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



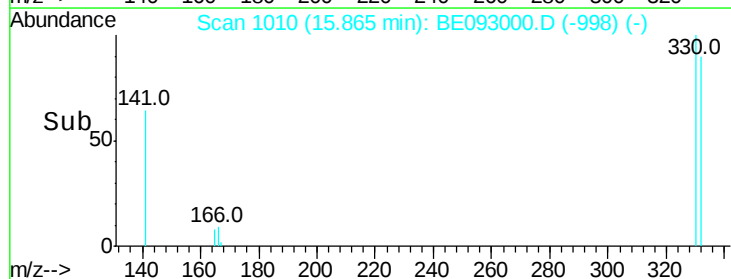
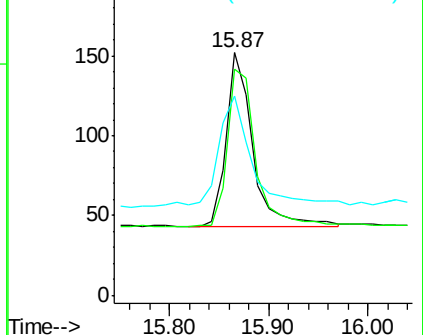


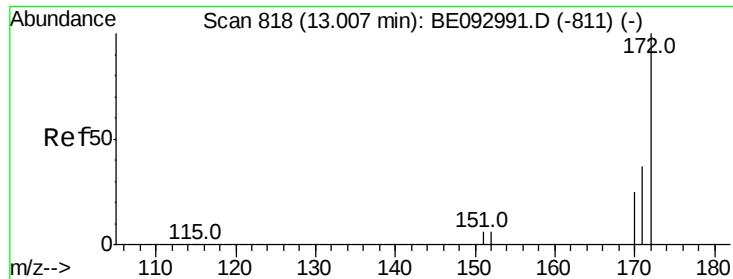

#15
2-Fluorobiphenyl
Concen: 0.52 ng
RT: 13.01 min Scan# 818
Delta R.T. -0.00 min
Lab File: BE093000.D
Acq: 11 May 2017 17:32




Instrument :
BNA_E
ClientSampleId :
LF001MW003-170508


Tot Ion:172 Resp: 3479
Ion Ratio Lower Upper
172 100
171 35.0 29.8 44.6
170 23.5 20.7 31.1

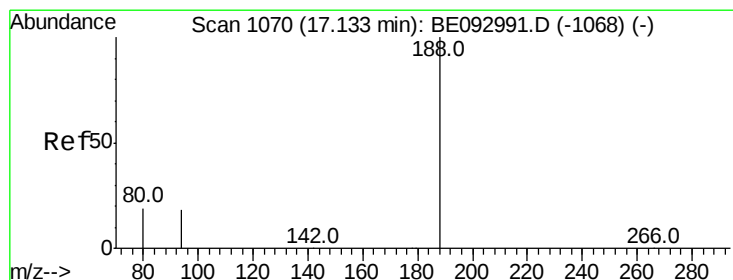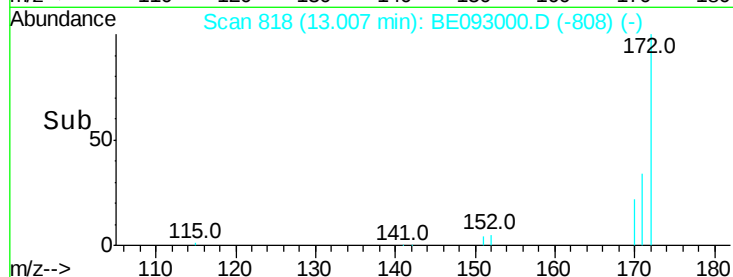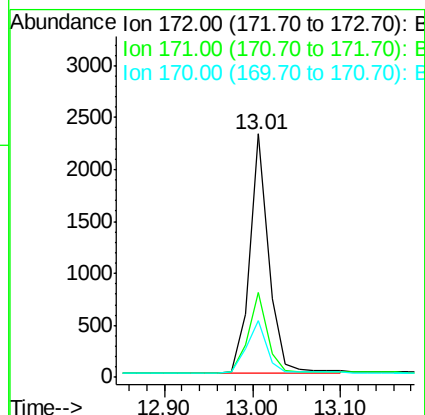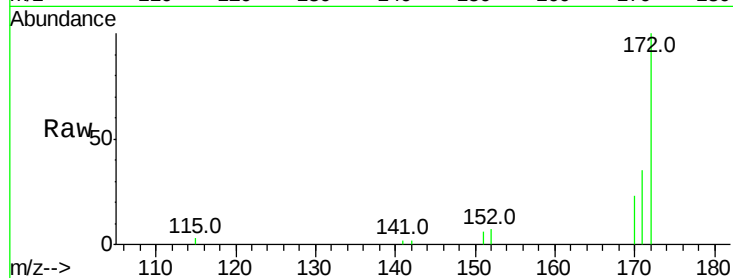

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.13 min Scan# 1069
Delta R.T. -0.00 min
Lab File: BE093000.D
Acq: 11 May 2017 17:32

Tgt Ion:188 Resp: 4935
Ion Ratio Lower Upper
188 100
94 14.4 11.3 16.9
80 14.3 11.7 17.5


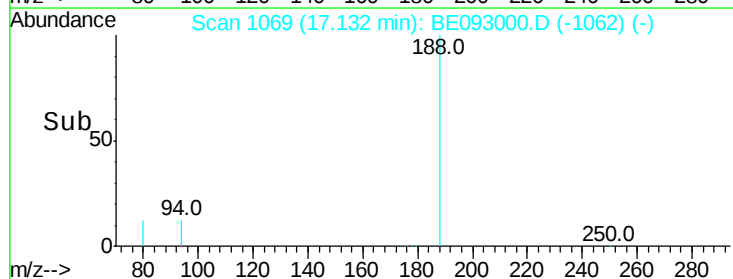
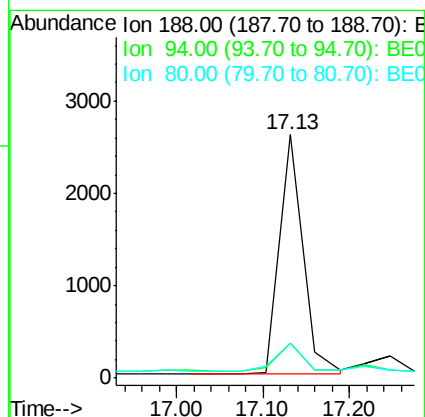
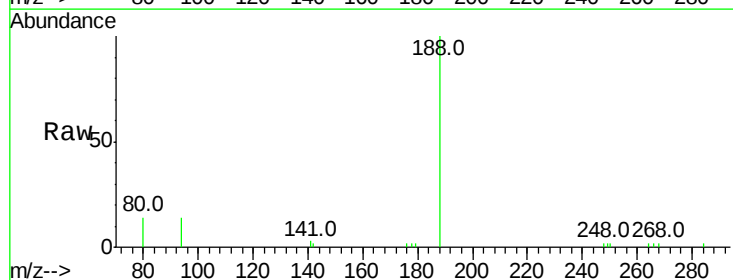


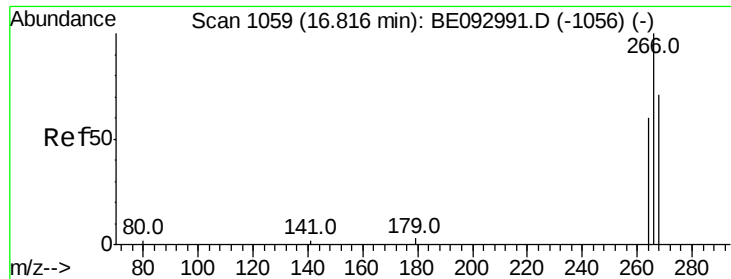

#22
 Pentachlorophenol
 Concen: 0.21 ng
 RT: 16.82 min Scan# 1058
 Delta R.T. 0.00 min
 Lab File: BE093000.D
 Acq: 11 May 2017 17:32




Instrument :
 BNA_E
 ClientSampleId :
 LF001MW003-170508


Tot Ion:266 Resp: 83
 Ion Ratio Lower Upper
 266 100
 264 85.1 58.2 87.2
 268 92.5 71.9 107.9

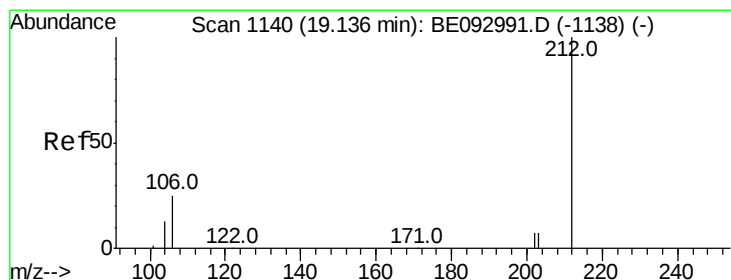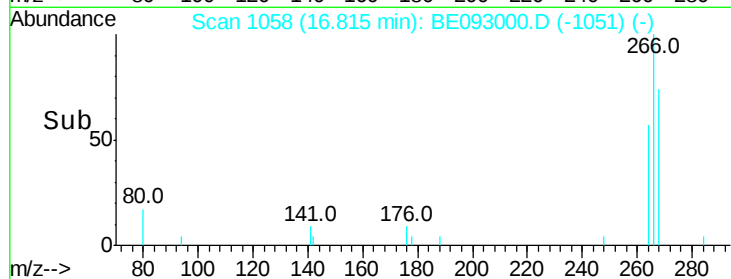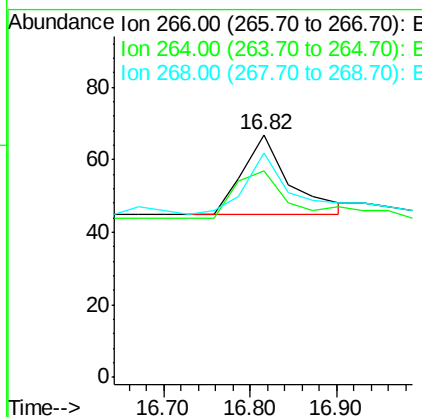

#25
 Fluoranthene-d10
 Concen: 0.38 ng
 RT: 19.14 min Scan# 1139
 Delta R.T. -0.02 min
 Lab File: BE093000.D
 Acq: 11 May 2017 17:32

Tgt Ion:212 Resp: 4916
 Ion Ratio Lower Upper
 212 100
 106 16.8 0.0 0.0#
 104 0.0 0.0 0.0

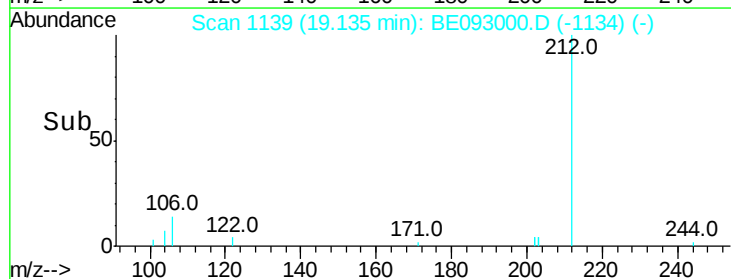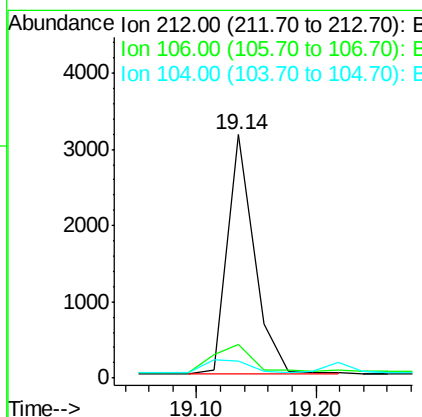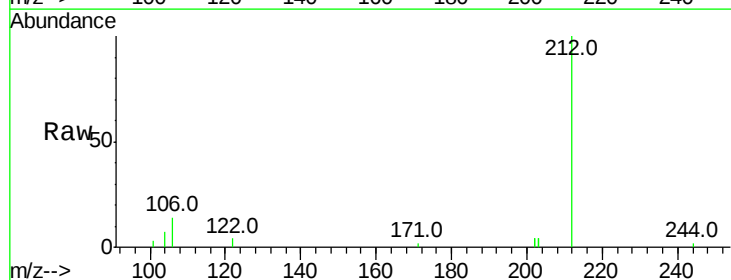

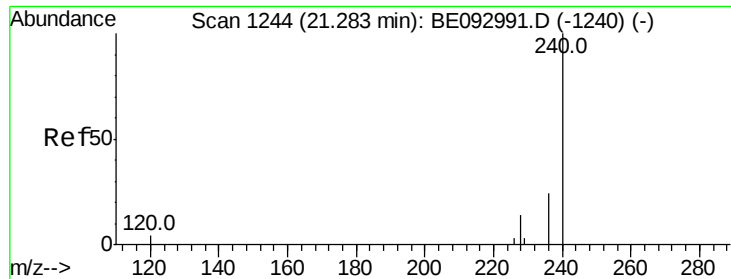

#27

Chrvsene-d12

Concen: 0.40 ng

RT: 21.28 min Scan# 1243

Delta R.T. 0.00 min

Lab File: BE093000.D





Acq: 11 May 2017 17:32

Instrument :
BNA_E

ClientSampleId :
LF001MW003-170508

Tot Ion:240 Resp: 5070

Ion	Ratio	Lower	Upper
240	100		
120	5.4	4.6	7.0
236	23.8	20.8	31.2

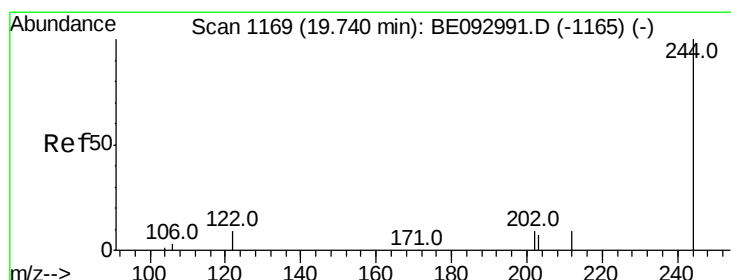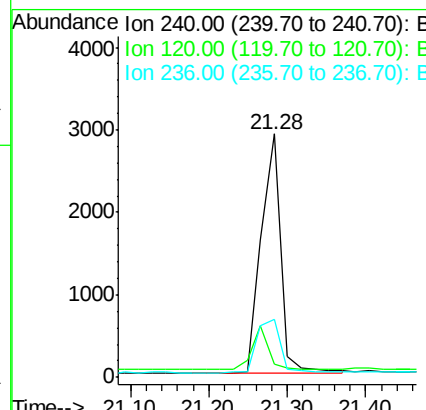

#29

Terphenyl-d14

Concen: 0.74 ng

RT: 19.74 min Scan# 1168




Delta R.T. 0.00 min


Lab File: BE093000.D

Acq: 11 May 2017 17:32

Tgt Ion:244 Resp: 6697

Ion	Ratio	Lower	Upper
244	100		
212	9.0	10.6	16.0#
122	5.2	15.4	23.0#

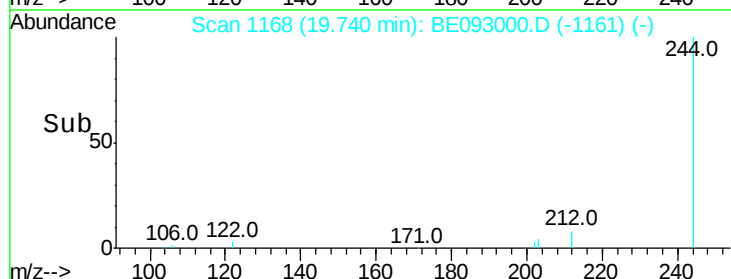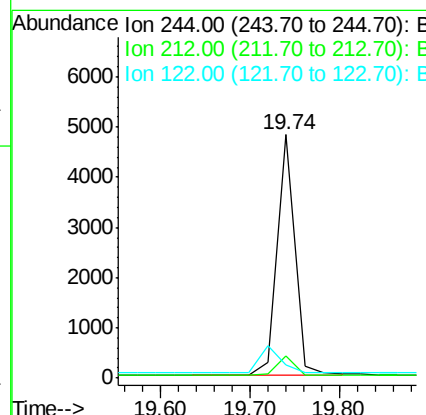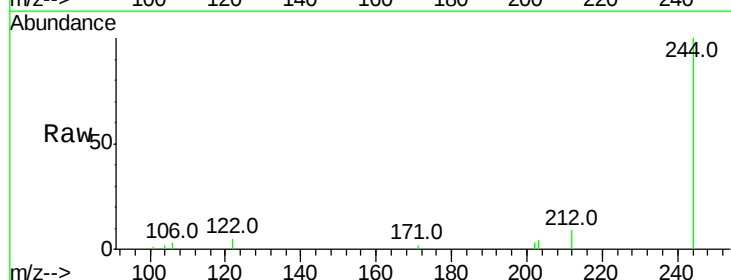



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.16 ng

RT: 21.20 min Scan# 1238

Delta R.T. -0.00 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32

Instrument :

BNA_E

ClientSampleId :

LF001MW003-170508


Tot Ion:149 Resp: 321

Ion Ratio Lower Upper

149 100

167 28.7 20.1 30.1




279 3.4 2.2 3.4#

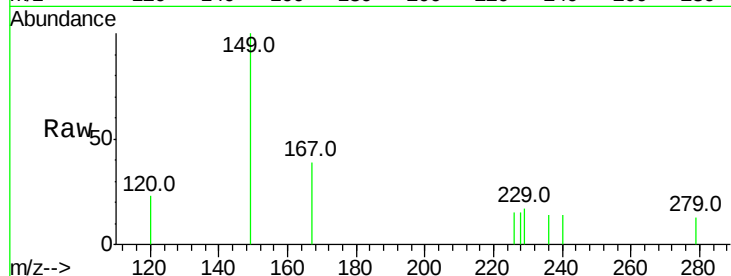

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

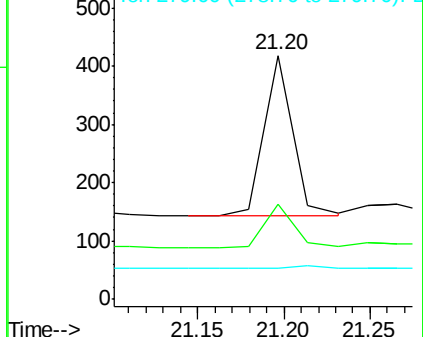

#34

Perylene-d12

Concen: 0.40 ng

RT: 23.69 min Scan# 1414

Delta R.T. -0.01 min

Lab File: BE093000.D

Acq: 11 May 2017 17:32


Tgt Ion:264 Resp: 4137

Ion Ratio Lower Upper

264 100

260 28.1 21.0 31.4

265 27.4 24.6 36.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

