


Data Path : Z:\HPCHEM1\BNA E\DATA\BE051117\
 Data File : BE092988.D
 Acq On : 11 May 2017 10:05
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 11 14:48:08 2017

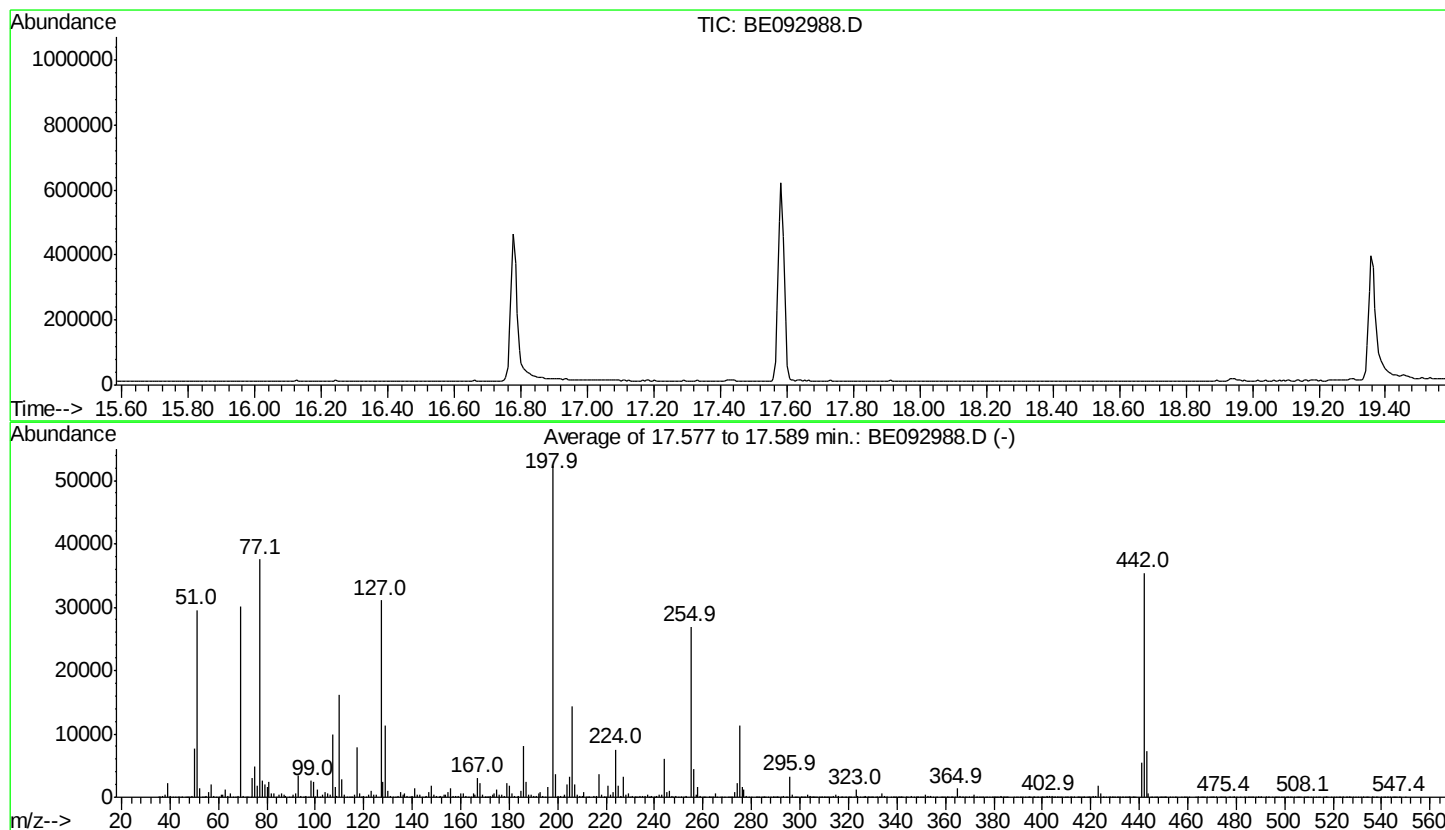

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.5	29567	PASS
68	69	0.00	2	0.8	237	PASS
69	198	0.00	100	57.5	30099	PASS
70	69	0.00	2	0.4	134	PASS
127	198	10	80	59.3	31056	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52345	PASS
199	198	5	9	6.9	3608	PASS
275	198	10	60	21.7	11354	PASS
365	198	1	100	2.6	1373	PASS
441	442	0.01	24	15.5	5497	PASS
442	198	50	100	67.6	35384	PASS
443	442	15	24	20.8	7350	PASS