


Data Path : Z:\HPCHEM1\BNA E\DATA\BE051217\
 Data File : BE093008.D
 Acq On : 12 May 2017 9:00
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 11 14:48:08 2017

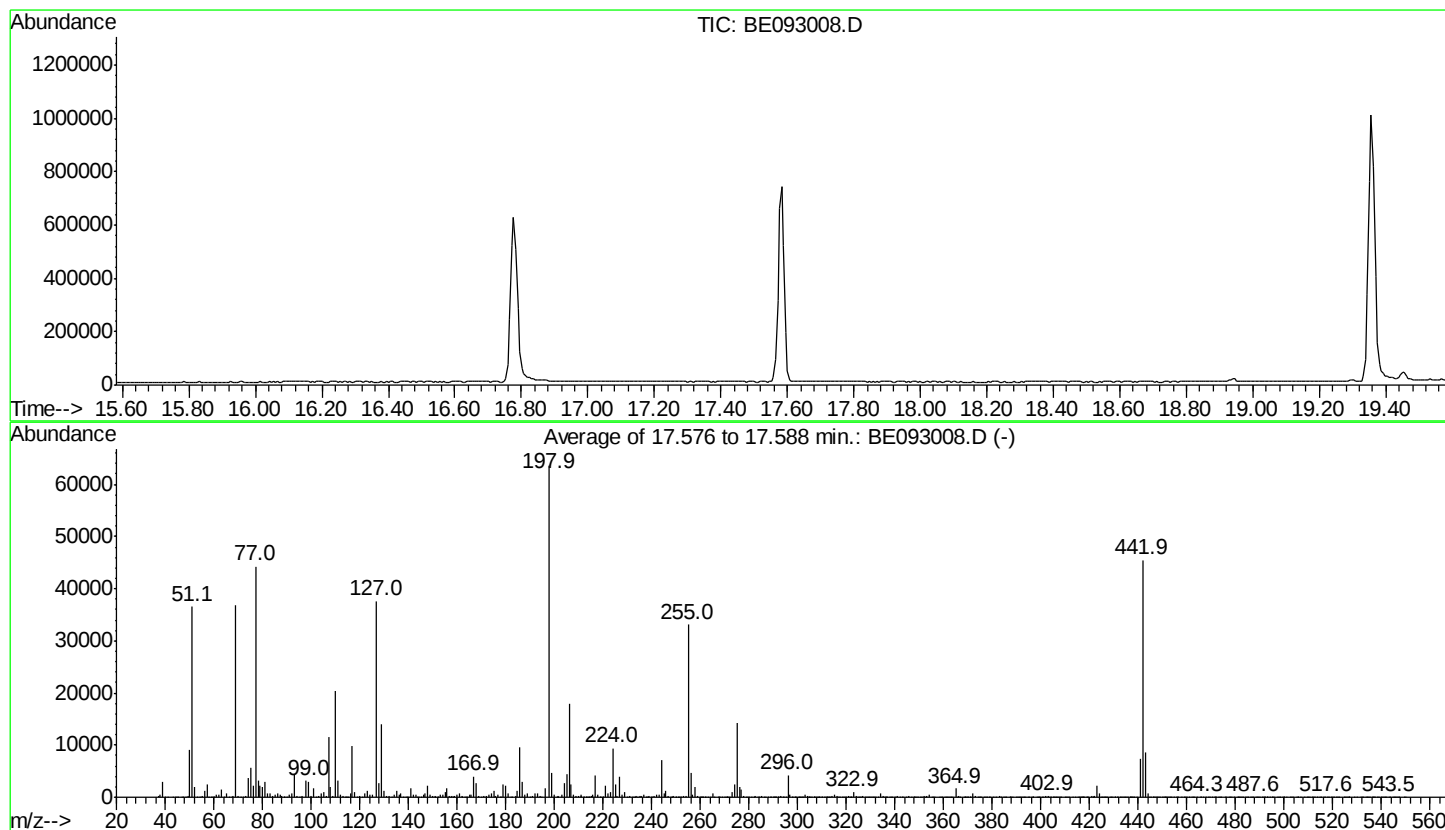

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.5	36573	PASS
68	69	0.00	2	1.0	362	PASS
69	198	0.00	100	57.9	36827	PASS
70	69	0.00	2	0.6	215	PASS
127	198	10	80	59.2	37633	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63595	PASS
199	198	5	9	7.2	4597	PASS
275	198	10	60	22.5	14282	PASS
365	198	1	100	2.7	1694	PASS
441	442	0.01	24	16.0	7268	PASS
442	198	50	100	71.4	45434	PASS
443	442	15	24	19.1	8677	PASS