
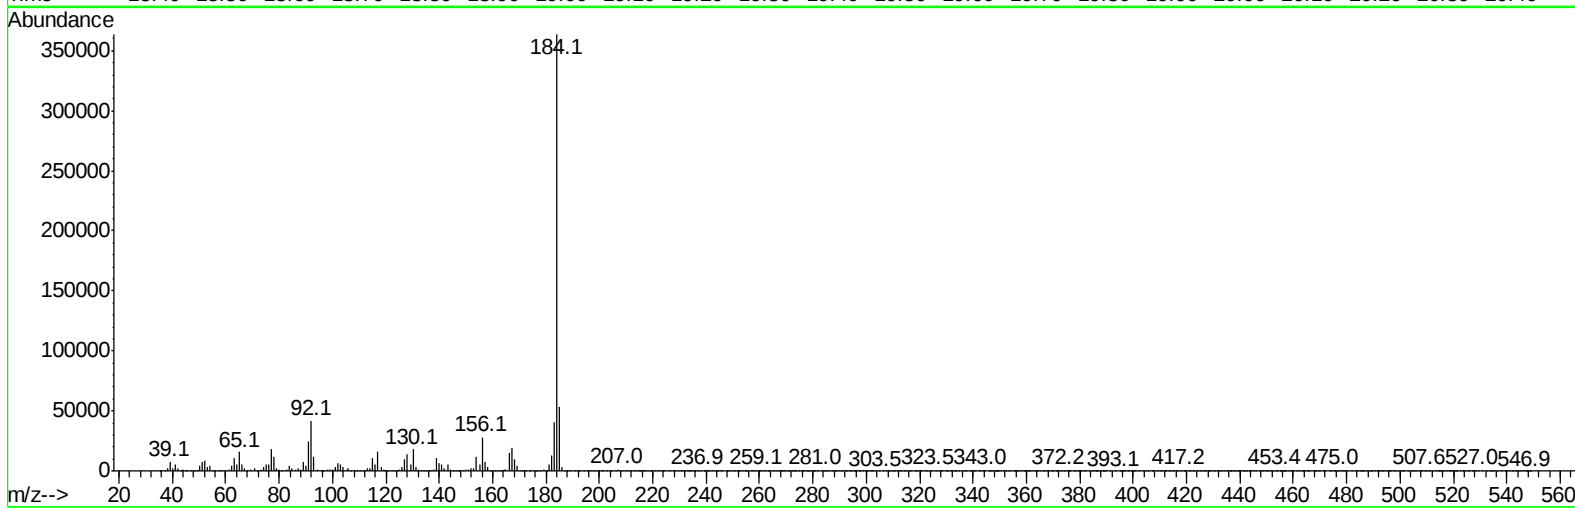


Data Path : Z:\HPCHEM1\BNA E\DATA\BE051517\
Data File : BE093032.D
Acq On : 15 May 2017 13:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 03:48:43 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 19:50:16 2017
Response via : Initial Calibration

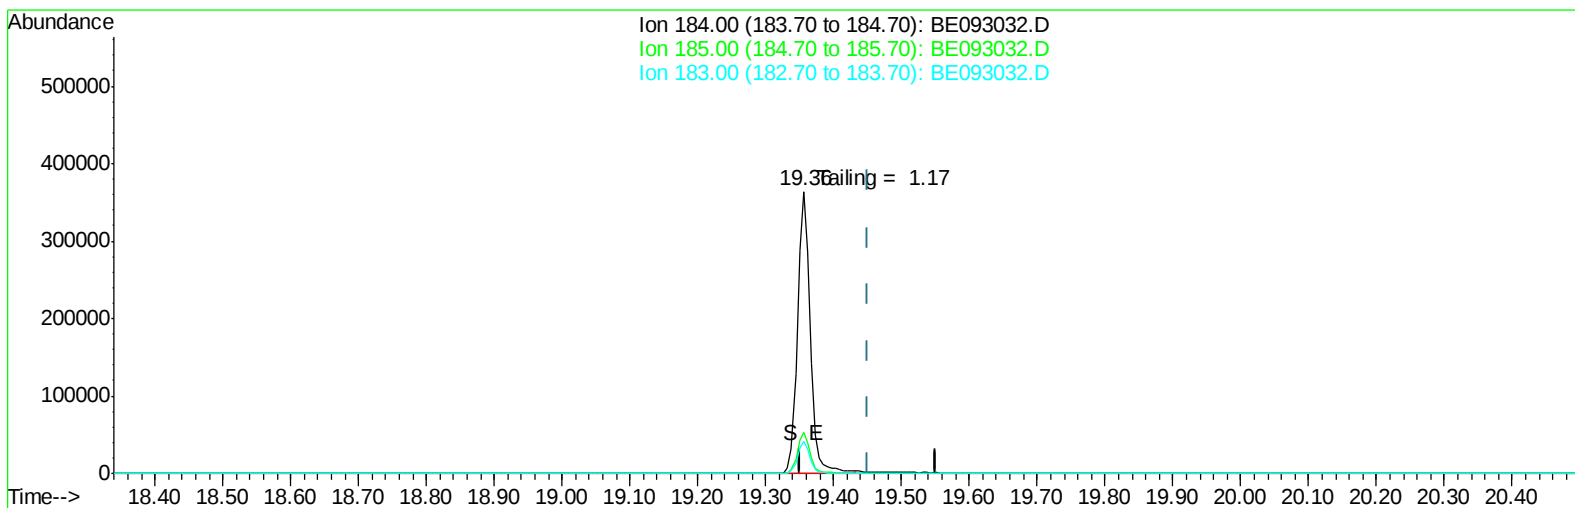

TIC: BE093032.D

(76) Benzidine



19.356min (-0.095) 1427292.11ng

response 463879

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.57
183.00	11.10	11.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE051517\
Data File : BE093032.D
Acq On : 15 May 2017 13:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 03:48:43 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 19:50:16 2017
Response via : Initial Calibration

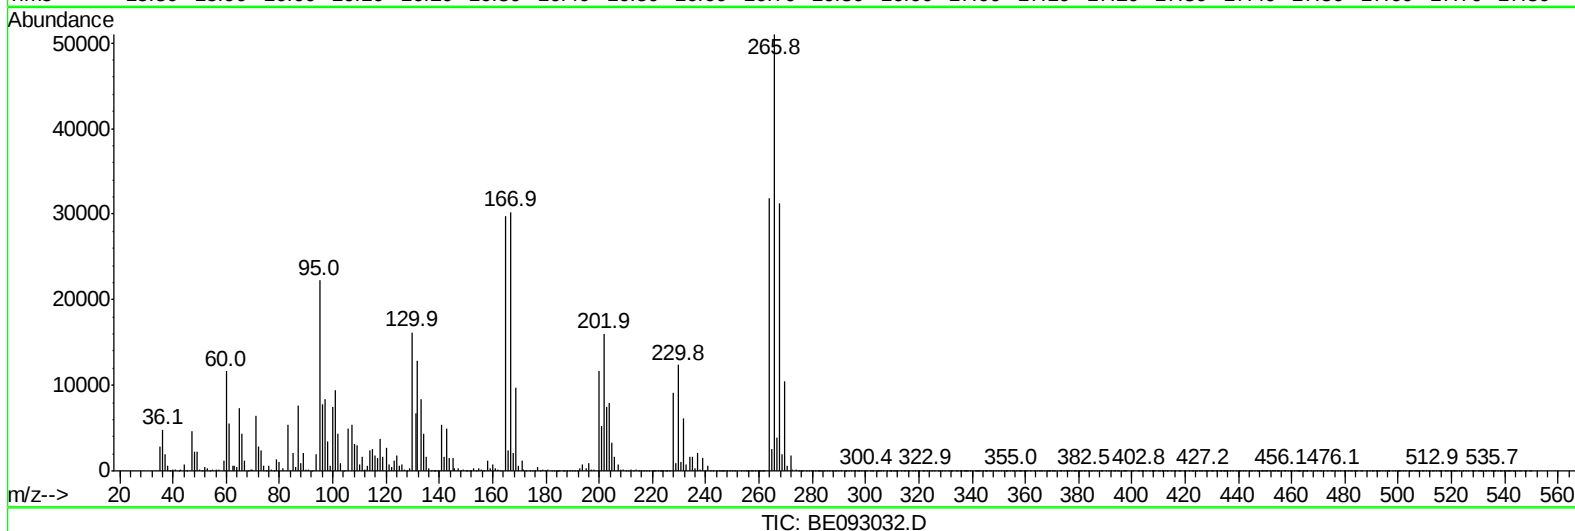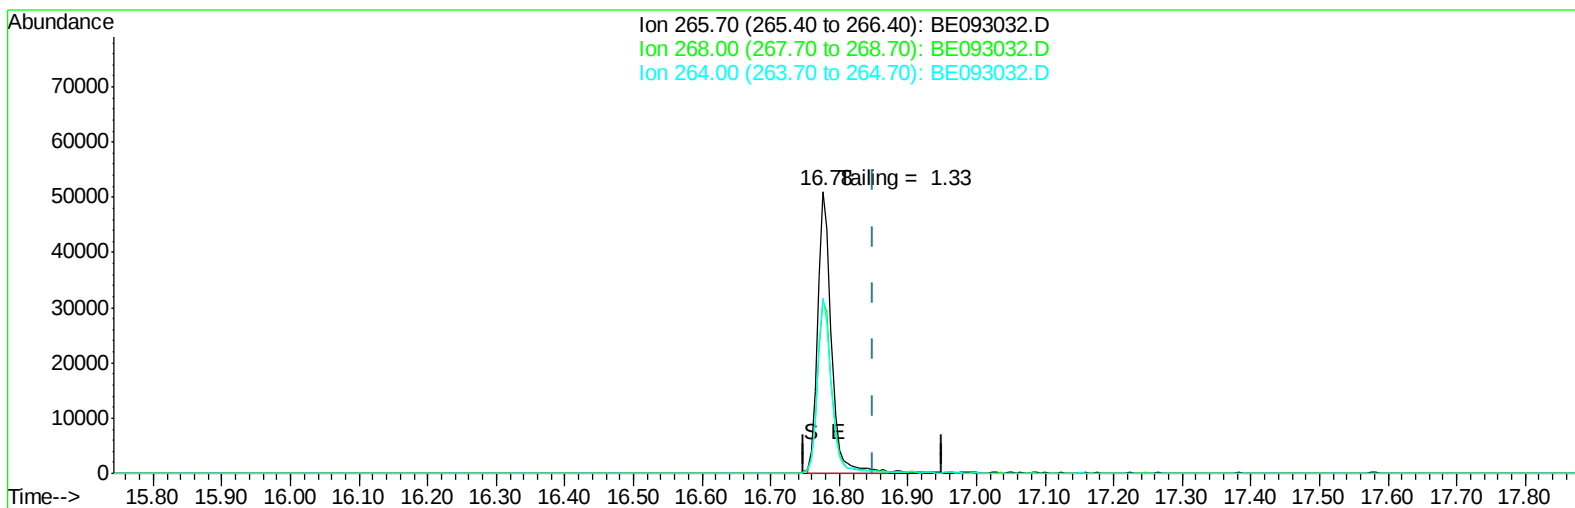

(69) Pentachlorophenol (C)

16.776min (-0.074) 682048.75ng

response 71376

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.35
264.00	61.20	62.38
0.00	0.00	0.00