

Data Path : Z:\HPCHEM1\BNA E\DATA\BE051517\
 Data File : BE093028.D
 Acq On : 15 May 2017 11:03
 Operator : SJ/MA
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.8

Quant Time: May 15 12:10:37 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE051517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 15 12:09:24 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	746	0.40	ng	0.00
7) Naphthalene-d8	10.52	136	3251	0.40	ng	0.00
13) Acenaphthene-d10	14.39	164	1623	0.40	ng	0.00
19) Phenanthrene-d10	17.13	188	4277	0.40	ng	0.00
27) Chrysene-d12	21.28	240	4501	0.40	ng	0.00
34) Perylene-d12	23.69	264	3721	0.40	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.35	112	1881	0.92	ng	0.00
5) Phenol-d6	6.92	99	2571	1.00	ng	0.00
8) Nitrobenzene-d5	8.88	82	2330	0.92	ng	0.00
11) 2-Methylnaphthalene-d10	12.11	152	3971	0.86	ng	0.00
14) 2,4,6-Tribromophenol	15.87	330	413	0.93	ng	-0.01
15) 2-Fluorobiphenyl	13.01	172	5548	0.86	ng	0.00
25) Fluoranthene-d10	19.14	212	9038	0.80	ng	0.00
29) Terphenyl-d14	19.74	244	6857	0.86	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.30	88	1166	0.78	ng	97
3) n-Nitrosodimethylamine	3.61	42	1150	0.90	ng	# 99
6) bis(2-Chloroethyl)ether	7.18	93	2109	0.84	ng	# 99
9) Naphthalene	10.58	128	6993	0.81	ng	97
10) Hexachlorobutadiene	10.87	225	924	0.78	ng	99
12) 2-Methylnaphthalene	12.19	142	4472	0.88	ng	95
16) Acenaphthylene	14.10	152	23375	0.85	ng	100
17) Acenaphthene	14.44	154	4200	0.84	ng	98
18) Fluorene	15.43	166	5205	0.83	ng	99
20) 4-Bromophenyl-phenylether	16.33	248	1075	0.78	ng	# 1
21) Hexachlorobenzene	16.47	284	1450	0.71	ng	# 100
22) Pentachlorophenol	16.82	266	368	0.71	ng	90
23) Phenanthrene	17.19	178	6933	0.68	ng	# 77
24) Anthracene	17.28	178	7244	0.82	ng	98
26) Fluoranthene	19.16	202	43747	0.80	ng	# 59
28) Pyrene	19.53	202	43294	0.77	ng	# 98
30) Benzo(a)anthracene	21.25	228	9760	0.88	ng	# 84
31) Chrysene	21.30	228	10648	0.77	ng	# 83
32) Bis(2-ethylhexyl)phthalate	21.20	149	4574	0.94	ng	98
33) Indeno(1,2,3-cd)pyrene	26.22	276	38975	0.88	ng	99
35) Benzo(b)fluoranthene	22.95	252	9616	0.80	ng	97
36) Benzo(k)fluoranthene	23.00	252	9620	0.80	ng	95
37) Benzo(a)pyrene	23.59	252	8742	0.84	ng	96
38) Dibenzo(a,h)anthracene	26.25	278	8290	0.88	ng	94
39) Benzo(g,h,i)perylene	27.00	276	35582	0.83	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE051517\
Data File : BE093028.D
Acq On : 15 May 2017 11:03
Operator : SJ/MA
Sample : SSTDIC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8

Quant Time: May 15 12:10:37 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE051517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 15 12:09:24 2017
Response via : Initial Calibration

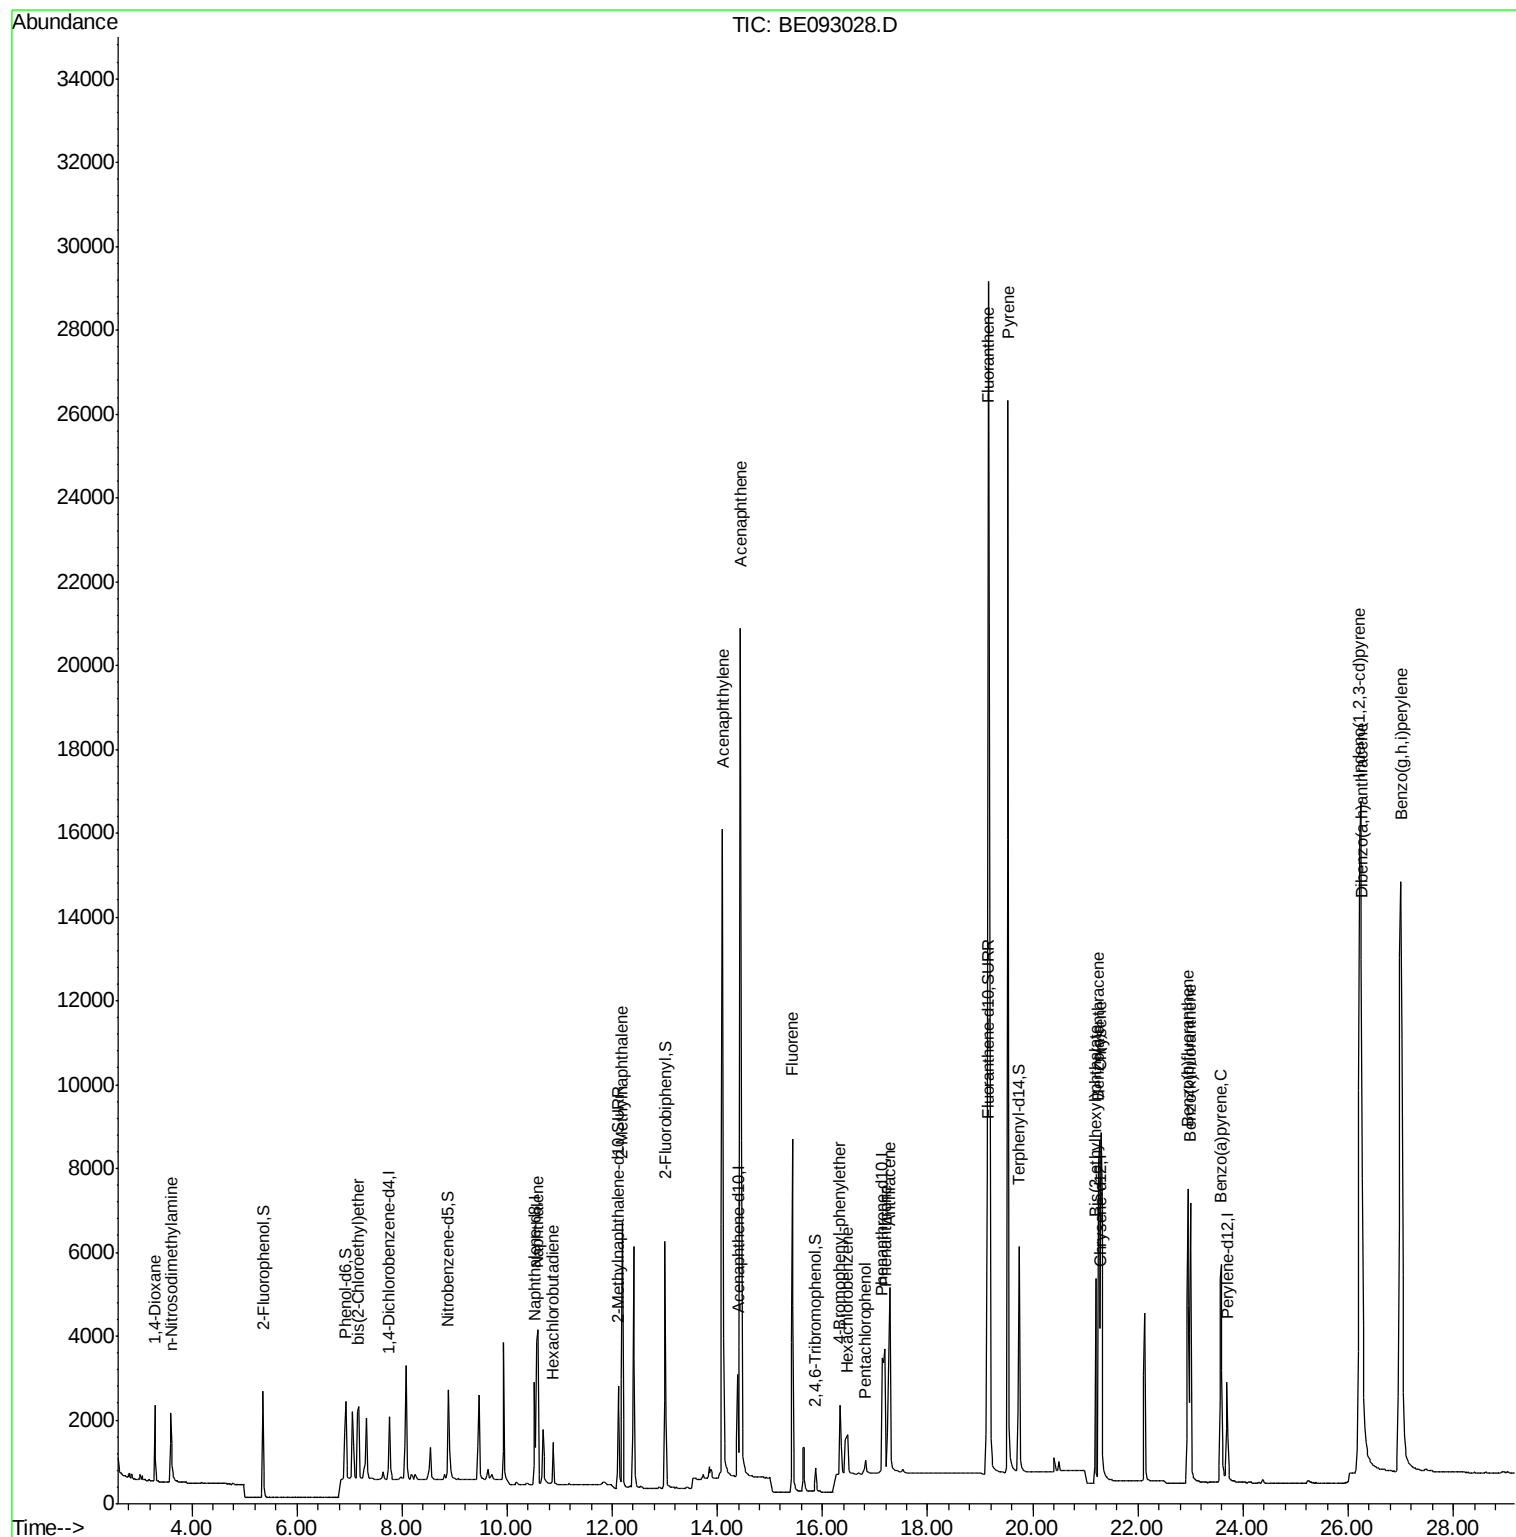

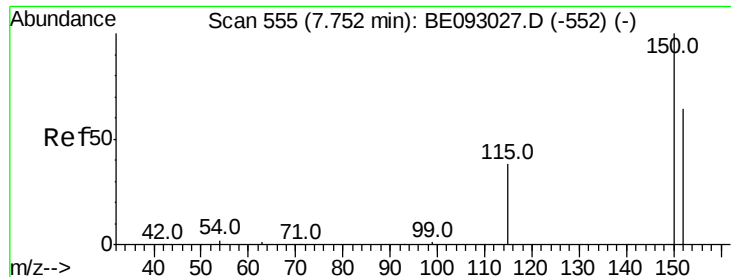

#1

1,4-Dichlorobenzene-d4

Concen: 0.40 ng

RT: 7.75 min Scan# 555

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDICC0.8


Tot Ion:152 Resp: 746

Ion Ratio Lower Upper




152 100

150 152.7 125.1 187.7

115 62.5 55.7 83.5

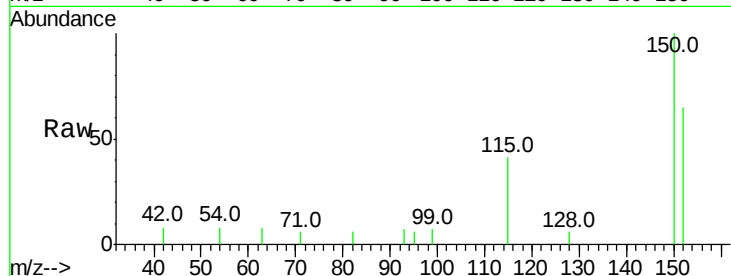

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

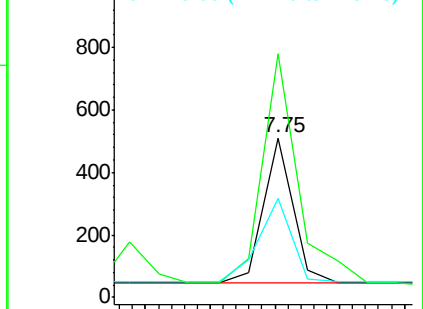

#2

1,4-Dioxane

Concen: 0.78 ng

RT: 3.30 min Scan# 62

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion: 88 Resp: 1166

Ion Ratio Lower Upper



88 100


58 80.0 62.2 93.4

43 31.8 23.2 34.8



Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

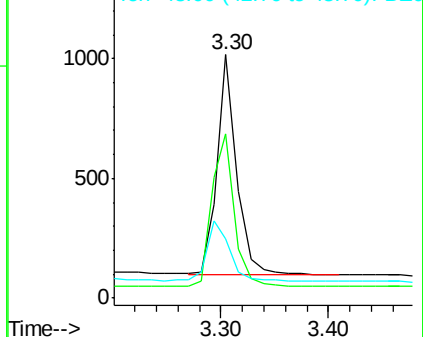



#3

n-Nitrosodimethylamine

Concen: 0.90 ng

RT: 3.61 min Scan# 88

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8


Tot Ion: 42 Resp: 1150

Ion Ratio Lower Upper

42 100

74 123.2 99.1 148.7




44 6.4 7.4 11.2#

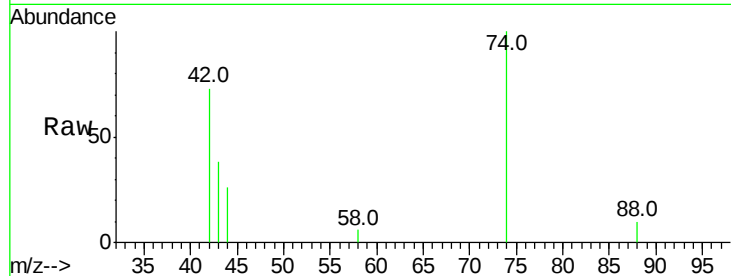

Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

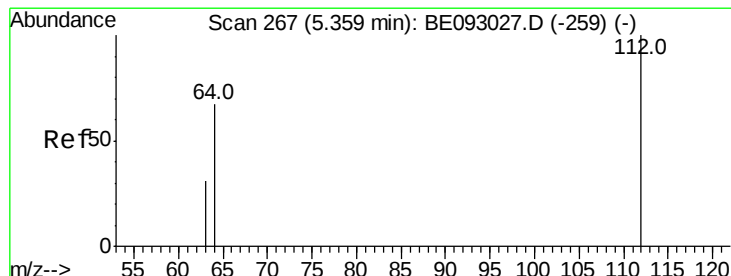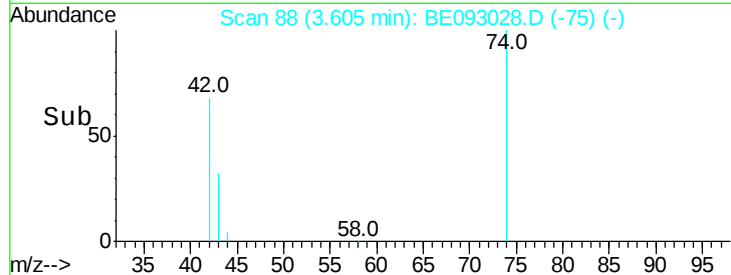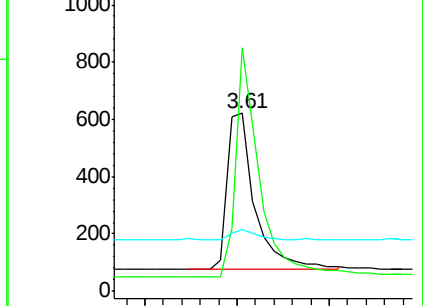

#4

2-Fluorophenol

Concen: 0.92 ng

RT: 5.35 min Scan# 266

Delta R.T. -0.01 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion: 112 Resp: 1881

Ion Ratio Lower Upper

112 100

64 70.6 56.4 84.6



63 35.7 29.3 43.9

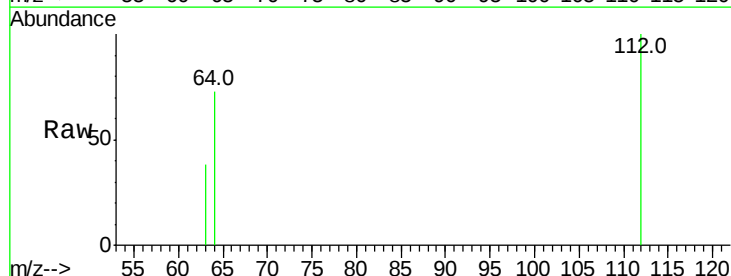


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

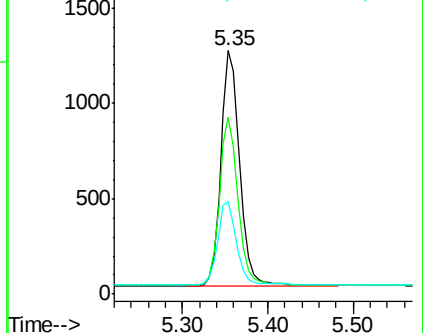

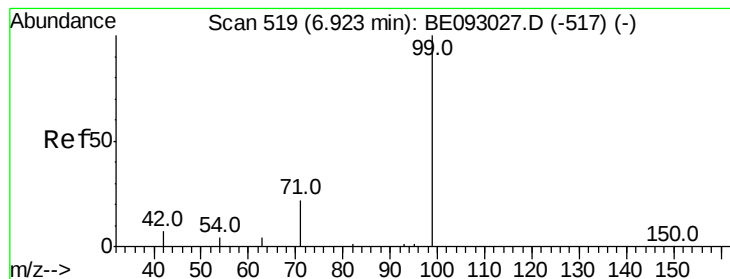

#5

Phenol-d6

Concen: 1.00 ng

RT: 6.92 min Scan# 519

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8


Tot Ion: 99 Resp: 2571

Ion Ratio Lower Upper

99 100

42 0.0 0.0 0.0




71 0.0 0.0 0.0

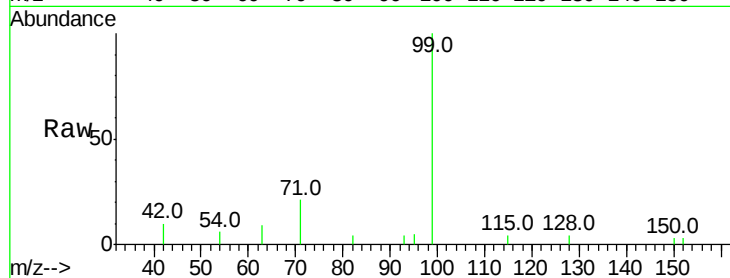

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

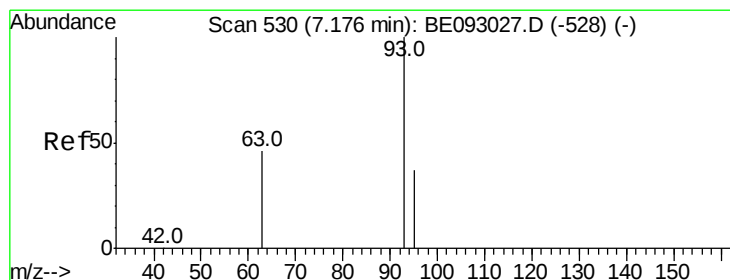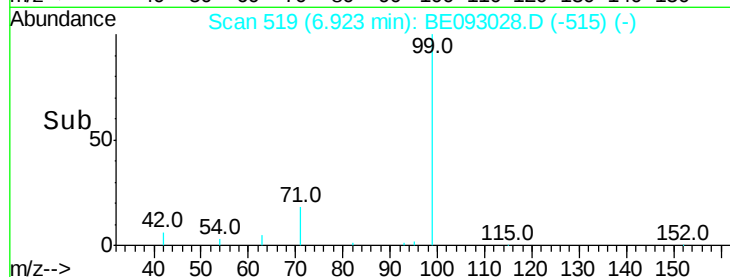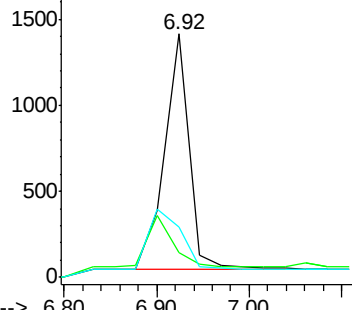

#6

bis(2-Chloroethyl)ether

Concen: 0.84 ng

RT: 7.18 min Scan# 530

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion: 93 Resp: 2109

Ion Ratio Lower Upper

93 100

63 0.0 0.0 0.0



95 32.1 25.4 38.0

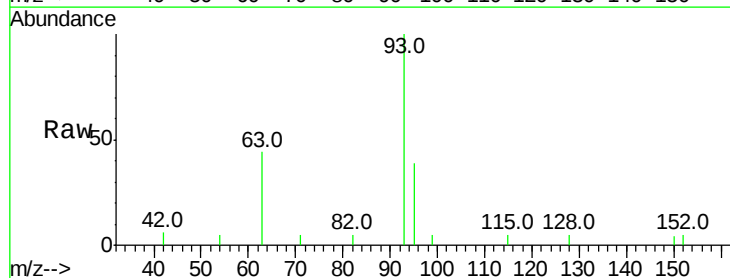


Abundance Ion 93.00 (92.70 to 93.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Ion 95.00 (94.70 to 95.70): BE0

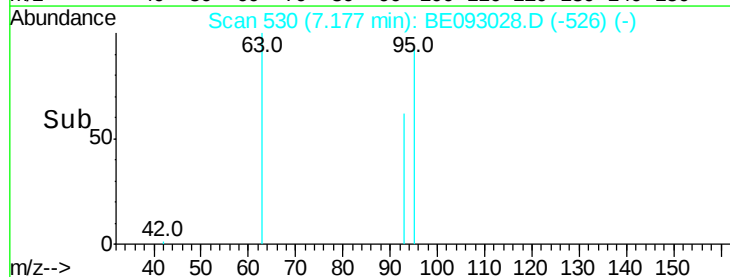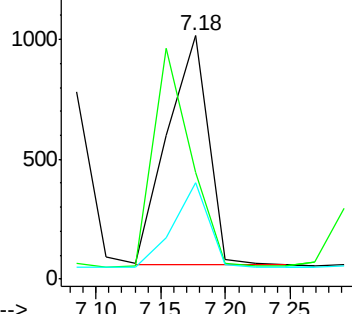



#7

Naphthalene-d8

Concen: 0.40 ng

RT: 10.52 min Scan# 678

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8

Tot Ion:136 Resp: 3251


Ion Ratio Lower Upper

136 100

137 12.4 9.8 14.8

54 11.1 10.3 15.5

68 10.1 9.0 13.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

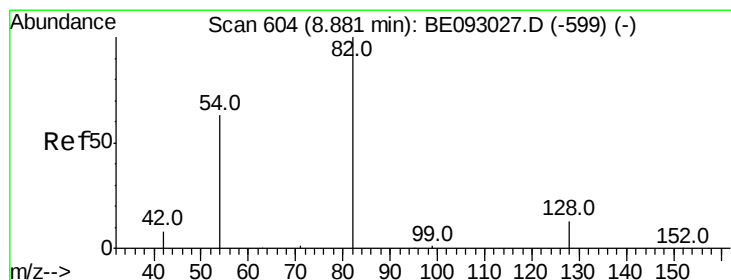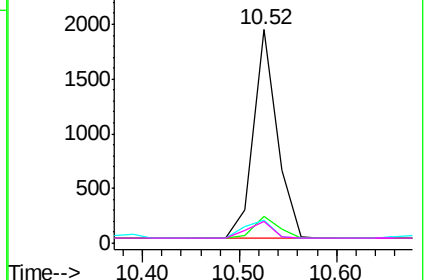

#8

Nitrobenzene-d5

Concen: 0.92 ng

RT: 8.88 min Scan# 604

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion: 82 Resp: 2330

Ion Ratio Lower Upper

82 100

128 18.0 17.0 25.4



54 60.0 53.8 80.6




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

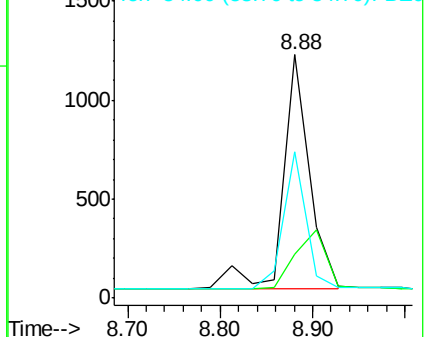



#9

Naphthalene

Concen: 0.81 ng

RT: 10.58 min Scan# 681

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8





Tot Ion:128 Resp: 6993

Ion Ratio Lower Upper

128 100

129 13.3 11.4 17.0

127 12.4 11.2 16.8

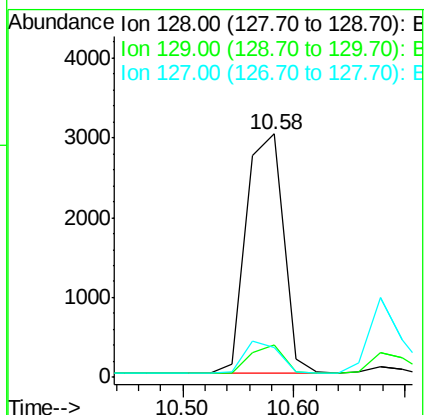

#10

Hexachlorobutadiene

Concen: 0.78 ng

RT: 10.87 min Scan# 696

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03




Tgt Ion:225 Resp: 924

Ion Ratio Lower Upper

225 100

223 63.1 49.7 74.5

227 63.3 50.3 75.5

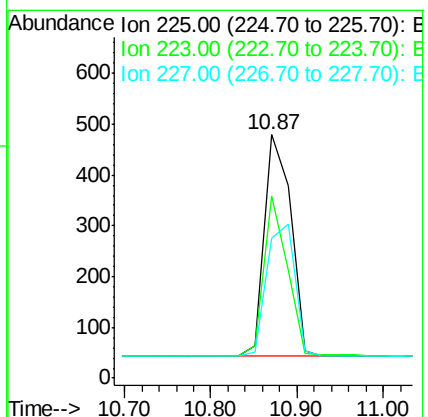



#11

2-Methylnaphthalene-d10

Concen: 0.86 ng

RT: 12.11 min Scan# 760

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :


SSTDIC0.8

Tot Ion:152 Resp: 3971

Ion Ratio Lower Upper

152 100

151 19.1 15.1 22.7

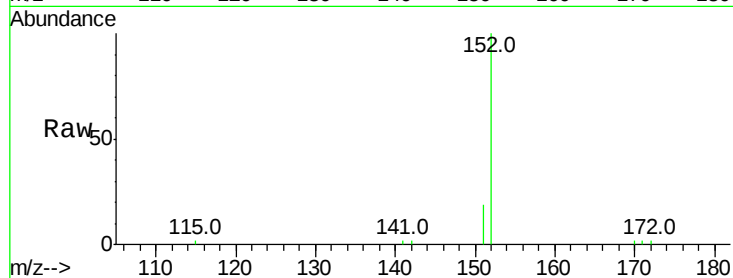

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

12.11

2500

2000



1500

1000

500

0

Time-->

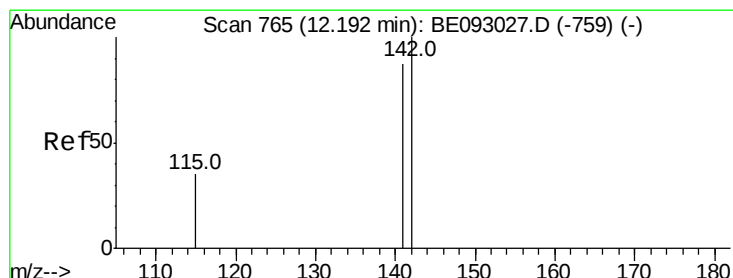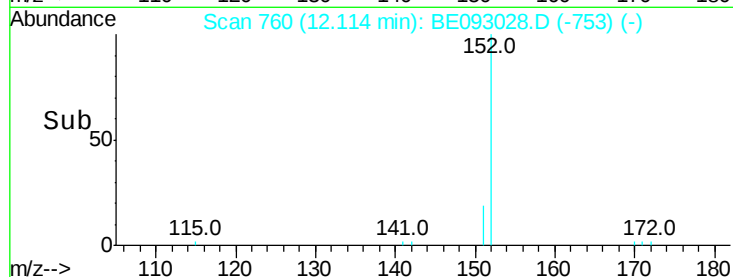

#12

2-Methylnaphthalene

Concen: 0.88 ng

RT: 12.19 min Scan# 765

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion:142 Resp: 4472

Ion Ratio Lower Upper

142 100

141 86.7 72.6 108.8

115 36.1 32.2 48.2

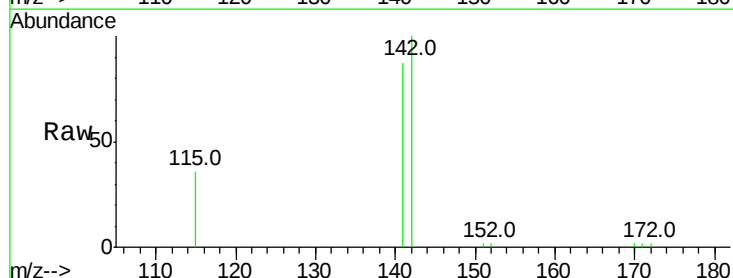

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

4000


3000

2000

1000

0

Time-->




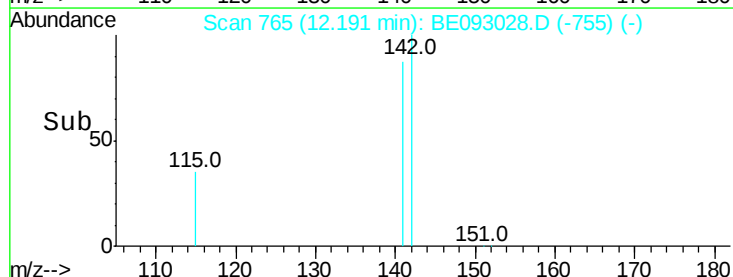




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.39 min Scan# 901
Delta R.T. 0.00 min
Lab File: BE093028.D
Acq: 15 May 2017 11:03




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tot Ion:164 Resp: 1623
Ion Ratio Lower Upper
164 100
162 99.7 84.6 127.0
160 46.4 41.8 62.6

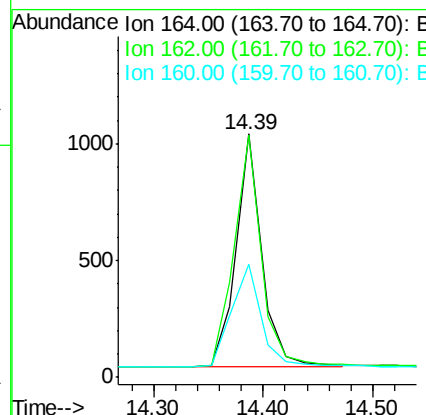

#14
2,4,6-Tribromophenol
Concen: 0.93 ng
RT: 15.87 min Scan# 1010
Delta R.T. -0.01 min
Lab File: BE093028.D
Acq: 15 May 2017 11:03

Tgt Ion:330 Resp: 413
Ion Ratio Lower Upper
330 100
332 93.9 77.7 116.5
141 55.4 56.2 84.4#



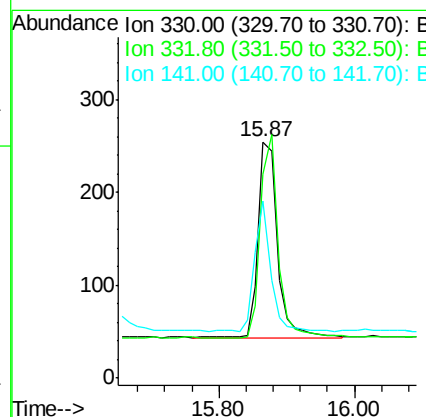



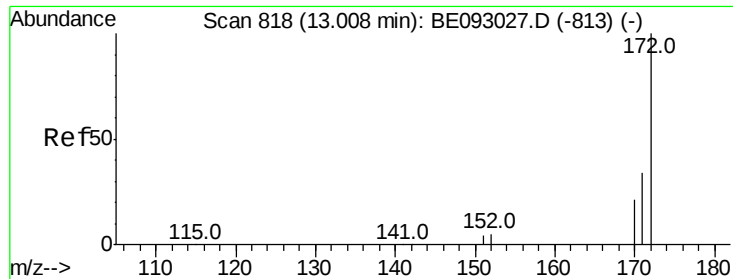

#15
2-Fluorobiphenyl
Concen: 0.86 ng
RT: 13.01 min Scan# 818
Delta R.T. -0.00 min
Lab File: BE093028.D
Acq: 15 May 2017 11:03




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8

Tot Ion:172 Resp: 5548
Ion Ratio Lower Upper
172 100
171 34.6 29.8 44.6
170 22.7 20.7 31.1

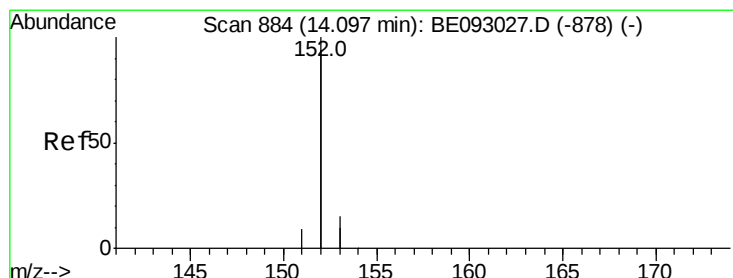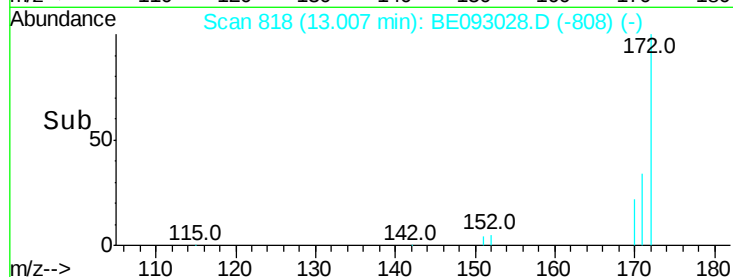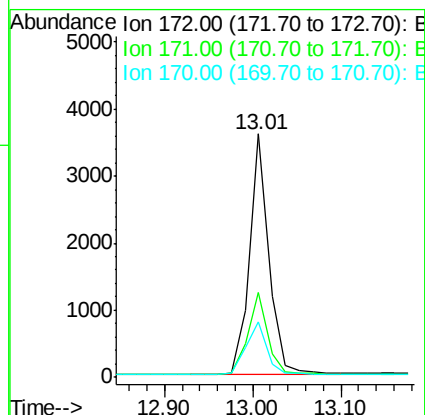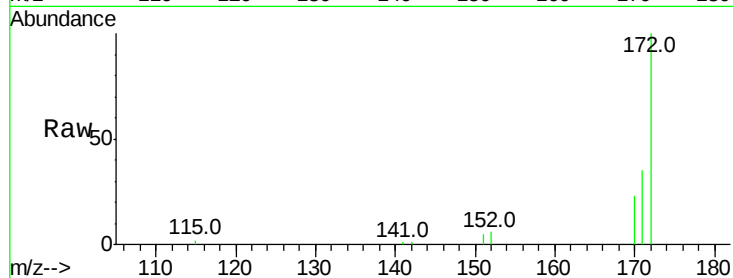

#16
Acenaphthylene
Concen: 0.85 ng
RT: 14.10 min Scan# 884
Delta R.T. 0.00 min
Lab File: BE093028.D
Acq: 15 May 2017 11:03

Tgt Ion:152 Resp: 23375
Ion Ratio Lower Upper
152 100
151 4.9 4.0 6.0
153 13.1 10.3 15.5


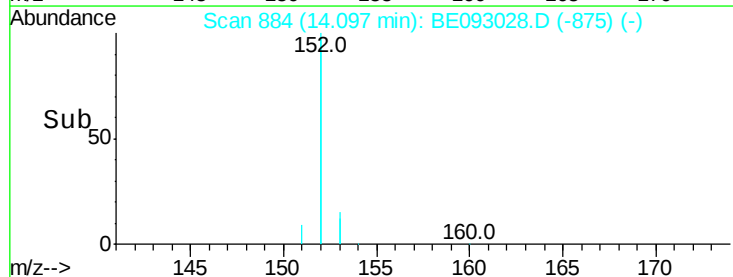
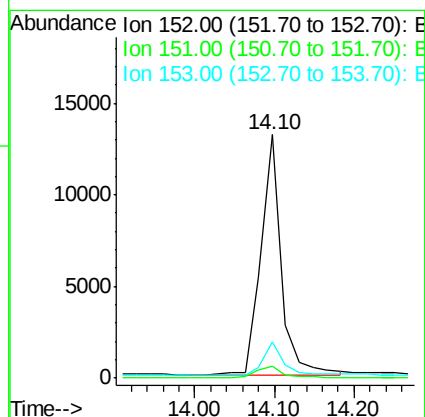
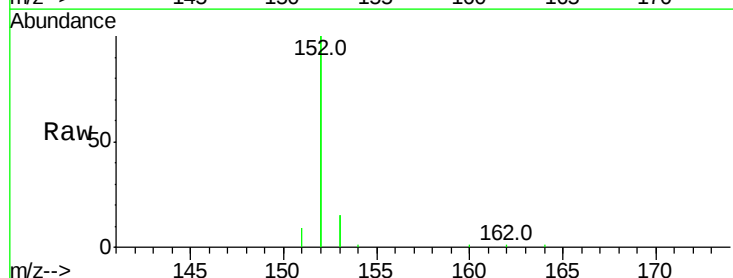




#17
Acenaphthene
Concen: 0.84 ng
RT: 14.44 min Scan# 904
Delta R.T. 0.00 min
Lab File: BE093028.D
Acq: 15 May 2017 11:03




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tot Ion:154 Resp: 4200
Ion Ratio Lower Upper
154 100
153 460.9 367.8 551.6
152 228.3 188.2 282.2

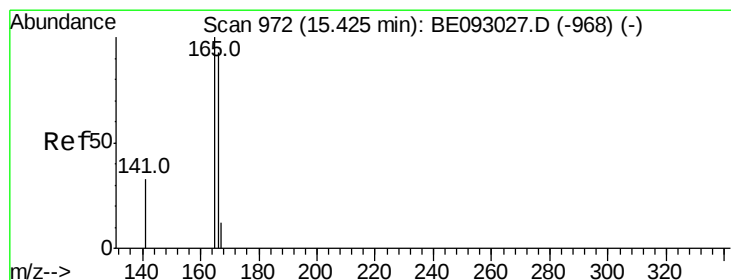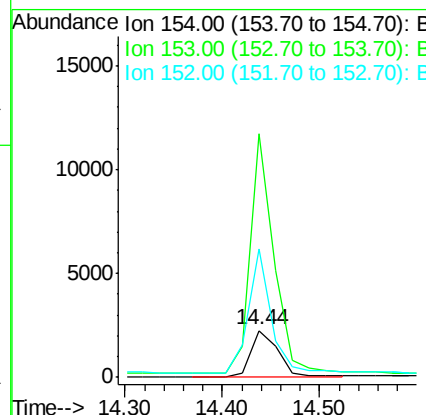

#18
Fluorene
Concen: 0.83 ng
RT: 15.43 min Scan# 972
Delta R.T. 0.00 min
Lab File: BE093028.D
Acq: 15 May 2017 11:03

Tgt Ion:166 Resp: 5205
Ion Ratio Lower Upper
166 100
165 99.2 78.6 117.8
167 14.2 11.1 16.7

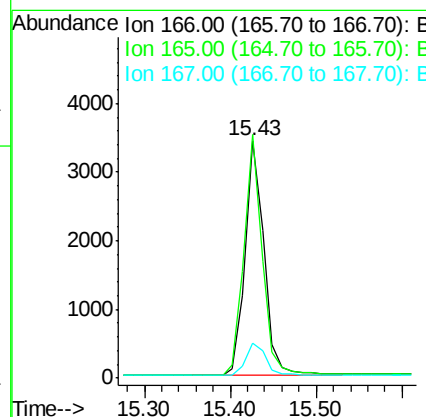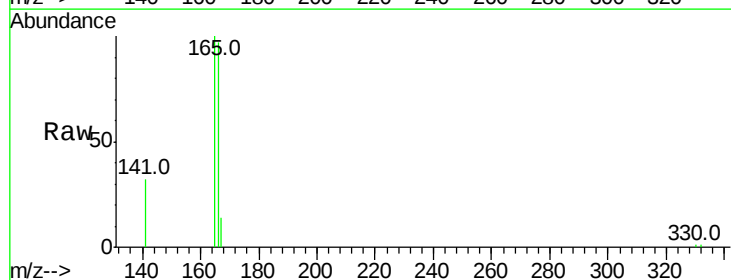



#19

Phenanthrene-d10

Concen: 0.40 ng

RT: 17.13 min Scan# 1069

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8


Tot Ion:188 Resp: 4277

Ion Ratio Lower Upper

188 100

94 14.5 11.3 16.9




80 14.6 11.7 17.5



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

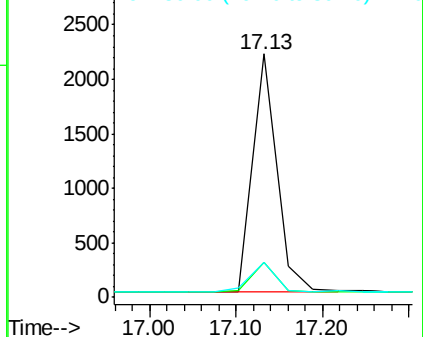

#20

4-Bromophenyl-phenylether

Concen: 0.78 ng

RT: 16.33 min Scan# 1041

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion:248 Resp: 1075

Ion Ratio Lower Upper

248 100

250 55.9 100.0 150.0#



141 210.7 40.0 60.0#



Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

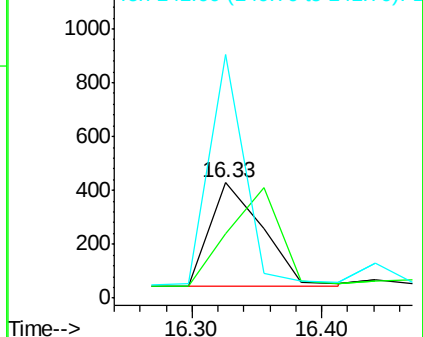



#21

Hexachlorobenzene

Concen: 0.71 ng

RT: 16.47 min Scan# 1046

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8


Tot Ion:284 Resp: 1450

Ion Ratio Lower Upper

284 100

142 0.0 0.0 0.0




249 0.0 0.0 0.0

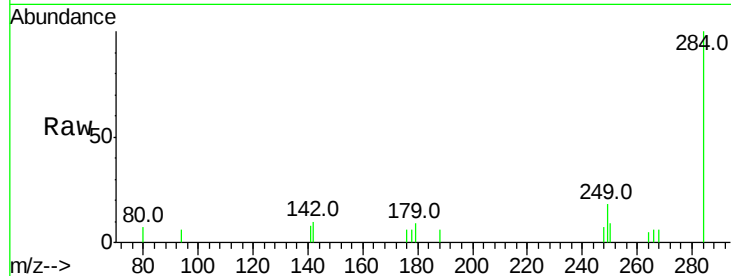

Abundance Ion 283.80 (283.50 to 284.50): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

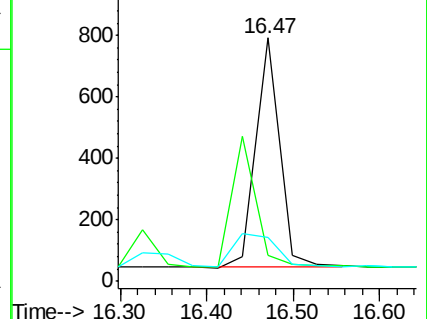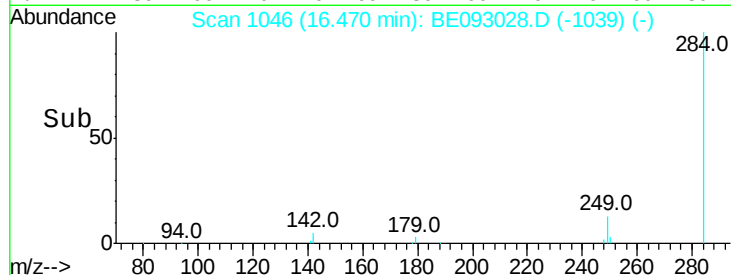

#22

Pentachlorophenol

Concen: 0.71 ng

RT: 16.82 min Scan# 1058

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion:266 Resp: 368

Ion Ratio Lower Upper

266 100

264 64.6 58.2 87.2



268 80.3 71.9 107.9




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

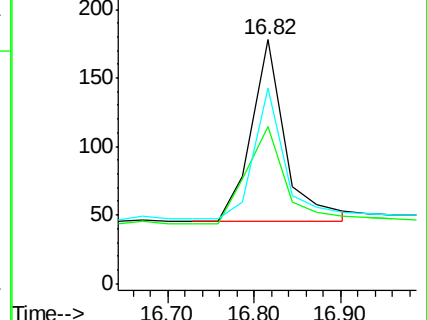

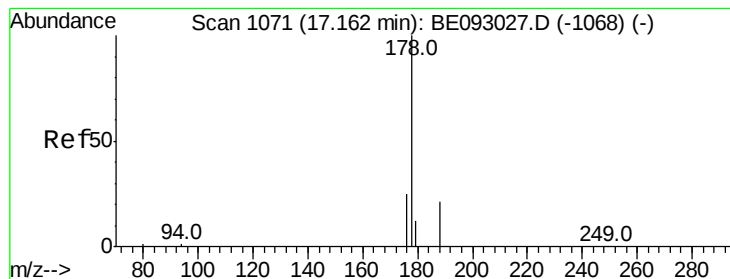

#23

Phenanthrene

Concen: 0.68 ng

RT: 17.19 min Scan# 1071

Delta R.T. 0.03 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8


Tot Ion:178 Resp: 6933

Ion Ratio Lower Upper

178 100

176 0.0 15.0 22.4#




179 16.2 12.7 19.1

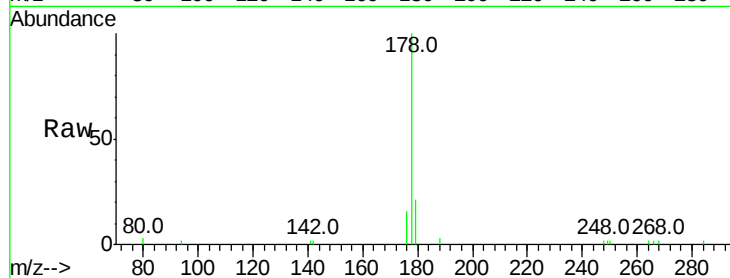

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

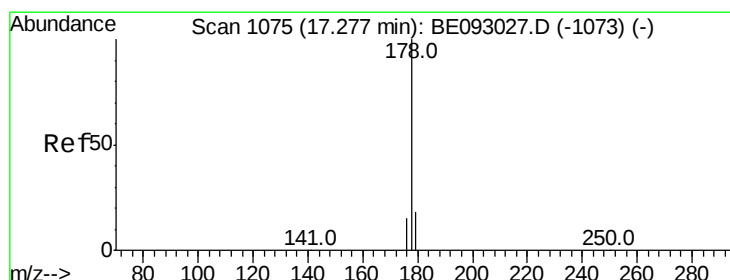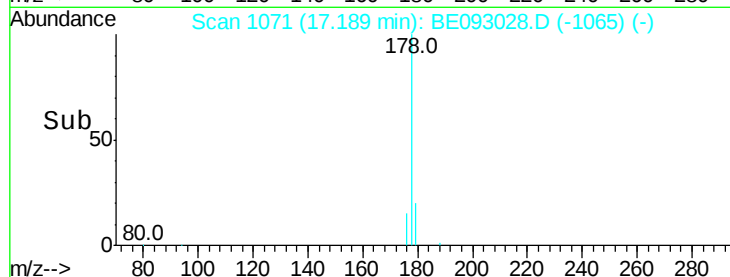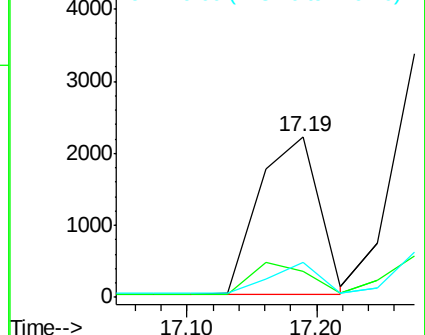

#24

Anthracene

Concen: 0.82 ng

RT: 17.28 min Scan# 1074

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion:178 Resp: 7244

Ion Ratio Lower Upper

178 100

176 17.8 14.6 22.0



179 16.2 12.0 18.0

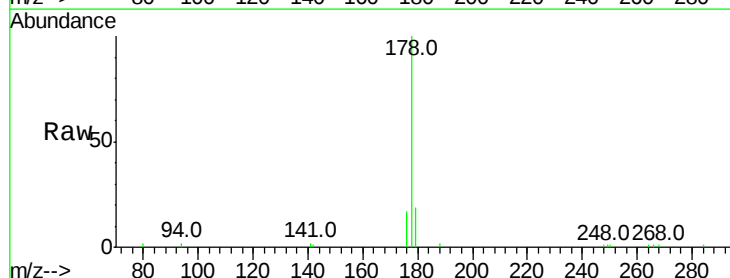


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E



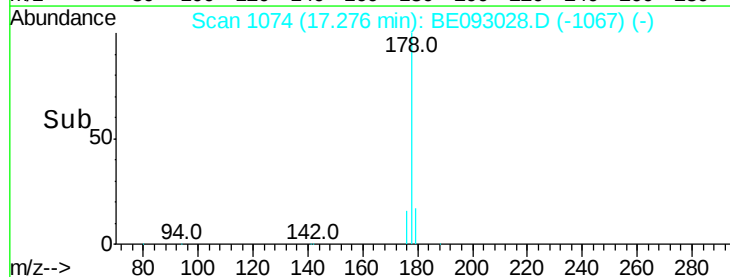
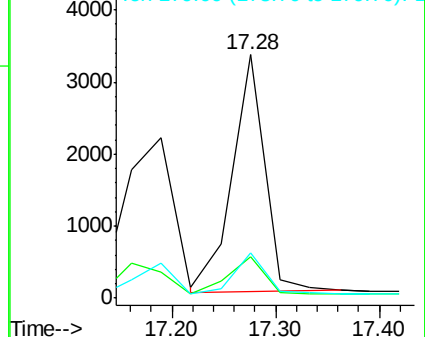




#25
 Fluoranthene-d10
 Concen: 0.80 ng
 RT: 19.14 min Scan# 1139
 Delta R.T. 0.00 min
 Lab File: BE093028.D
 Acq: 15 May 2017 11:03




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.8


Tot Ion:212 Resp: 9038
 Ion Ratio Lower Upper
 212 100
 106 15.5 0.0 0.0#
 104 0.0 0.0 0.0

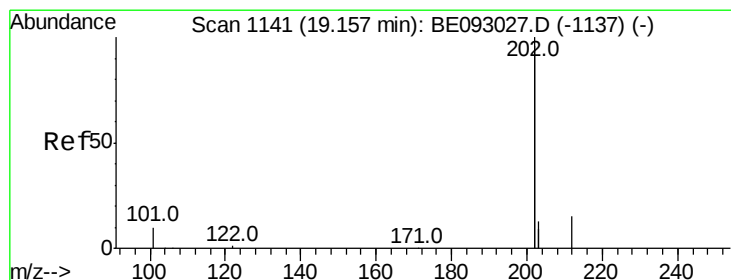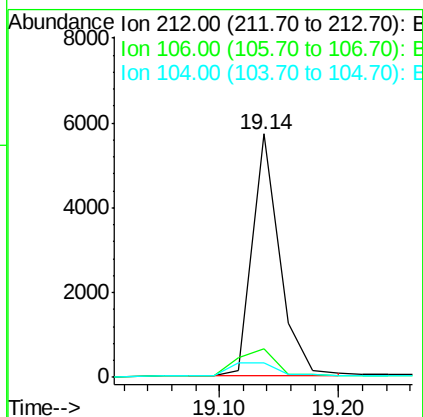

#26
 Fluoranthene
 Concen: 0.80 ng
 RT: 19.16 min Scan# 1140
 Delta R.T. 0.00 min
 Lab File: BE093028.D
 Acq: 15 May 2017 11:03

Tgt Ion:202 Resp: 43747
 Ion Ratio Lower Upper
 202 100
 101 3.4 0.0 0.0#
 203 0.0 14.4 21.6#

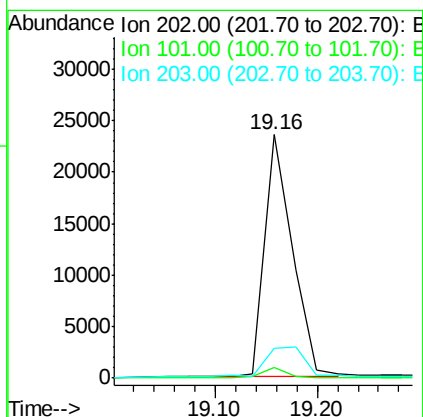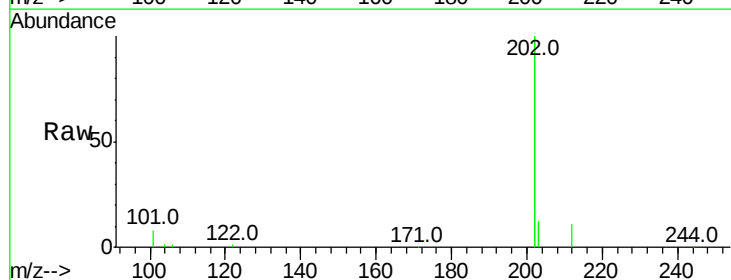



#27

Chrysene-d12

Concen: 0.40 ng

RT: 21.28 min Scan# 1243

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8


Tot Ion:240 Resp: 4501

Ion Ratio Lower Upper

240 100

120 4.3 4.6 7.0#




236 23.3 20.8 31.2



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

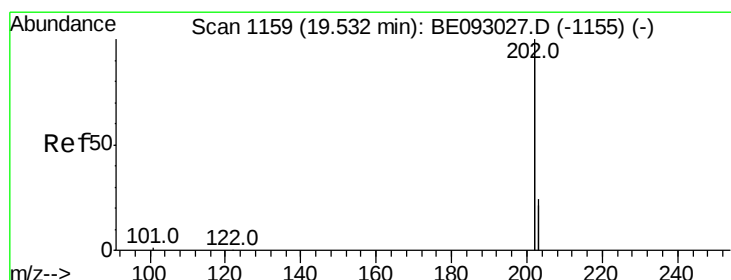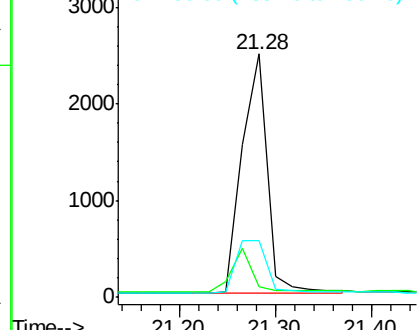

#28

Pyrene

Concen: 0.77 ng

RT: 19.53 min Scan# 1158

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion:202 Resp: 43294

Ion Ratio Lower Upper

202 100

200 0.0 0.0 0.0



203 18.1 13.7 20.5




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

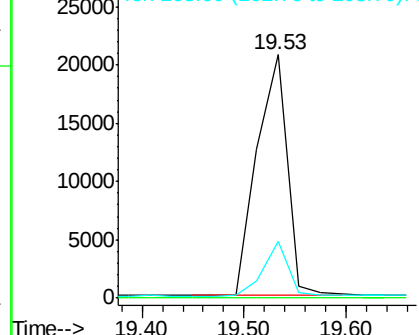



#29

Terphenyl-d14

Concen: 0.86 ng

RT: 19.74 min Scan# 1168

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8


Tot Ion:244 Resp: 6857

Ion Ratio Lower Upper

244 100

212 8.4 10.6 16.0#




122 3.8 15.4 23.0#

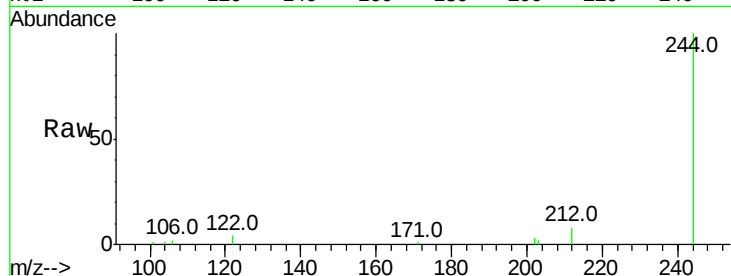

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

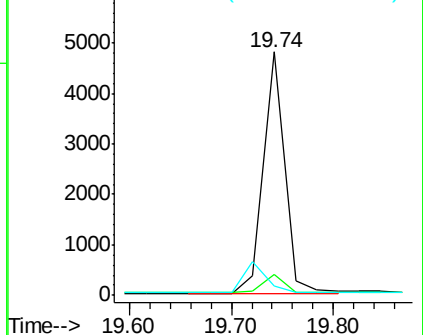

#30

Benzo(a)anthracene

Concen: 0.88 ng

RT: 21.25 min Scan# 1241

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion:228 Resp: 9760

Ion Ratio Lower Upper

228 100

226 33.2 19.7 29.5#



229 17.2 19.2 28.8#




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

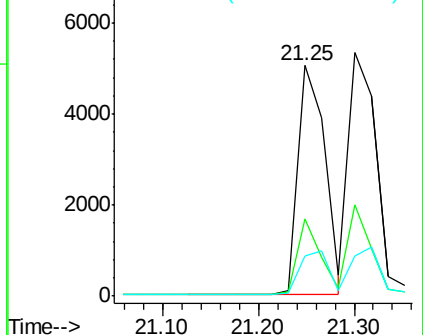



#31

Chrysene

Concen: 0.77 ng

RT: 21.30 min Scan# 1244

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8





Tot Ion:228 Resp: 10648

Ion Ratio Lower Upper

228 100

226 37.3 21.5 32.3#

229 16.6 18.6 28.0#

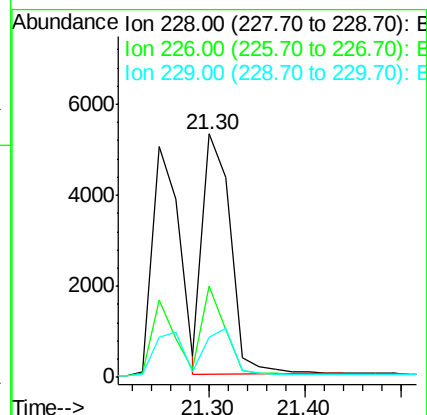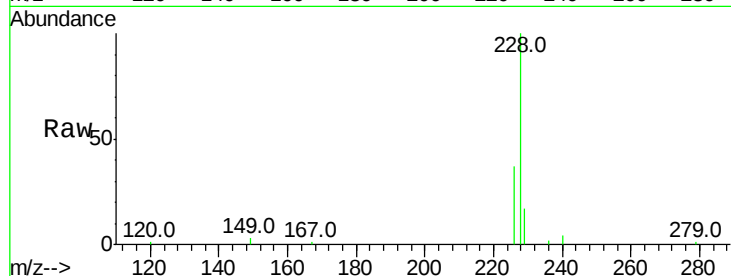

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.94 ng

RT: 21.20 min Scan# 1238

Delta R.T. -0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03




Tgt Ion:149 Resp: 4574


Ion Ratio Lower Upper

149 100

167 26.3 20.1 30.1

279 2.3 2.2 3.4


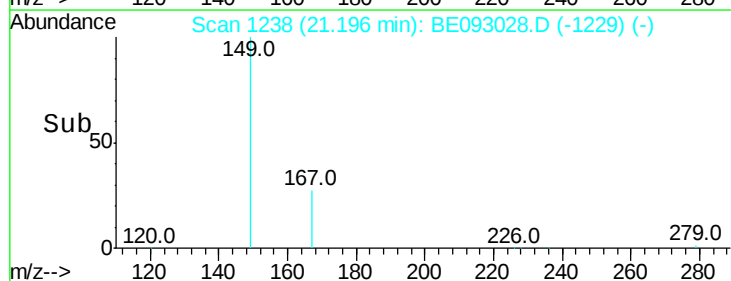
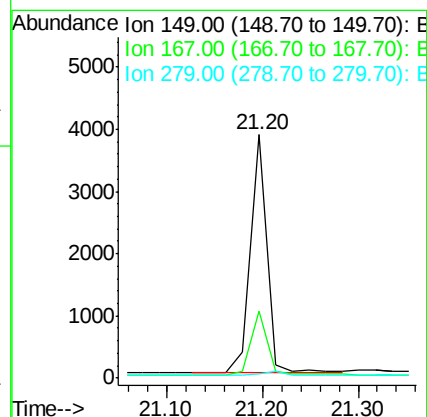





#33
 Indeno(1,2,3-cd)pyrene
 Concen: 0.88 ng
 RT: 26.22 min Scan# 1625
 Delta R.T. 0.00 min
 Lab File: BE093028.D
 Acq: 15 May 2017 11:03




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.8


Tot Ion:276 Resp: 38975
 Ion Ratio Lower Upper
 276 100
 138 33.3 27.4 41.2
 277 25.0 20.1 30.1

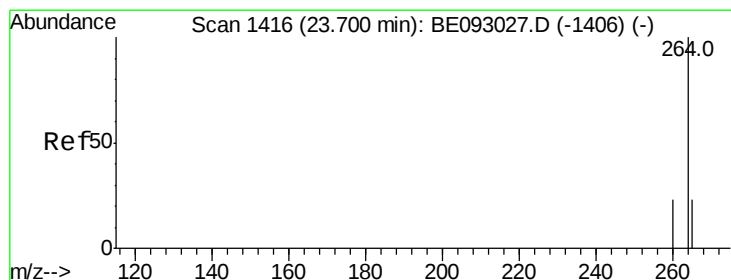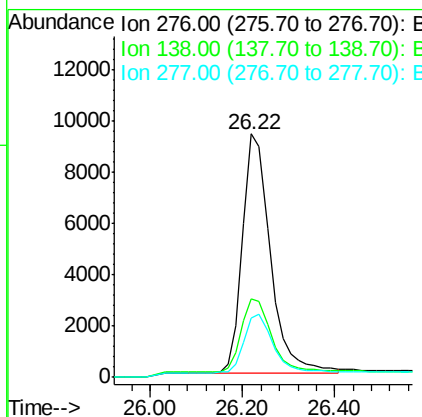

#34
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.69 min Scan# 1414
 Delta R.T. -0.01 min
 Lab File: BE093028.D
 Acq: 15 May 2017 11:03

Tgt Ion:264 Resp: 3721
 Ion Ratio Lower Upper
 264 100
 260 27.5 21.0 31.4
 265 30.7 24.6 36.8

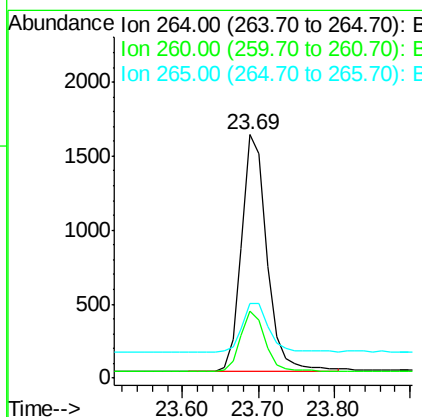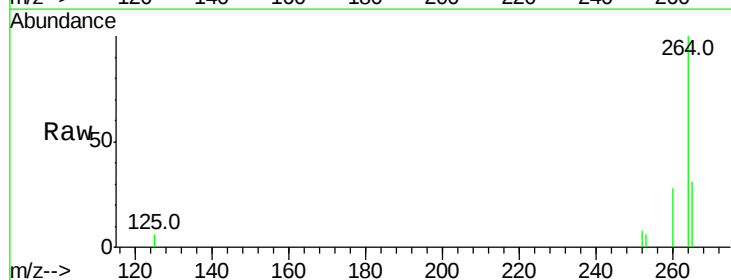



#35

Benzo(b)fluoranthene

Concen: 0.80 ng

RT: 22.95 min Scan# 1350

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8


Tot Ion:252 Resp: 9616

Ion Ratio Lower Upper

252 100

253 22.7 18.5 27.7




125 14.3 13.4 20.0



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

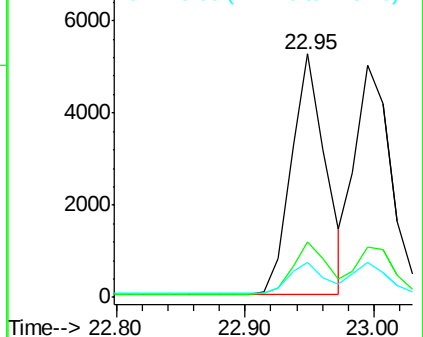

#36

Benzo(k)fluoranthene

Concen: 0.80 ng

RT: 23.00 min Scan# 1354

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion:252 Resp: 9620

Ion Ratio Lower Upper

252 100

253 21.8 20.3 30.5



125 14.9 12.2 18.4




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

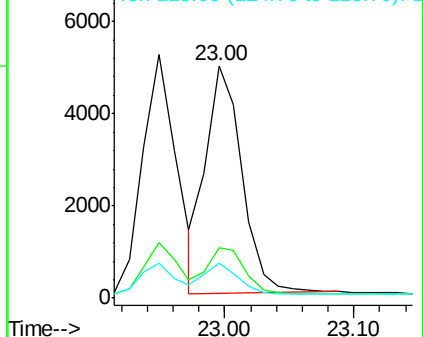



#37

Benzo(a)pyrene

Concen: 0.84 ng

RT: 23.59 min Scan# 1405

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8


Tot Ion:252 Resp: 8742

Ion Ratio Lower Upper




252 100

253 24.1 19.9 29.9

125 15.0 14.6 21.8



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

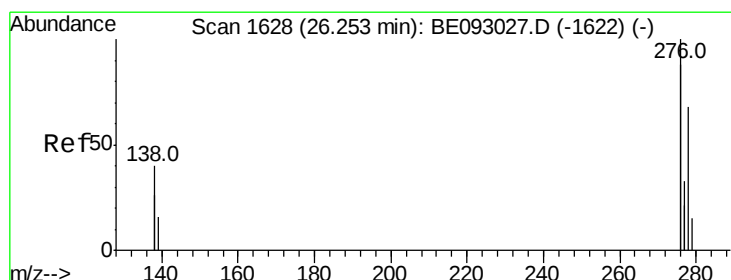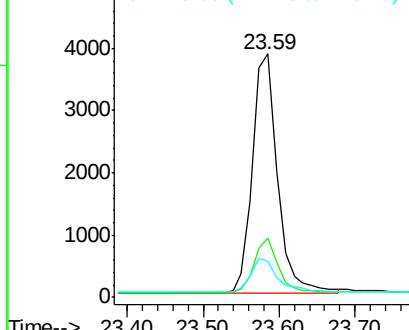

#38

Dibenzo(a,h)anthracene

Concen: 0.88 ng

RT: 26.25 min Scan# 1627

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03


Tgt Ion:278 Resp: 8290

Ion Ratio Lower Upper



278 100


139 23.3 21.4 32.0

279 25.1 22.2 33.2



Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

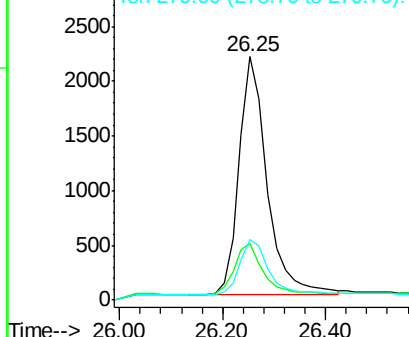

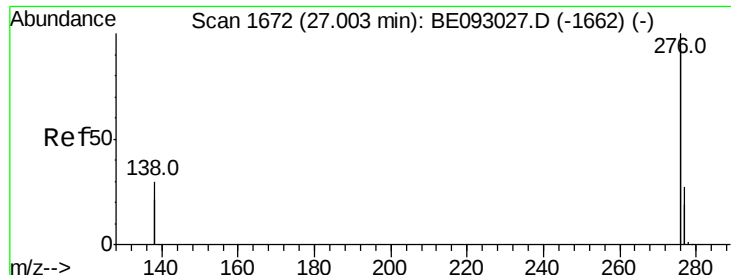

#39

Benzo(a,h,i)perylene

Concen: 0.83 ng

RT: 27.00 min Scan# 1671

Delta R.T. 0.00 min

Lab File: BE093028.D

Acq: 15 May 2017 11:03

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8


Tot Ion:276 Resp: 35582

Ion Ratio Lower Upper

276 100

277 26.0 21.2 31.8

138 28.5 24.5 36.7

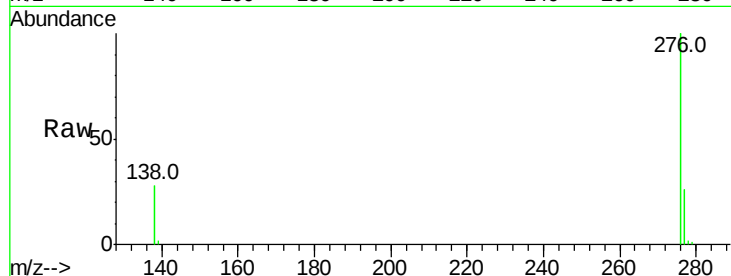

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

