


Data Path : Z:\HPCHEM1\BNA E\Data\BE051517\  
 Data File : BE093024.D  
 Acq On : 15 May 2017 8:33  
 Operator : SJ/MA  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE051517.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon May 15 13:35:57 2017

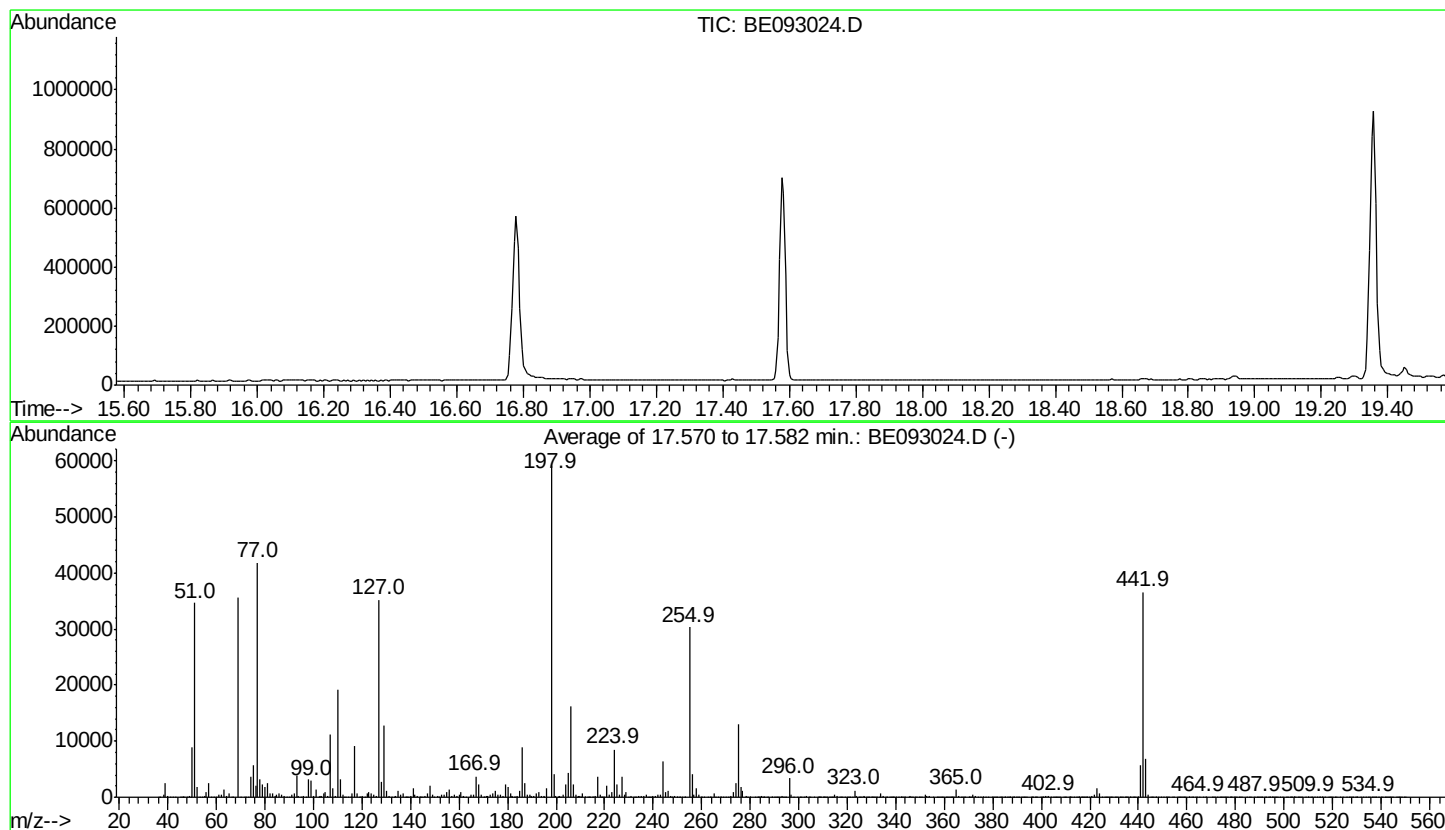

AutoFind: Scans 2550, 2551, 2552; Background Corrected with Scan 2541

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 58.6      | 34635   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 60.2      | 35576   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 110     | PASS             |
| 127         | 198          | 10           | 80           | 59.5      | 35171   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 59133   | PASS             |
| 199         | 198          | 5            | 9            | 7.0       | 4143    | PASS             |
| 275         | 198          | 10           | 60           | 21.9      | 12932   | PASS             |
| 365         | 198          | 1            | 100          | 2.3       | 1351    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.9      | 5804    | PASS             |
| 442         | 198          | 50           | 100          | 61.9      | 36609   | PASS             |
| 443         | 442          | 15           | 24           | 18.8      | 6890    | PASS             |