


Data Path : Z:\HPCHEM1\BNA E\DATA\BE051517\
 Data File : BE093032.D
 Acq On : 15 May 2017 13:44
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 15 13:35:57 2017

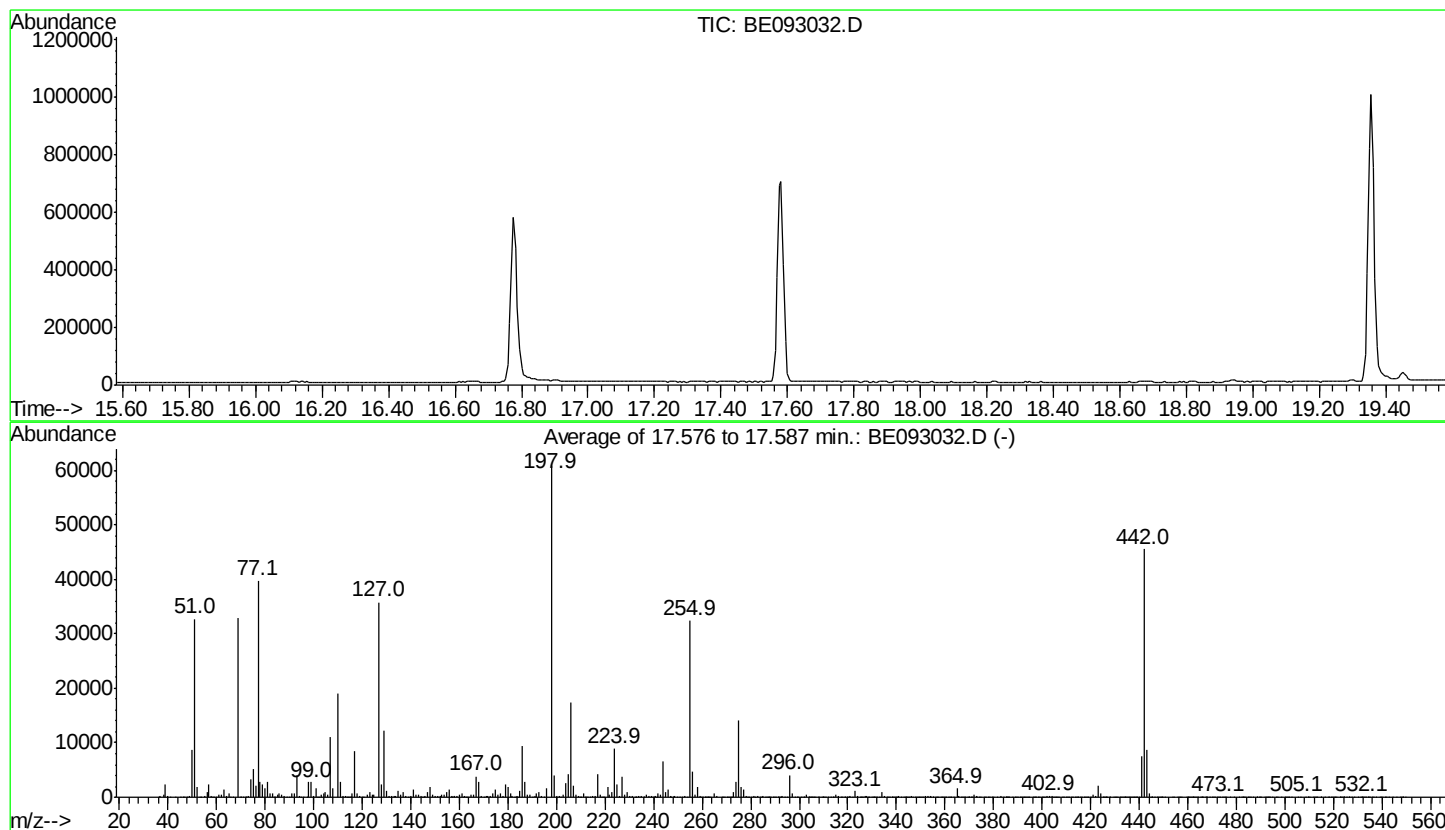

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.7	32718	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	54.0	32877	PASS
70	69	0.00	2	0.3	88	PASS
127	198	10	80	58.8	35789	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60903	PASS
199	198	5	9	6.6	4018	PASS
275	198	10	60	23.1	14053	PASS
365	198	1	100	2.7	1616	PASS
441	442	0.01	24	16.8	7642	PASS
442	198	50	100	74.8	45549	PASS
443	442	15	24	19.0	8676	PASS