


Data Path : Z:\HPCHEM1\BNA E\Data\BE051616\
Data File : BE091772.D
Acq On : 16 May 2016 14:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 26 16:09:46 2016

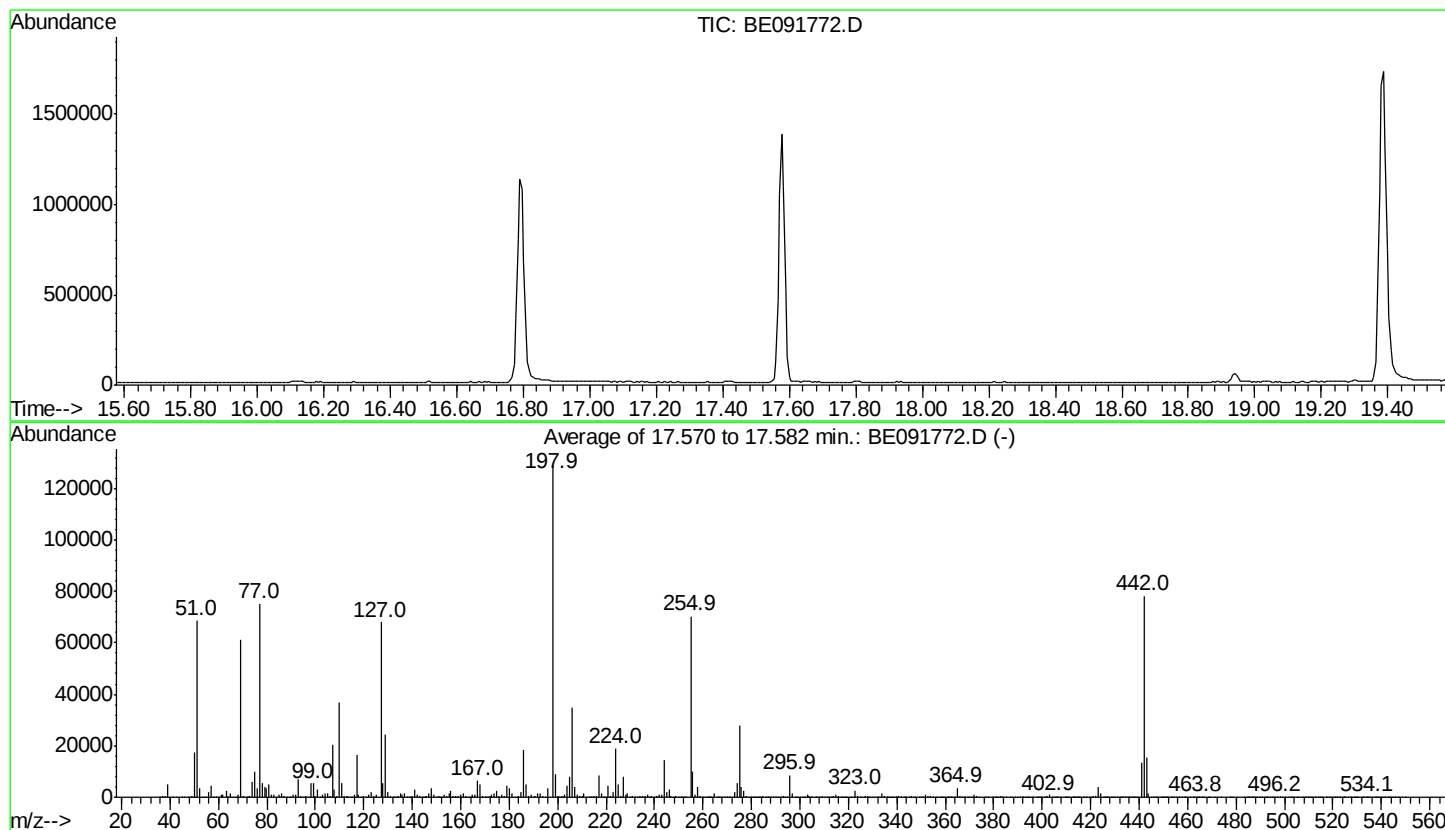

AutoFind: Scans 2550, 2551, 2552; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	68438	PASS
68	69	0.00	2	1.7	1031	PASS
69	198	0.00	100	47.4	61024	PASS
70	69	0.00	2	0.5	288	PASS
127	198	10	80	52.7	67900	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	128799	PASS
199	198	5	9	6.8	8781	PASS
275	198	10	60	21.8	28085	PASS
365	198	1	100	2.8	3667	PASS
441	442	0.01	24	17.3	13513	PASS
442	198	50	100	60.7	78136	PASS
443	442	15	24	19.8	15463	PASS