
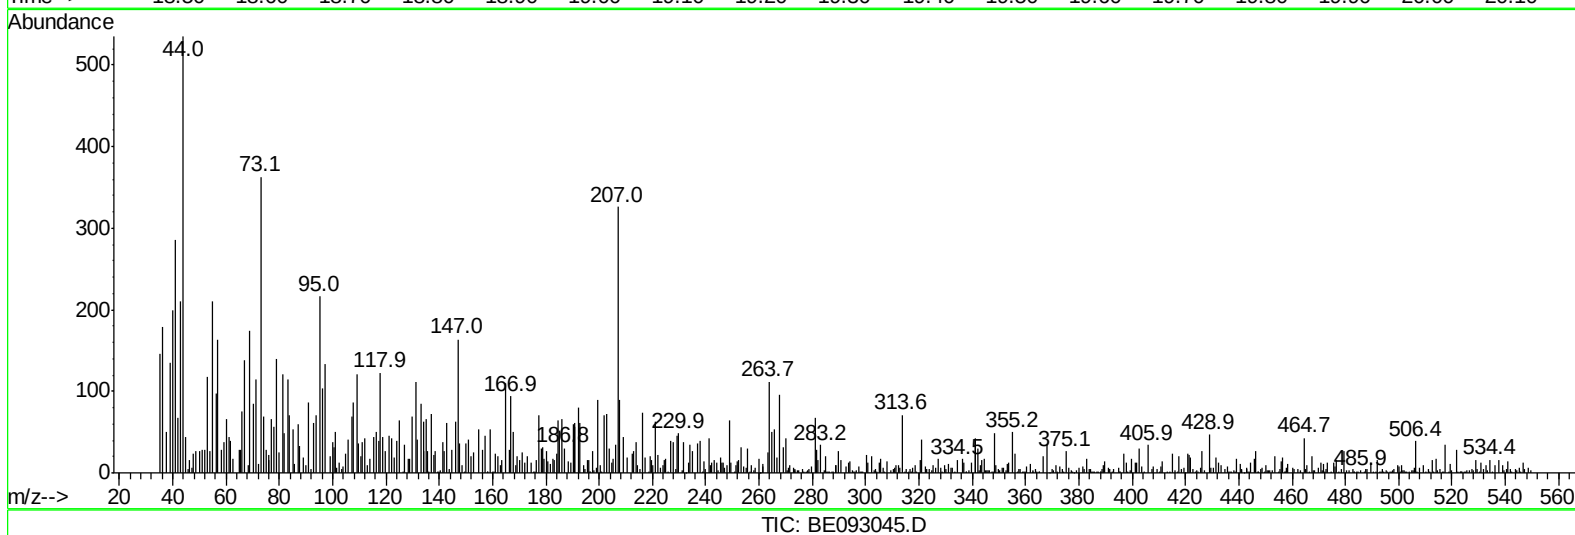


Data Path : Z:\HPCHEM1\BNA E\DATA\BE051617\
Data File : BE093045.D
Acq On : 16 May 2017 8:46
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 02:02:26 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

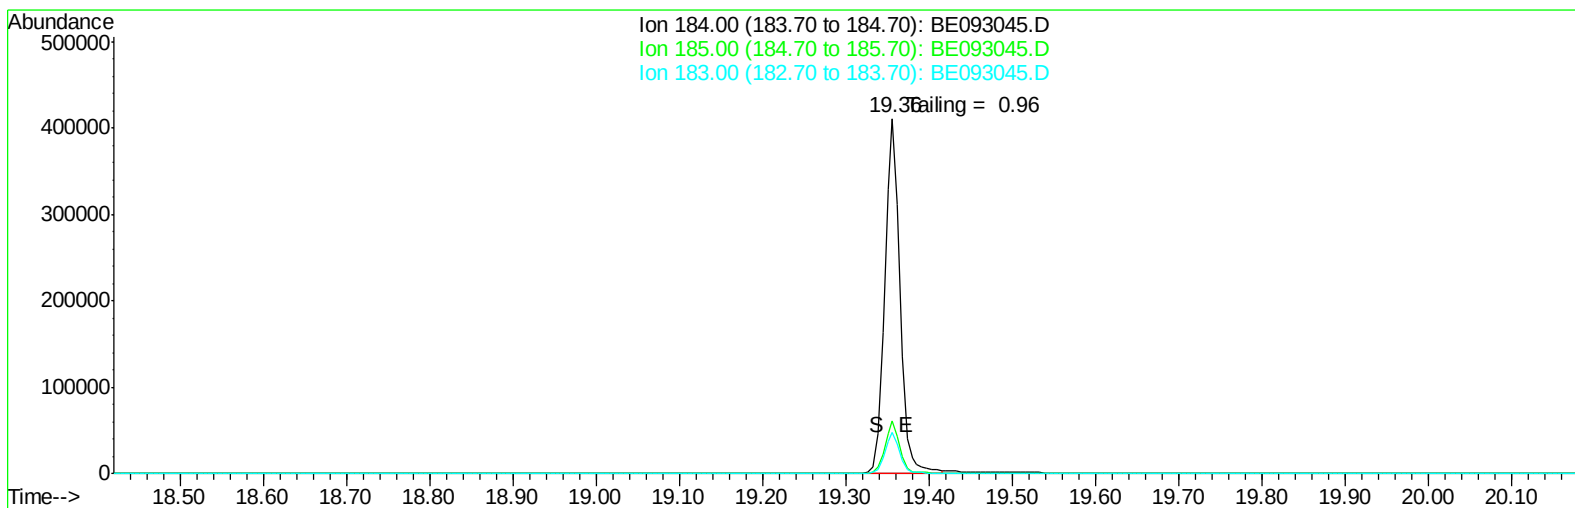

TIC: BE093045.D

(76) Benzidine



17.006min (+0.029) 332.42ng

response 143

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	59.09#
183.00	12.20	17.05#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE051617\
Data File : BE093045.D
Acq On : 16 May 2017 8:46
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 02:02:26 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

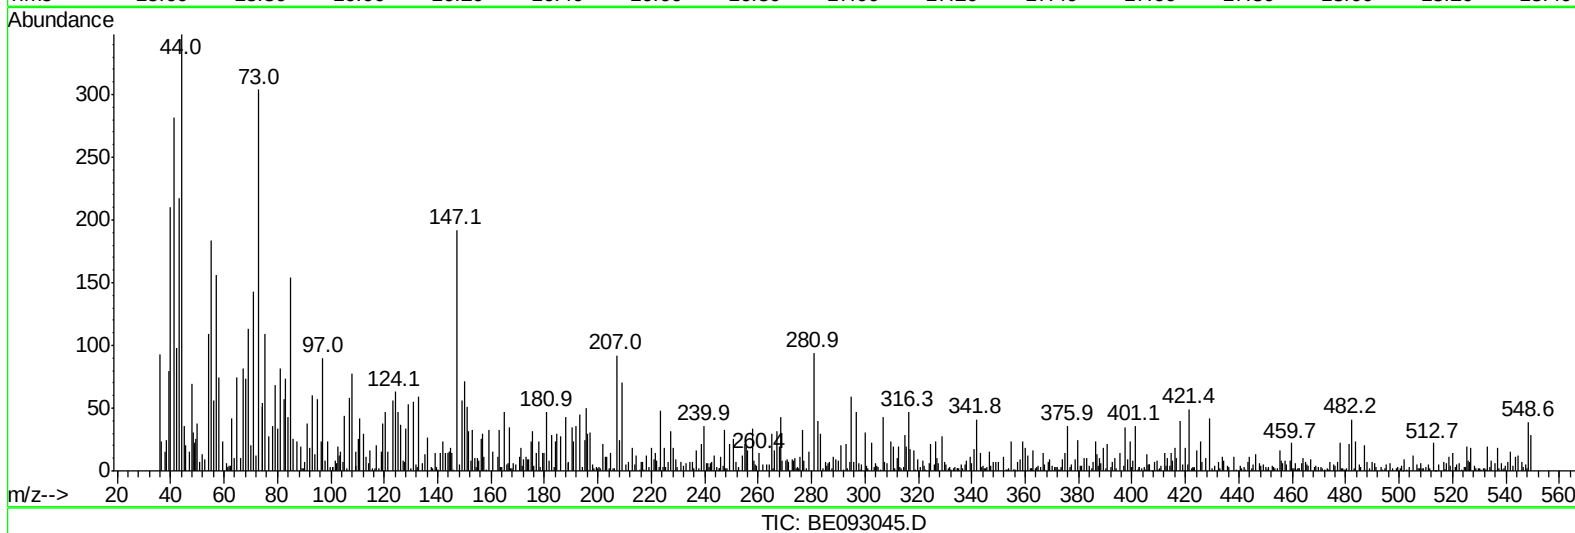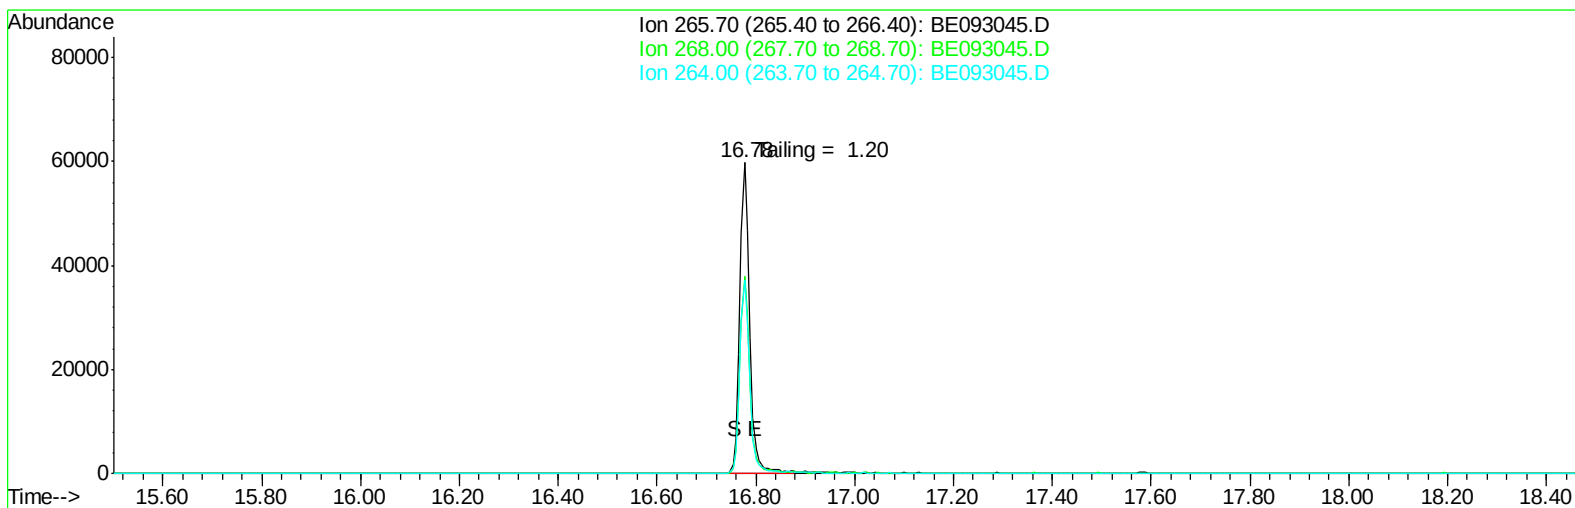

(69) Pentachlorophenol (C)

14.732min (+0.014) 52.22ng

response 12

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	344.44#
264.00	64.60	27.78#
0.00	0.00	0.00