


Data Path : Z:\HPCHEM1\BNA E\DATA\BE051617\
Data File : BE093045.D
Acq On : 16 May 2017 8:46
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 15 13:35:57 2017

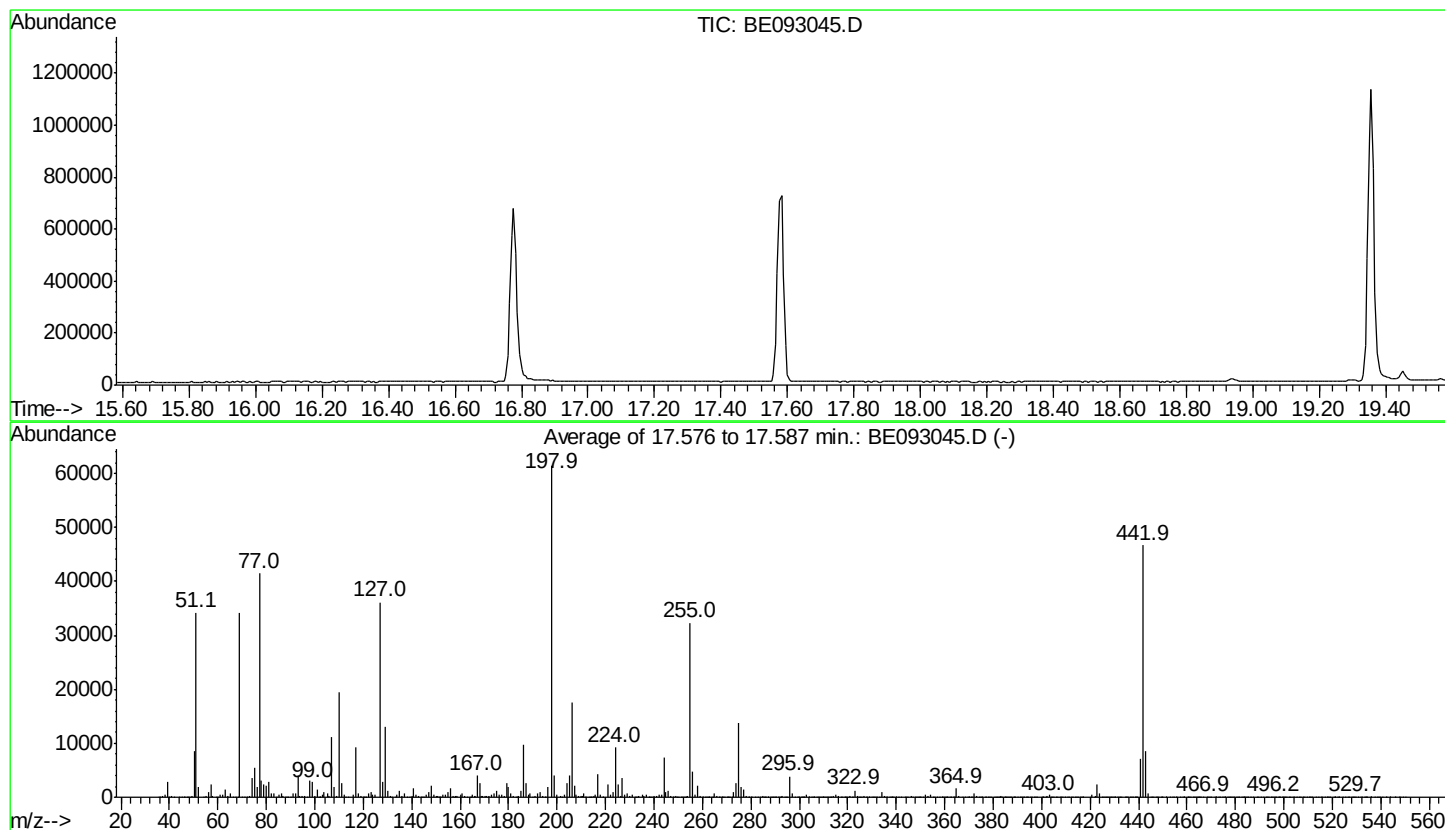

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.8	34273	PASS
68	69	0.00	2	0.3	101	PASS
69	198	0.00	100	55.8	34262	PASS
70	69	0.00	2	0.2	63	PASS
127	198	10	80	58.9	36153	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61429	PASS
199	198	5	9	6.5	4022	PASS
275	198	10	60	22.5	13816	PASS
365	198	1	100	2.6	1585	PASS
441	442	0.01	24	15.1	7066	PASS
442	198	50	100	76.0	46696	PASS
443	442	15	24	18.4	8586	PASS