

Data Path : Z:\HPCHEM1\BNA E\Data\Be051816\
 Data File : BE091791.D
 Acq On : 18 May 2016 13:49
 Operator : UM/SJ
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4

Quant Time: May 18 18:01:31 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE042616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 26 16:09:46 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	32763	5.00	ng	-0.02
7) Naphthalene-d8	10.55	136	154986	5.00	ng	-0.02
13) Acenaphthene-d10	14.41	164	94783	5.00	ng	-0.01
19) Phenanthrene-d10	17.14	188	256789	5.00	ng	-0.01
26) Chrysene-d12	21.29	240	382256	5.00	ng	-0.02
35) Perylene-d12	23.73	264	365867	5.00	ng	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.37	112	2867	0.36	ng	-0.02
5) Phenol-d6	6.95	99	3761	0.35	ng	0.00
8) Nitrobenzene-d5	8.94	82	3501	0.35	ng	-0.01
14) 2,4,6-Tribromophenol	15.88	330	1181	0.49	ng	-0.01
15) 2-Fluorobiphenyl	13.02	172	9997	0.37	ng	-0.01
29) Terphenyl-d14	19.74	244	17904	0.30	ng	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.31	88	1515	0.30	ng	98
3) n-Nitrosodimethylamine	3.63	42	1955	0.33	ng	# 97
6) bis(2-Chloroethyl)ether	7.21	93	3561	0.38	ng	# 80
9) Nitrobenzene	8.98	77	3516	0.34	ng	# 94
10) Naphthalene	10.61	128	11947	0.38	ng	99
11) Hexachlorobutadiene	10.90	225	2484	0.54	ng	88
12) 2-Methylnaphthalene	12.22	142	7632	0.38	ng	93
16) Acenaphthylene	14.12	152	14365	0.39	ng	# 80
17) Acenaphthene	14.46	154	8455	0.36	ng	# 83
18) Fluorene	15.44	166	11433	0.39	ng	98
20) 4-Bromophenyl-phenylether	16.33	248	3541	0.38	ng	94
21) Hexachlorobenzene	16.45	284	3592	0.39	ng	99
22) Pentachlorophenol	16.79	266	1472	0.39	ng	92
23) Phenanthrene	17.17	178	23188	0.40	ng	98
24) Anthracene	17.26	178	20095	0.38	ng	99
25) Fluoranthene	19.19	202	26158	0.43	ng	# 96
27) Benzidine	19.38	184	5959	0.35	ng	# 83
28) Pyrene	19.55	202	27329	0.32	ng	100
30) Benzo(a)anthracene	21.27	228	59337	0.64	ng	93
31) 3,3'-Dichlorobenzidine	21.22	252	17834	0.37	ng	# 88
32) Chrysene	21.27	228	59667	0.61	ng	97
33) Bis(2-ethylhexyl)phthalate	21.20	149	12752	0.45	ng	# 80
34) Indeno(1,2,3-cd)pyrene	26.27	276	34315	0.40	ng	94
36) Benzo(b)fluoranthene	22.98	252	29912	0.35	ng	98
37) Benzo(k)fluoranthene	23.02	252	30838	0.35	ng	98
38) Benzo(a)pyrene	23.61	252	28899	0.36	ng	100
39) Dibenzo(a,h)anthracene	26.29	278	28029	0.37	ng	96
40) Benzo(g,h,i)perylene	27.06	276	28928	0.37	ng	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\Data\Be051816\
Data File : BE091791.D
Acq On : 18 May 2016 13:49
Operator : UM/SJ
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Quant Time: May 18 18:01:31 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE042616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 26 16:09:46 2016
Response via : Initial Calibration

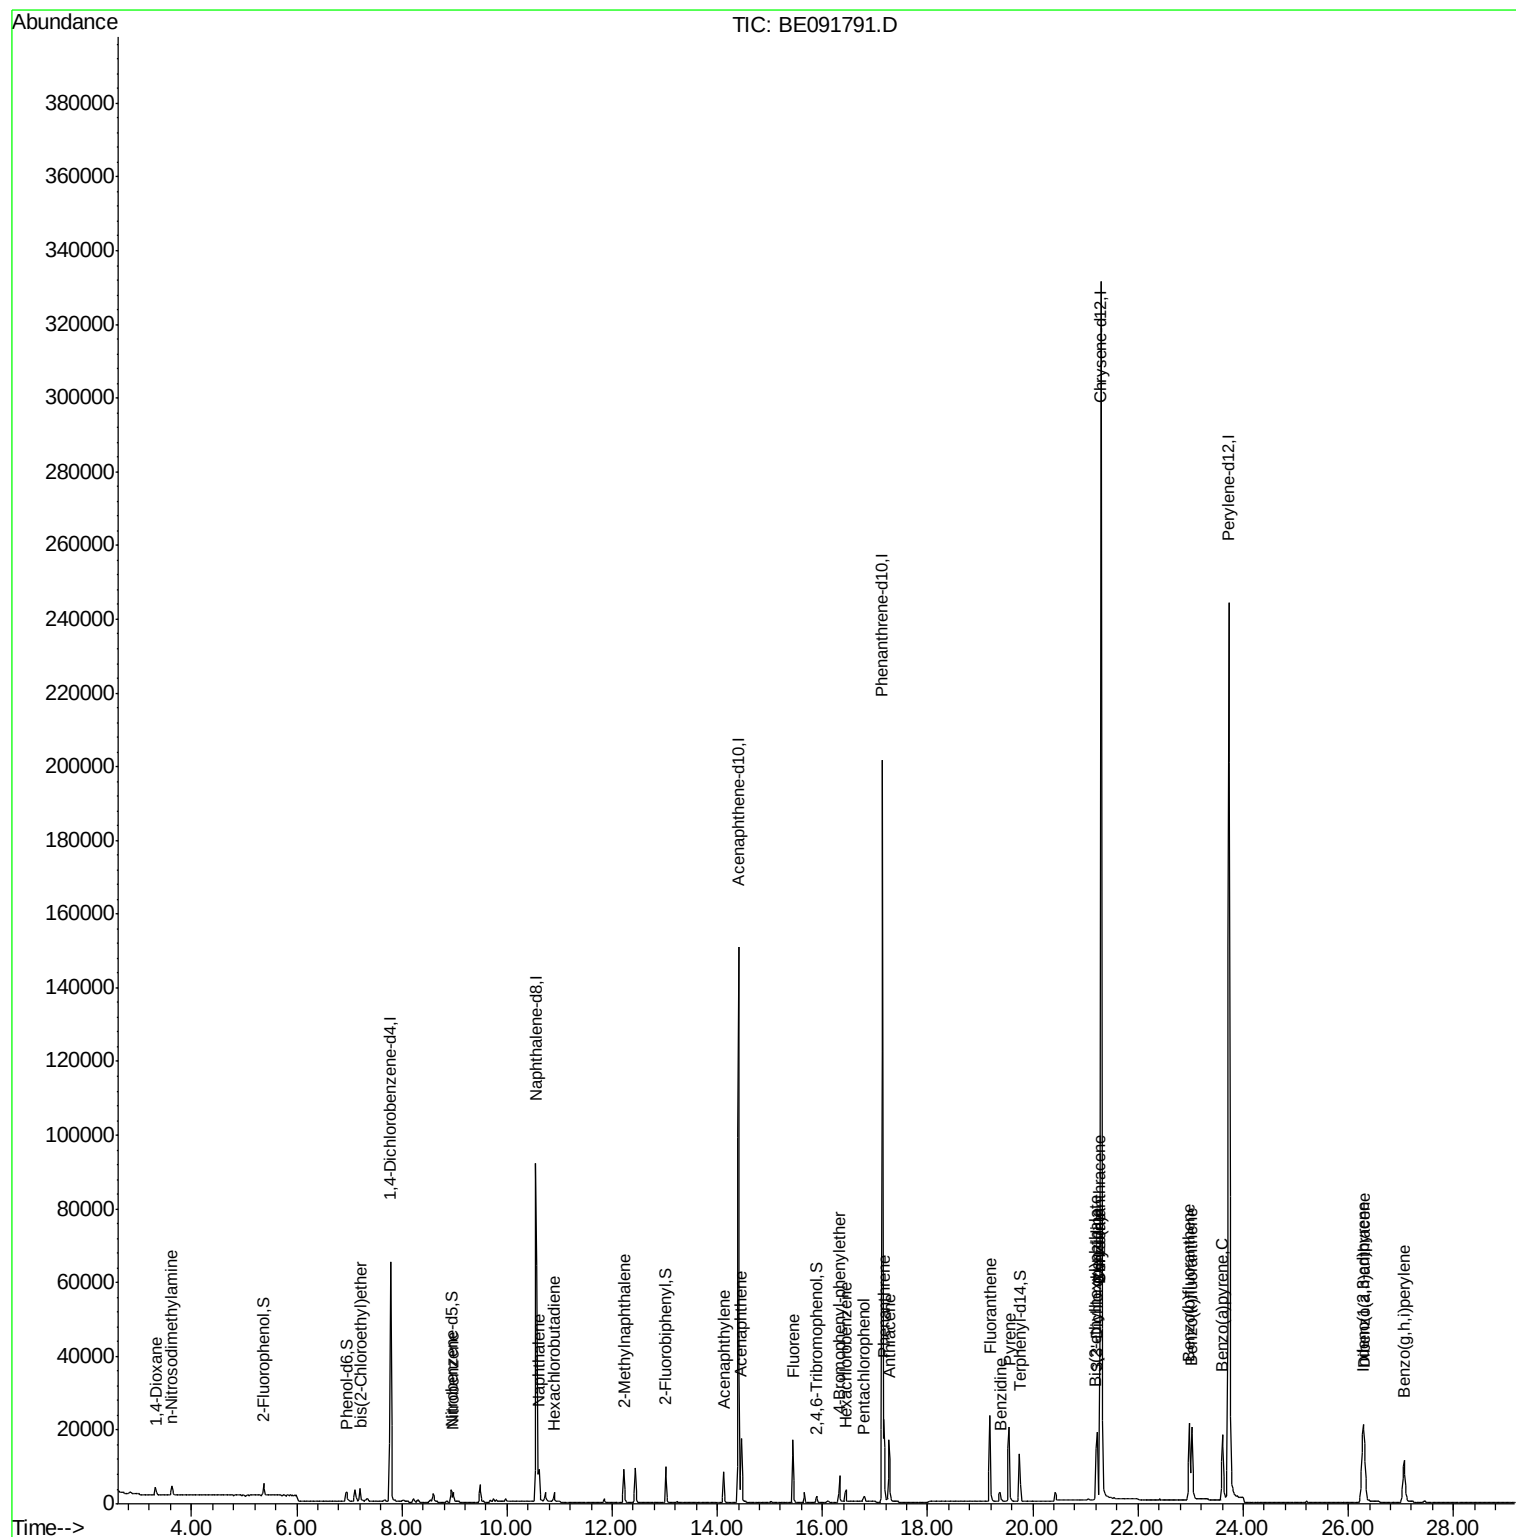



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.79 min Scan# 299

Delta R.T. -0.02 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4


Tot Ion:152 Resp: 32763

Ion Ratio Lower Upper

152 100

150 162.3 122.6 183.8




115 64.0 52.8 79.2

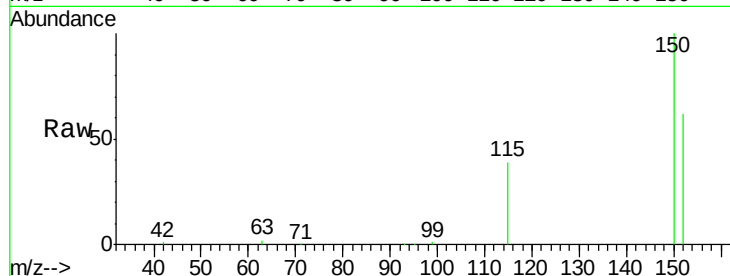

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

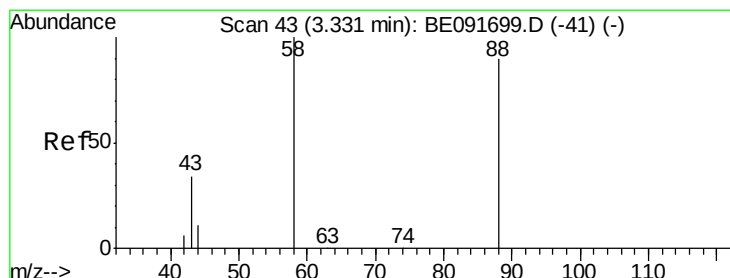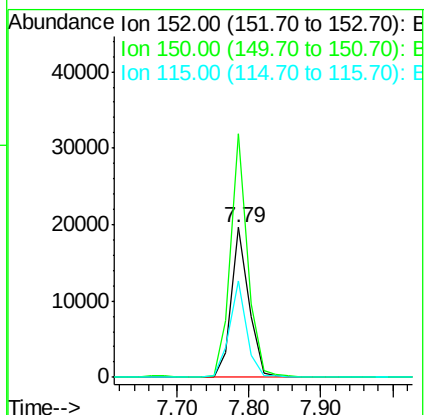

#2

1,4-Dioxane

Concen: 0.30 ng

RT: 3.31 min Scan# 42

Delta R.T. -0.02 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49


Tgt Ion: 88 Resp: 1515

Ion Ratio Lower Upper

88 100

58 82.0 65.8 98.6



43 35.9 25.3 37.9

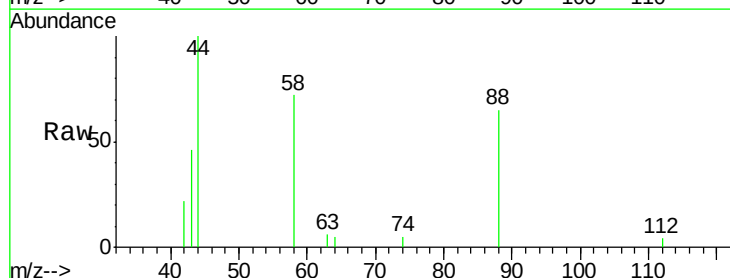


Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

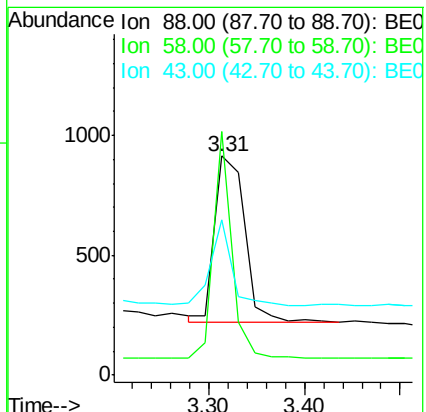



#3

n-Nitrosodimethylamine

Concen: 0.33 ng

RT: 3.63 min Scan# 60

Delta R.T. -0.00 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4


Tot Ion: 42 Resp: 1955

Ion Ratio Lower Upper

42 100

74 111.6 87.9 131.9




44 14.1 6.6 9.8#

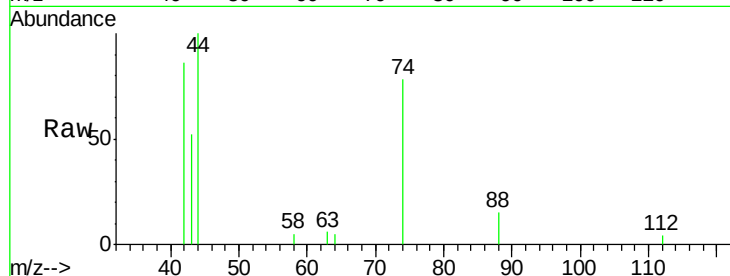

Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

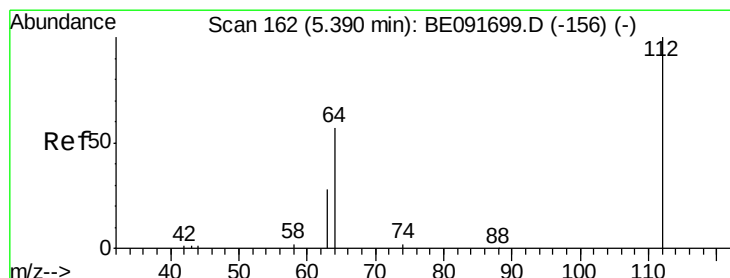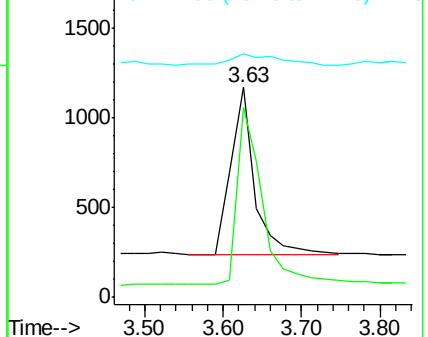

#4

2-Fluorophenol

Concen: 0.36 ng

RT: 5.37 min Scan# 161

Delta R.T. -0.02 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49


Tgt Ion: 112 Resp: 2867

Ion Ratio Lower Upper

112 100

64 64.7 30.9 46.3#



63 34.2 16.7 25.1#

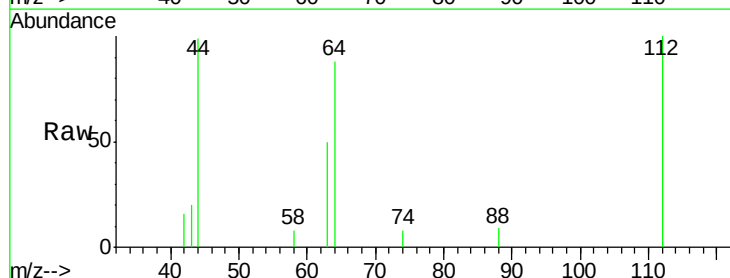


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

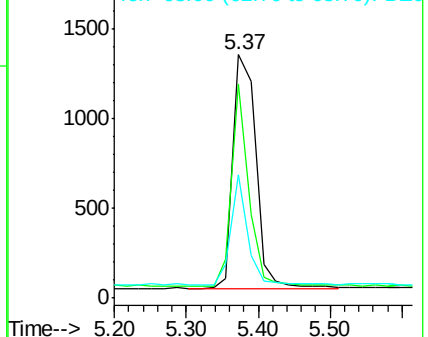



#5

Phenol-d6

Concen: 0.35 ng

RT: 6.95 min Scan# 251

Delta R.T. 0.00 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4


Tot Ion: 99 Resp: 3761

Ion Ratio Lower Upper

99 100

42 25.1 16.2 24.2#




71 35.3 29.0 43.4



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

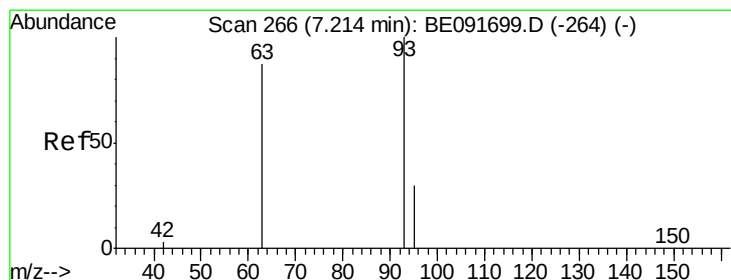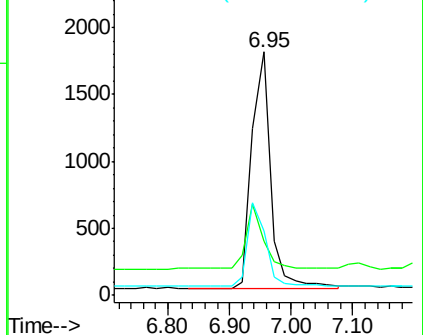

#6

bis(2-Chloroethyl)ether

Concen: 0.38 ng

RT: 7.21 min Scan# 266

Delta R.T. 0.00 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49


Tgt Ion: 93 Resp: 3561

Ion Ratio Lower Upper

93 100

63 81.7 49.5 74.3#



95 32.2 22.2 33.4




Abundance Ion 93.00 (92.70 to 93.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Ion 95.00 (94.70 to 95.70): BE0

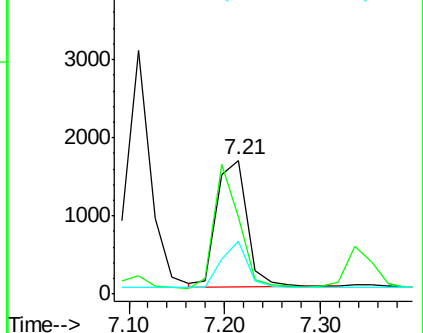



#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.55 min Scan# 510

Delta R.T. -0.02 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4

Tot Ion:136 Resp: 154986


Ion Ratio Lower Upper

136 100

137 9.9 8.9 13.3

54 11.9 8.2 12.4

68 8.1 6.2 9.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

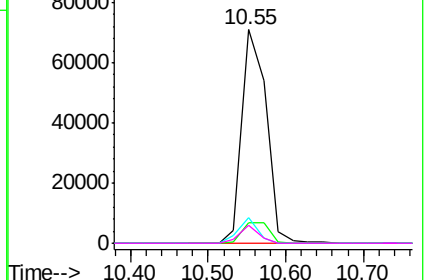

#8

Nitrobenzene-d5

Concen: 0.35 ng

RT: 8.94 min Scan# 390

Delta R.T. -0.01 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49


Tgt Ion: 82 Resp: 3501

Ion Ratio Lower Upper

82 100

128 33.2 25.4 38.0



54 60.4 48.4 72.6




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

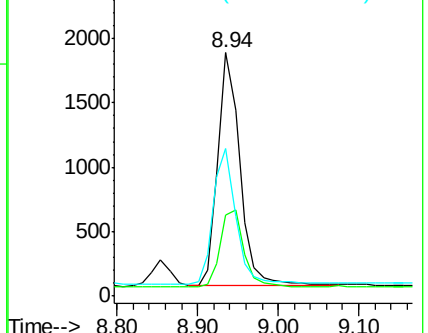



#9

Nitrobenzene

Concen: 0.34 ng

RT: 8.98 min Scan# 394

Delta R.T. -0.01 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4





Tot Ion: 77 Resp: 3516

Ion Ratio Lower Upper

77 100

123 36.7 26.9 40.3

65 14.2 9.4 14.2#

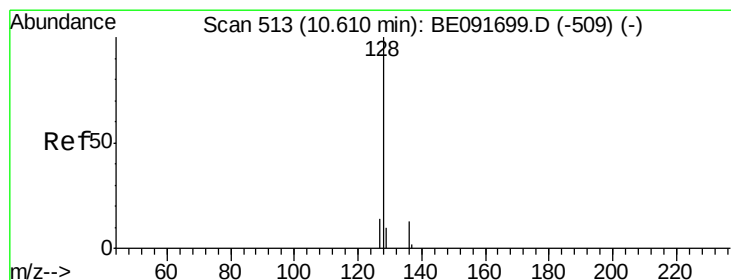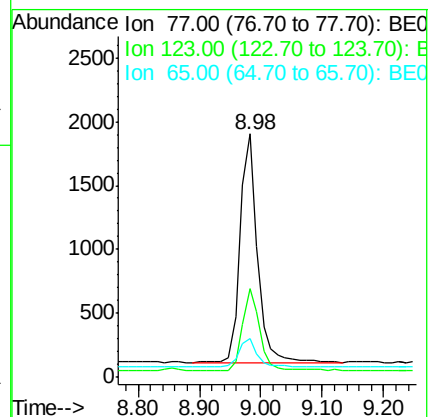

#10

Naphthalene

Concen: 0.38 ng

RT: 10.61 min Scan# 513

Delta R.T. -0.00 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49




Tgt Ion: 128 Resp: 11947


Ion Ratio Lower Upper

128 100

129 12.1 9.3 13.9

127 12.9 10.7 16.1



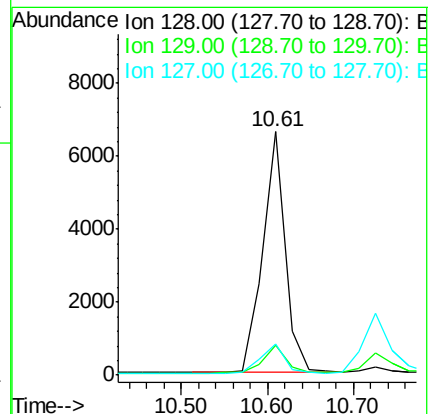





#11
Hexachlorobutadiene
Concen: 0.54 ng
RT: 10.90 min Scan# 528
Delta R.T. -0.02 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49




Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4


Tot Ion:225 Resp: 2484
Ion Ratio Lower Upper
225 100
223 70.7 49.0 73.6
227 71.5 50.3 75.5

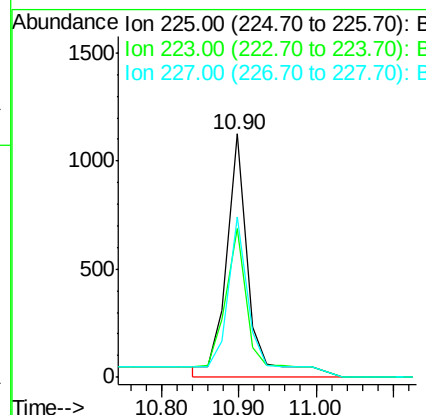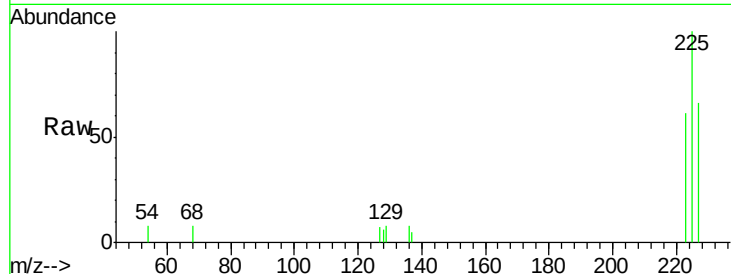

#12
2-Methylnaphthalene
Concen: 0.38 ng
RT: 12.22 min Scan# 637
Delta R.T. -0.01 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49

Tgt Ion:142 Resp: 7632
Ion Ratio Lower Upper
142 100
141 83.9 71.4 107.0
115 32.3 30.3 45.5

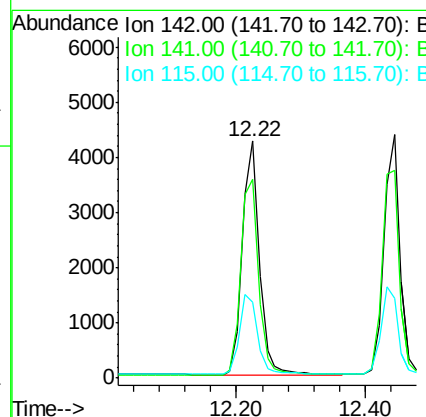



#13

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.41 min Scan# 819

Delta R.T. -0.01 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4


Tot Ion:164 Resp: 94783

Ion Ratio Lower Upper

164 100

162 98.7 85.3 127.9




160 41.2 46.2 69.2#



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

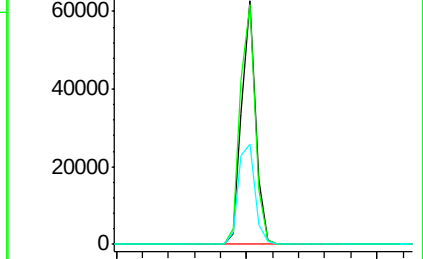

#14

2,4,6-Tribromophenol

Concen: 0.49 ng

RT: 15.88 min Scan# 938

Delta R.T. -0.01 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49


Tgt Ion:330 Resp: 1181

Ion Ratio Lower Upper

330 100

332 96.7 79.1 118.7



141 41.8 125.4 188.0#




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




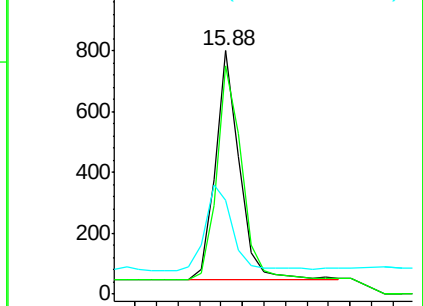


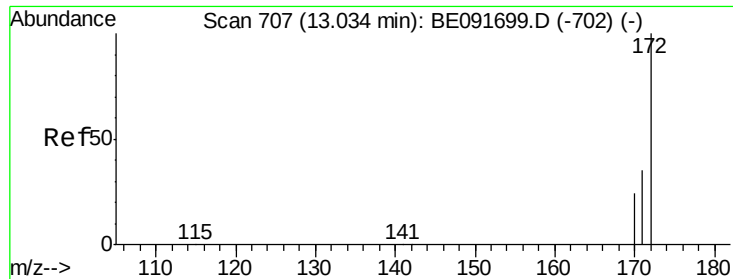

#15
2-Fluorobiphenyl
Concen: 0.37 ng
RT: 13.02 min Scan# 706
Delta R.T. -0.01 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49




Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4


Tot Ion:172 Resp: 9997
Ion Ratio Lower Upper
172 100
171 36.8 28.8 43.2
170 26.0 19.3 28.9

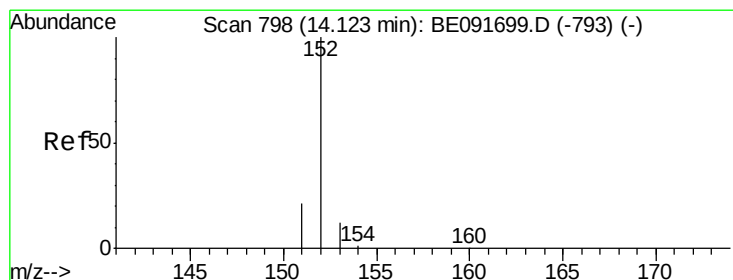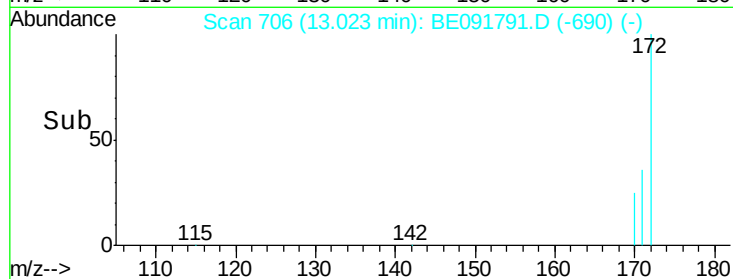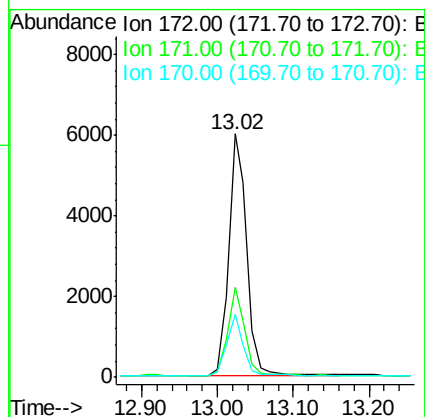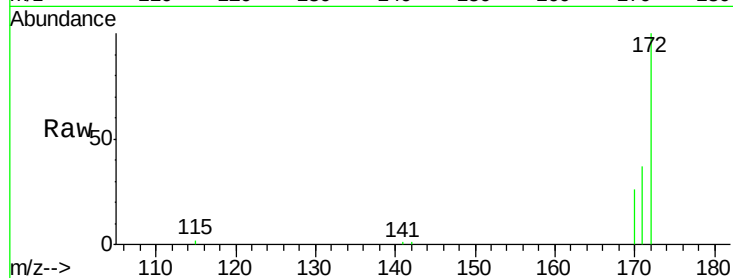

#16
Acenaphthylene
Concen: 0.39 ng
RT: 14.12 min Scan# 798
Delta R.T. -0.00 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49

Tgt Ion:152 Resp: 14365
Ion Ratio Lower Upper
152 100
151 17.7 3.9 5.9#
153 18.2 10.3 15.5#


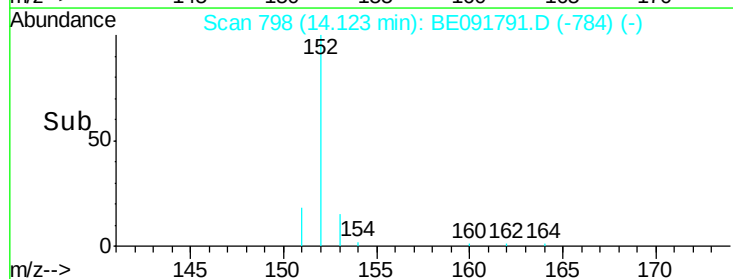
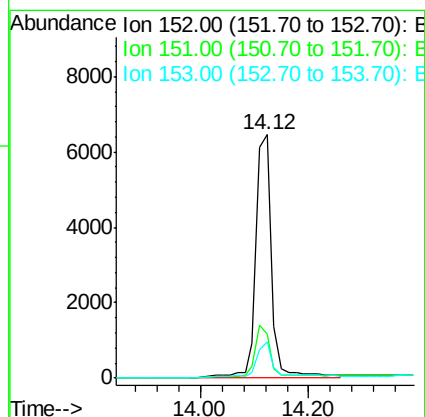
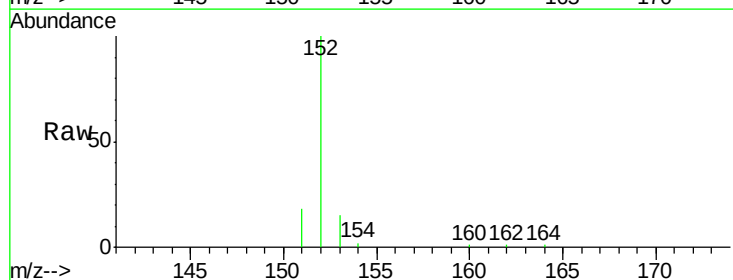




#17
Acenaphthene
Concen: 0.36 ng
RT: 14.46 min Scan# 823
Delta R.T. -0.01 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49




Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4


Tot Ion:154 Resp: 8455
Ion Ratio Lower Upper
154 100
153 118.2 80.0 120.0
152 60.4 40.0 60.0#

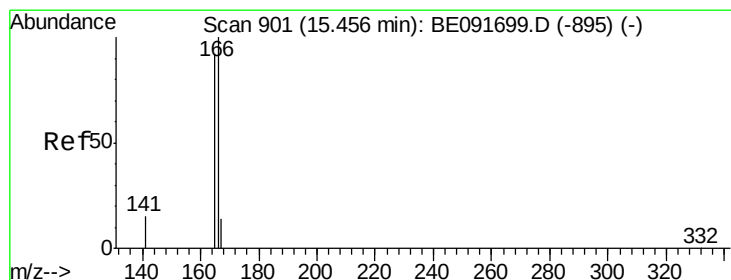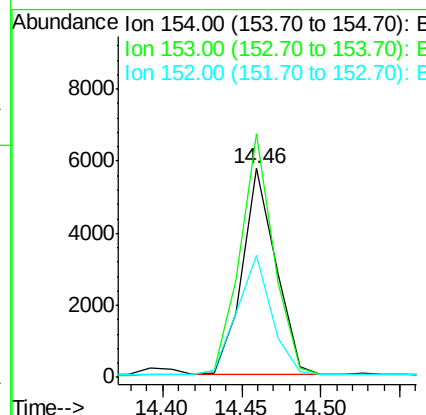

#18
Fluorene
Concen: 0.39 ng
RT: 15.44 min Scan# 900
Delta R.T. -0.01 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49

Tgt Ion:166 Resp: 11433
Ion Ratio Lower Upper
166 100
165 98.9 80.8 121.2
167 13.5 10.9 16.3

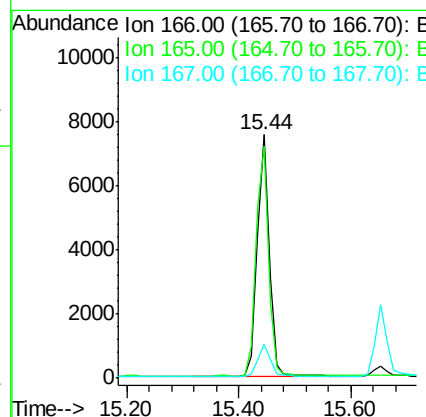

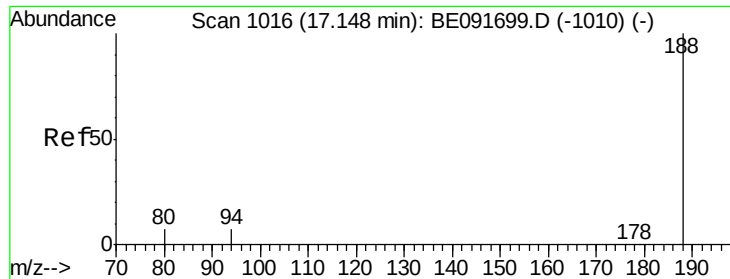

#19

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.14 min Scan# 1015

Delta R.T. -0.01 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4


Tot Ion:188 Resp: 256789

Ion Ratio Lower Upper

188 100

94 7.1 8.7 13.1#




80 6.3 9.4 14.0#

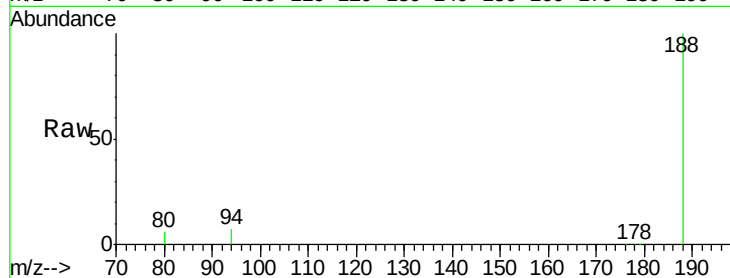

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

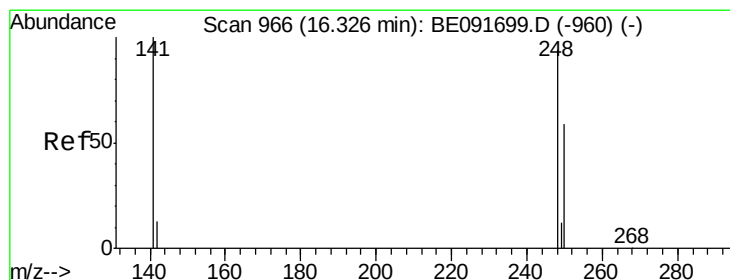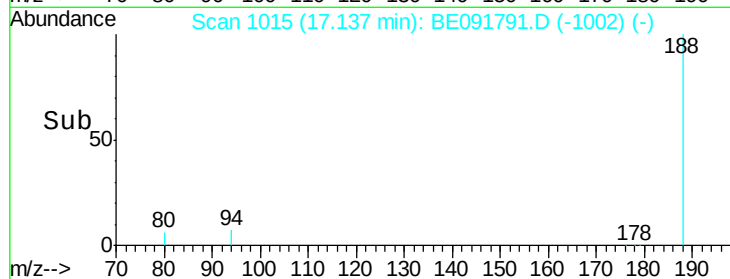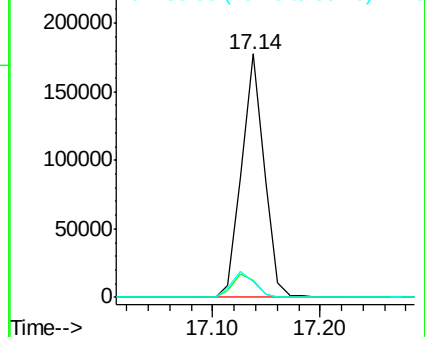

#20

4-Bromophenyl-phenylether

Concen: 0.38 ng

RT: 16.33 min Scan# 966

Delta R.T. -0.00 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49


Tgt Ion:248 Resp: 3541

Ion Ratio Lower Upper

248 100

250 99.9 80.5 120.7



141 79.6 72.0 108.0

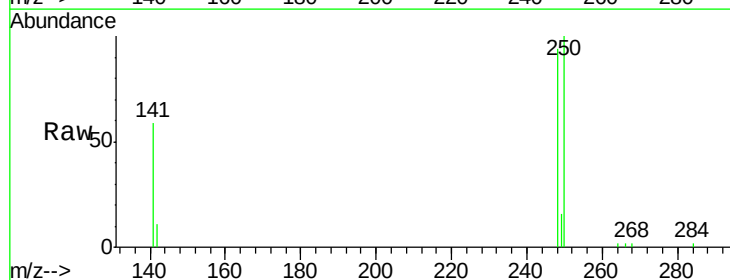


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E



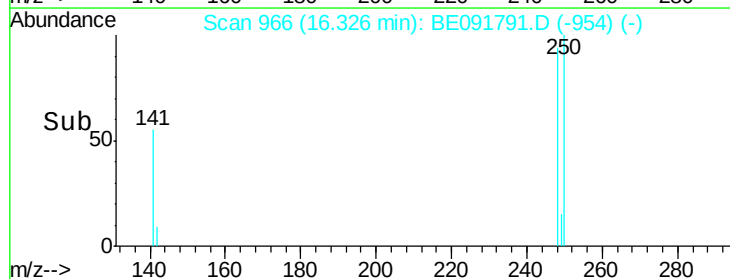
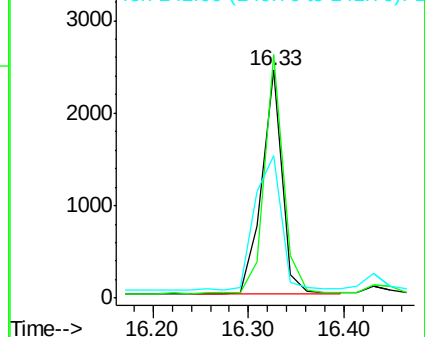




#21
Hexachlorobenzene
Concen: 0.39 ng
RT: 16.45 min Scan# 973
Delta R.T. -0.00 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49




Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4


Tot Ion:284 Resp: 3592
Ion Ratio Lower Upper
284 100
142 40.7 32.2 48.2
249 32.2 25.4 38.2

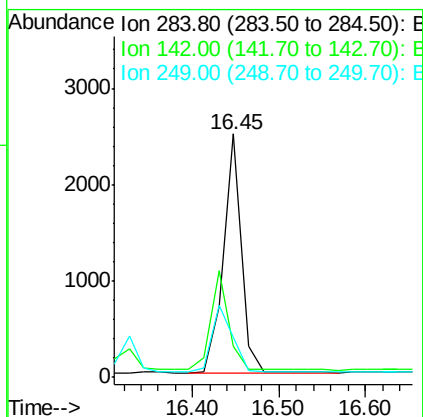

#22
Pentachlorophenol
Concen: 0.39 ng
RT: 16.79 min Scan# 993
Delta R.T. 0.00 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49

Tgt Ion:266 Resp: 1472
Ion Ratio Lower Upper
266 100
268 70.5 58.2 87.2
264 59.3 56.2 84.4



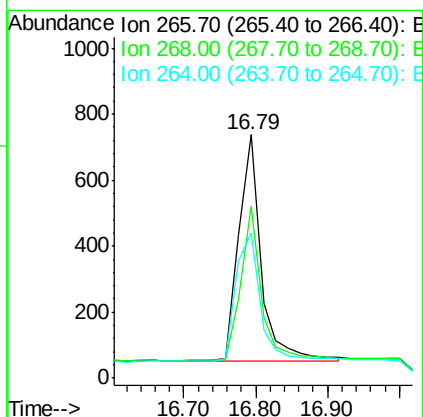





#23
Phenanthrene
Concen: 0.40 ng
RT: 17.17 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49




Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4


Tot Ion:178 Resp: 23188
Ion Ratio Lower Upper
178 100
176 19.9 15.3 22.9
179 16.7 12.6 18.8

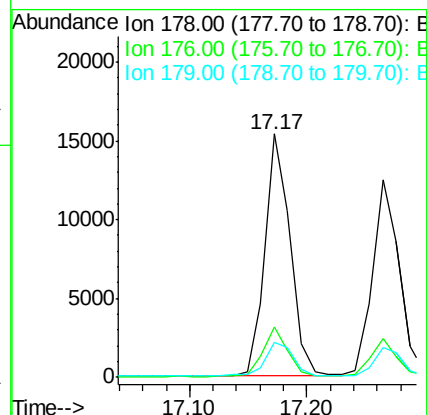

#24
Anthracene
Concen: 0.38 ng
RT: 17.26 min Scan# 1026
Delta R.T. -0.01 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49

Tgt Ion:178 Resp: 20095
Ion Ratio Lower Upper
178 100
176 18.6 14.6 21.8
179 15.0 11.8 17.6

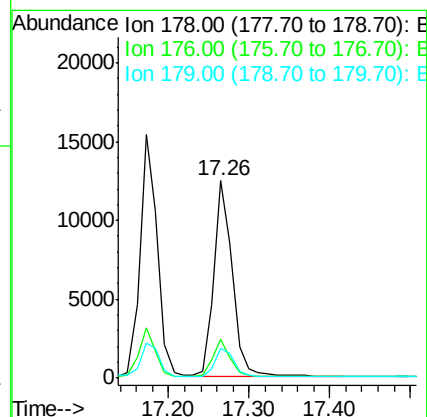



#25

Fluoranthene

Concen: 0.43 ng

RT: 19.19 min Scan# 1150

Delta R.T. 0.00 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4


Tot Ion:202 Resp: 26158

Ion Ratio Lower Upper

202 100

101 10.8 11.0 16.6#




203 17.7 13.9 20.9



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

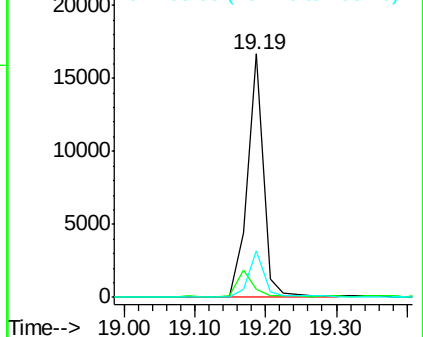

#26

Chrysene-d12

Concen: 5.00 ng

RT: 21.29 min Scan# 1247

Delta R.T. -0.02 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49


Tgt Ion:240 Resp: 382256

Ion Ratio Lower Upper

240 100

120 5.3 11.0 16.4#



236 29.3 21.7 32.5




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E




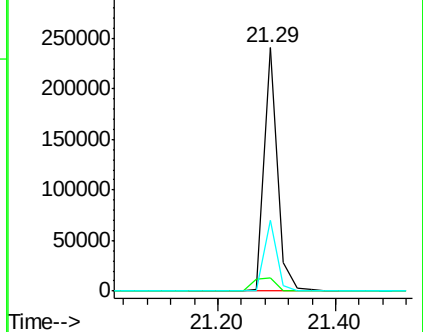




#27
Benzidine
Concen: 0.35 ng
RT: 19.38 min Scan# 1160
Delta R.T. 0.00 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49




Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4


Tot Ion:184 Resp: 5959
Ion Ratio Lower Upper
184 100
185 19.0 22.3 33.5#
183 12.5 16.4 24.6#

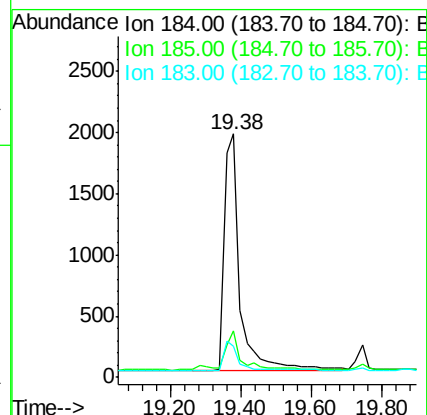

#28
Pyrene
Concen: 0.32 ng
RT: 19.55 min Scan# 1169
Delta R.T. 0.00 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49

Tgt Ion:202 Resp: 27329
Ion Ratio Lower Upper
202 100
200 21.0 16.8 25.2
203 17.6 14.0 21.0

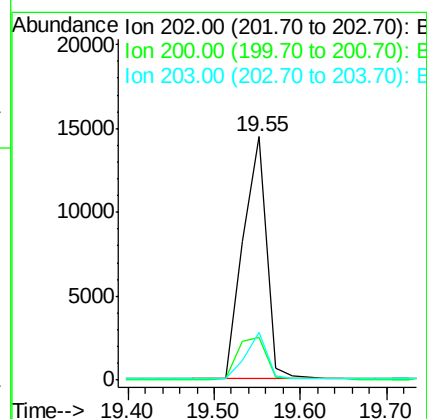



#29

Terphenyl-d14

Concen: 0.30 ng

RT: 19.74 min Scan# 1179

Delta R.T. -0.02 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4


Tot Ion:244 Resp: 17904

Ion Ratio Lower Upper




244 100

212 9.5 6.9 10.3

122 9.8 11.0 16.4#

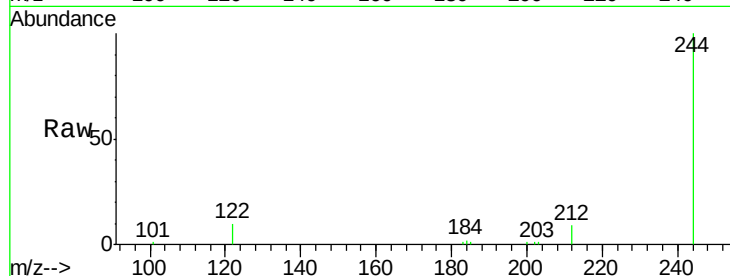

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

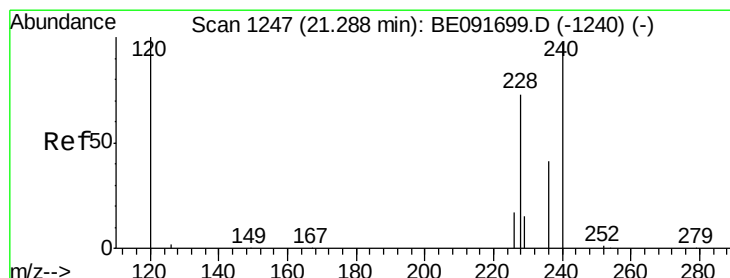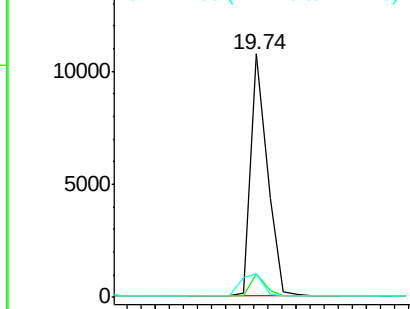

#30

Benzo(a)anthracene

Concen: 0.64 ng

RT: 21.27 min Scan# 1246

Delta R.T. -0.02 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49


Tgt Ion:228 Resp: 59337

Ion Ratio Lower Upper



228 100


226 30.6 21.0 31.4

229 17.4 15.7 23.5

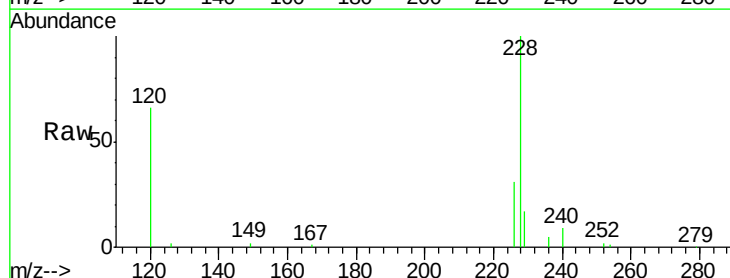

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

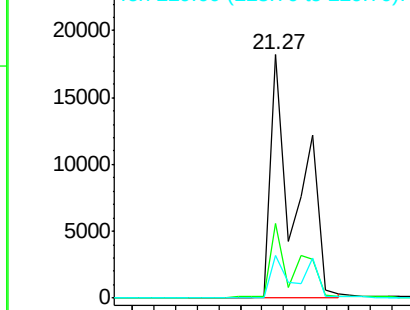







#31
 3,3'-Dichlorobenzidine
 Concen: 0.37 ng
 RT: 21.22 min Scan# 1244
 Delta R.T. -0.02 min
 Lab File: BE091791.D
 Acq: 18 May 2016 13:49

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4

Tot Ion:252 Resp: 17834
 Ion Ratio Lower Upper
 252 100
 254 69.5 51.1 76.7
 126 2.7 12.6 18.8#

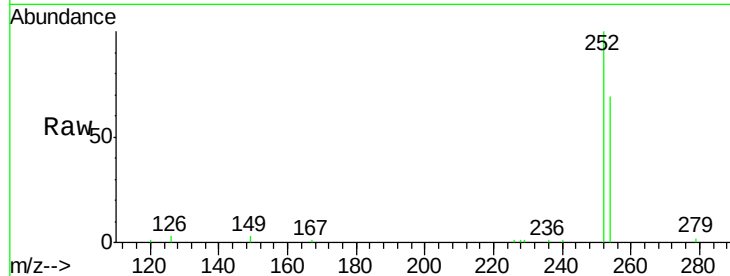


Abundance Ion 252.00 (251.70 to 252.70): E
 Ion 254.00 (253.70 to 254.70): E
 Ion 126.00 (125.70 to 126.70): E

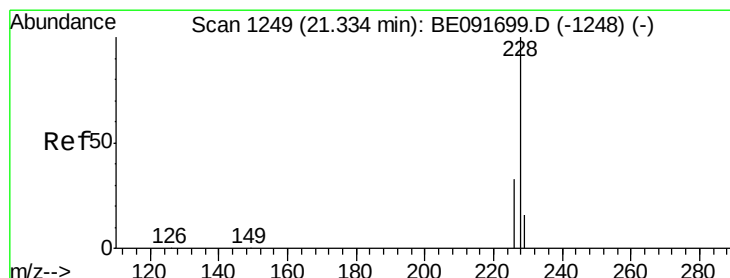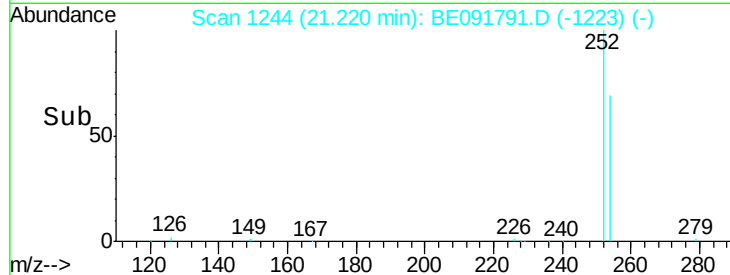
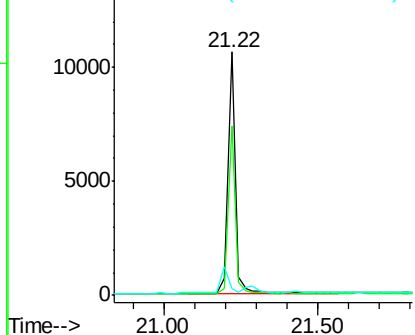



#32
 Chrysene
 Concen: 0.61 ng
 RT: 21.27 min Scan# 1246
 Delta R.T. -0.07 min
 Lab File: BE091791.D
 Acq: 18 May 2016 13:49

Tgt Ion:228 Resp: 59667
 Ion Ratio Lower Upper
 228 100
 226 30.6 24.0 36.0
 229 17.4 15.9 23.9

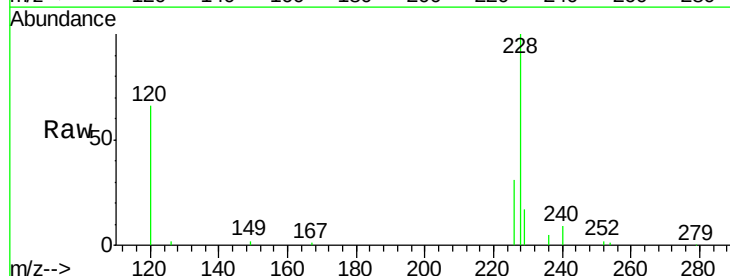

Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 226.00 (225.70 to 226.70): E
 Ion 229.00 (228.70 to 229.70): E

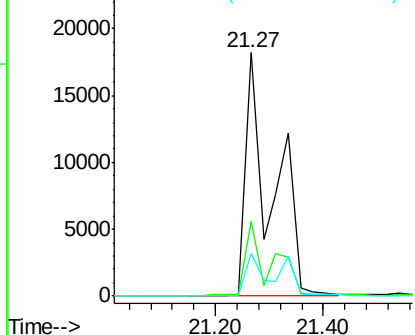







#33
 Bis(2-ethylhexyl)phthalate
 Concen: 0.45 ng
 RT: 21.20 min Scan# 1243
 Delta R.T. -0.02 min
 Lab File: BE091791.D
 Acq: 18 May 2016 13:49

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4

Tot Ion:149 Resp: 12752
 Ion Ratio Lower Upper
 149 100
 167 31.1 19.5 29.3#
 279 0.0 10.0 15.0#




Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E


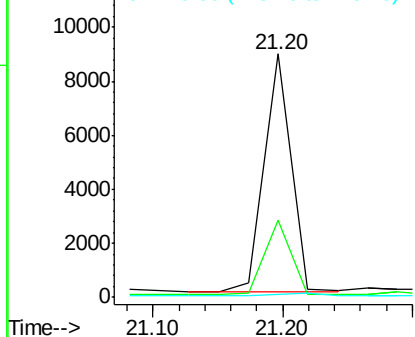



#34
 Indeno(1,2,3-cd)pyrene
 Concen: 0.40 ng
 RT: 26.27 min Scan# 1642
 Delta R.T. -0.03 min
 Lab File: BE091791.D
 Acq: 18 May 2016 13:49

Tgt Ion:276 Resp: 34315
 Ion Ratio Lower Upper
 276 100
 138 24.0 23.4 35.2
 277 24.5 19.8 29.8



Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

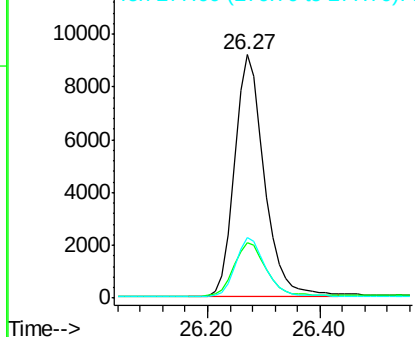




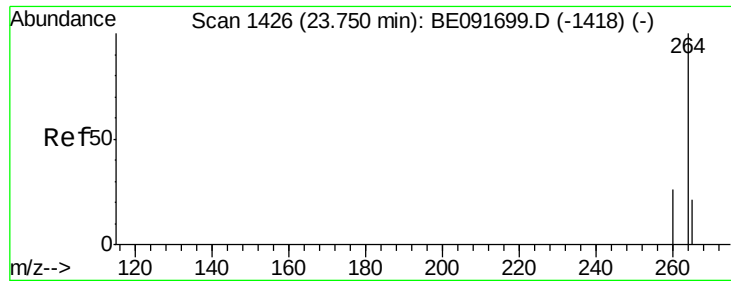


#35
Pervlene-d12
Concen: 5.00 ng
RT: 23.73 min Scan# 1424
Delta R.T. -0.02 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion:264 Resp: 365867




Ion	Ratio	Lower	Upper
264	100		
260	25.5	20.0	30.0
265	21.1	17.5	26.3

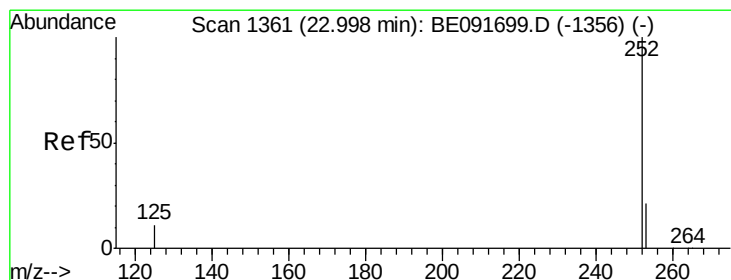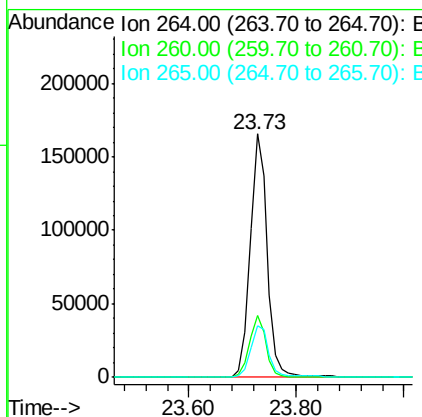


#36
Benzo(b)fluoranthene
Concen: 0.35 ng
RT: 22.98 min Scan# 1359
Delta R.T. -0.02 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49

Tgt Ion:252 Resp: 29912

Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.4	26.0
125	11.5	10.2	15.2



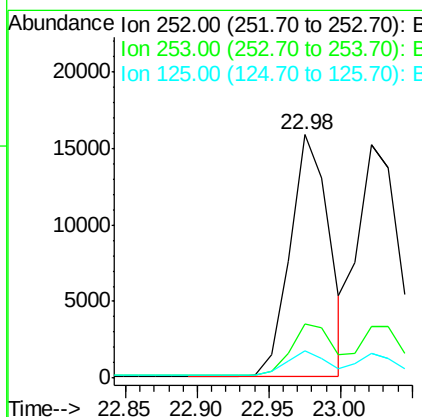
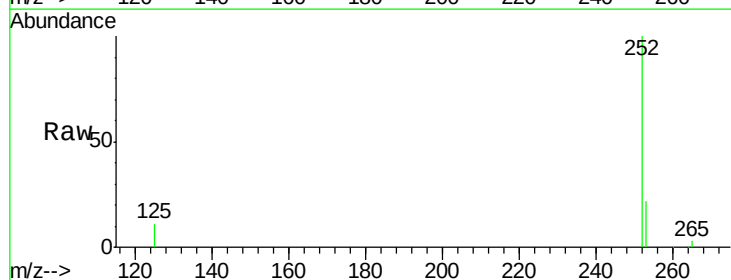




#37
Benzo(k)fluoranthene
Concen: 0.35 ng
RT: 23.02 min Scan# 1363
Delta R.T. -0.02 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49




Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4


Tot Ion:252 Resp: 30838
Ion Ratio Lower Upper
252 100
253 21.9 17.6 26.4
125 10.4 9.9 14.9

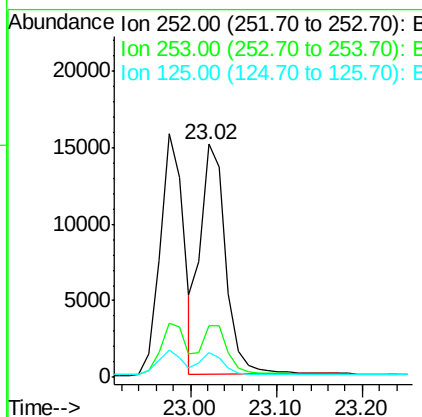

#38
Benzo(a)pyrene
Concen: 0.36 ng
RT: 23.61 min Scan# 1414
Delta R.T. -0.02 min
Lab File: BE091791.D
Acq: 18 May 2016 13:49

Tgt Ion:252 Resp: 28899
Ion Ratio Lower Upper
252 100
253 22.8 18.1 27.1
125 13.5 11.0 16.4

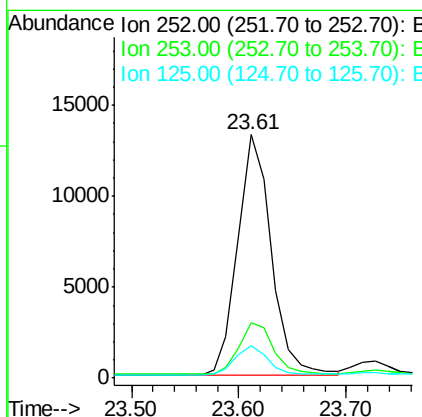



#39

Dibenzo(a,h)anthracene

Concen: 0.37 ng

RT: 26.29 min Scan# 1644

Delta R.T. -0.05 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4


Tot Ion:278 Resp: 28029

Ion Ratio Lower Upper

278 100

139 16.5 16.0 24.0




279 24.4 19.4 29.2



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

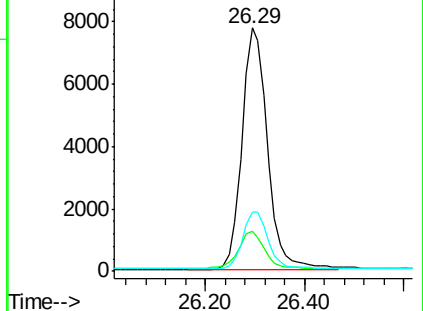

#40

Benzo(g,h,i)perylene

Concen: 0.37 ng

RT: 27.06 min Scan# 1710

Delta R.T. -0.05 min

Lab File: BE091791.D

Acq: 18 May 2016 13:49


Tgt Ion:276 Resp: 28928

Ion Ratio Lower Upper

276 100

277 24.2 18.6 28.0

138 20.8 20.4 30.6



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

