
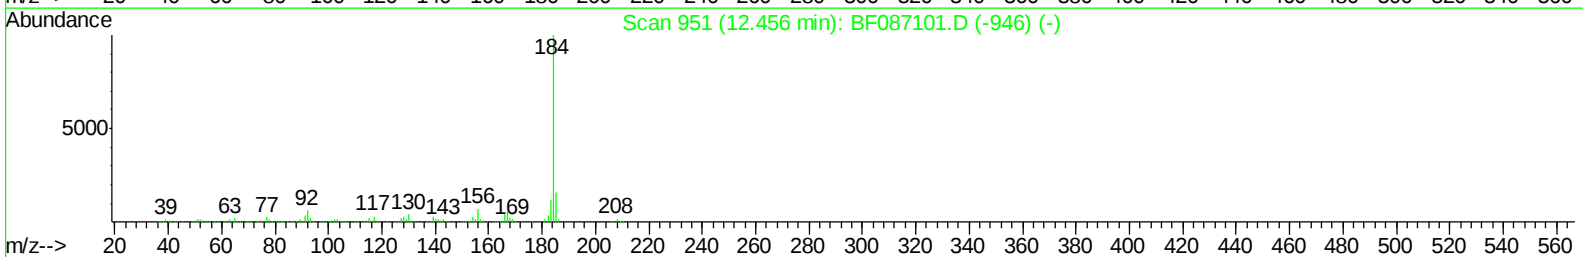
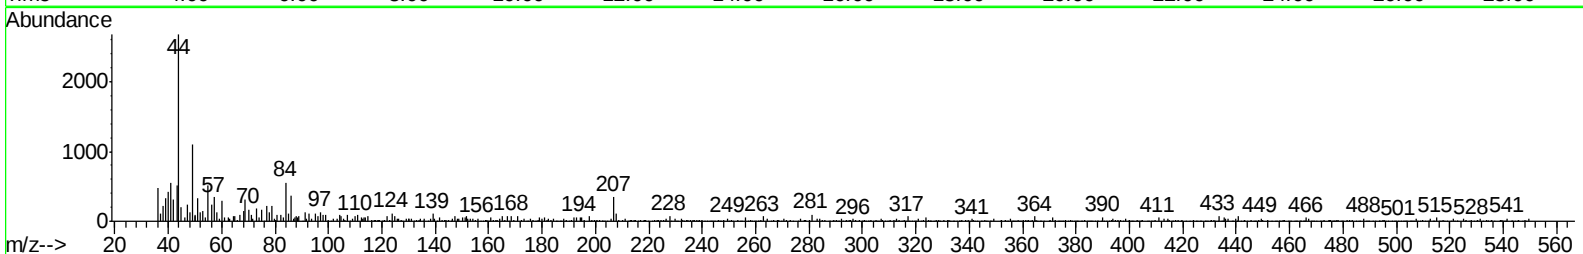


Data Path : Z:\HPCHEM1\BNA_E\Data\Be051816\
Data File : BE091790.D
Acq On : 18 May 2016 11:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 05:07:00 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

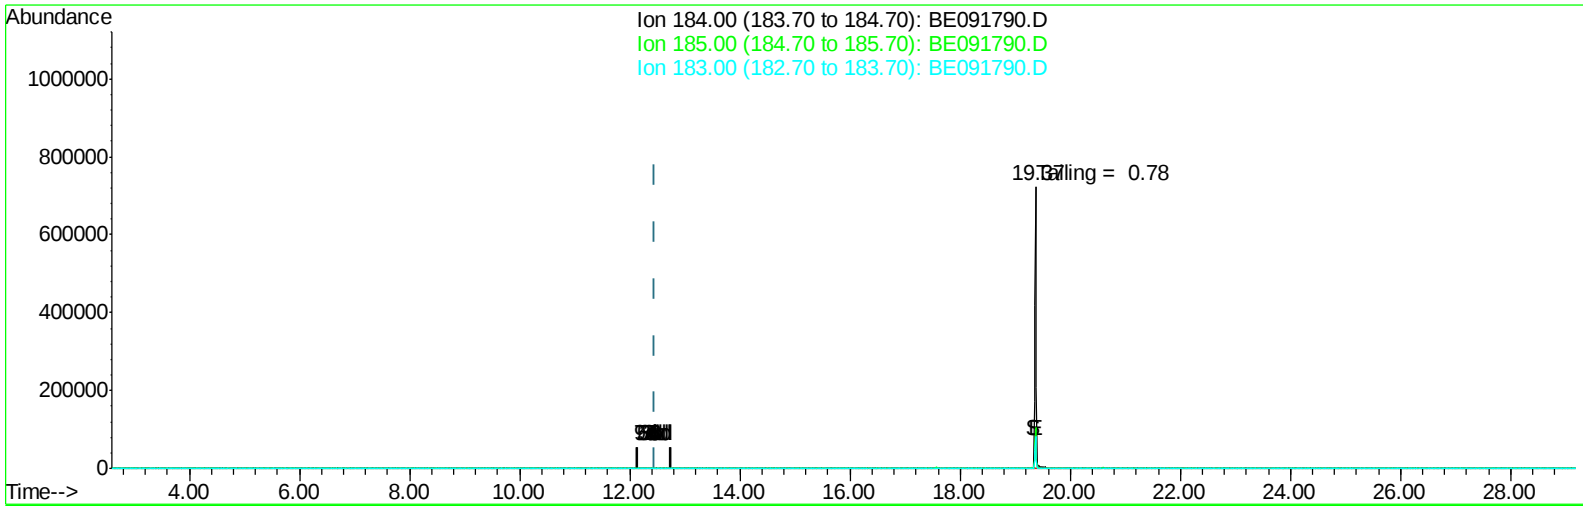

TIC: BE091790.D

(76) Benzidine




12.417min (-0.050) -20.00ng

response 26

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	20.00
183.00	12.20	57.50#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\Be051816\
Data File : BE091790.D
Acq On : 18 May 2016 11:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 05:07:00 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

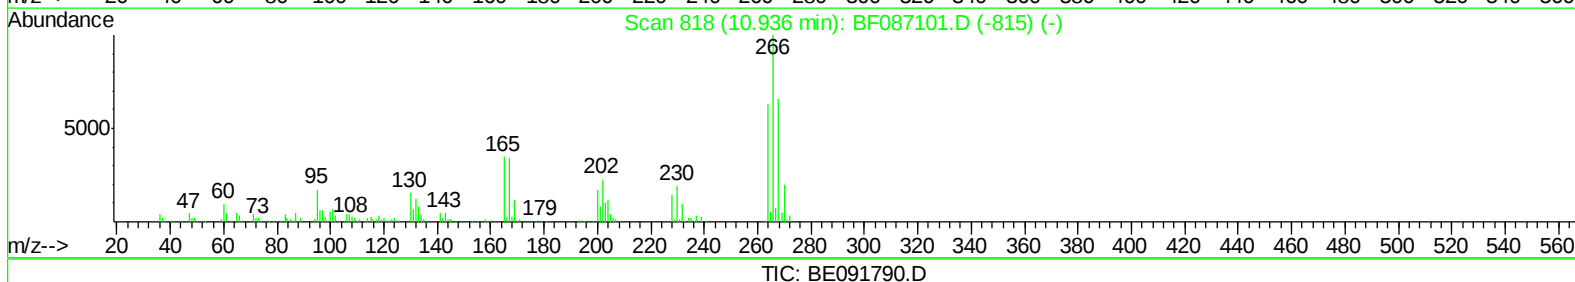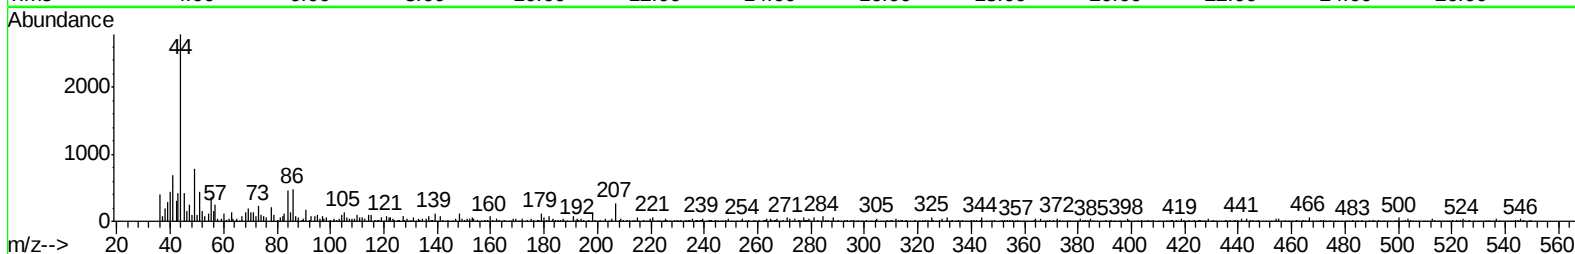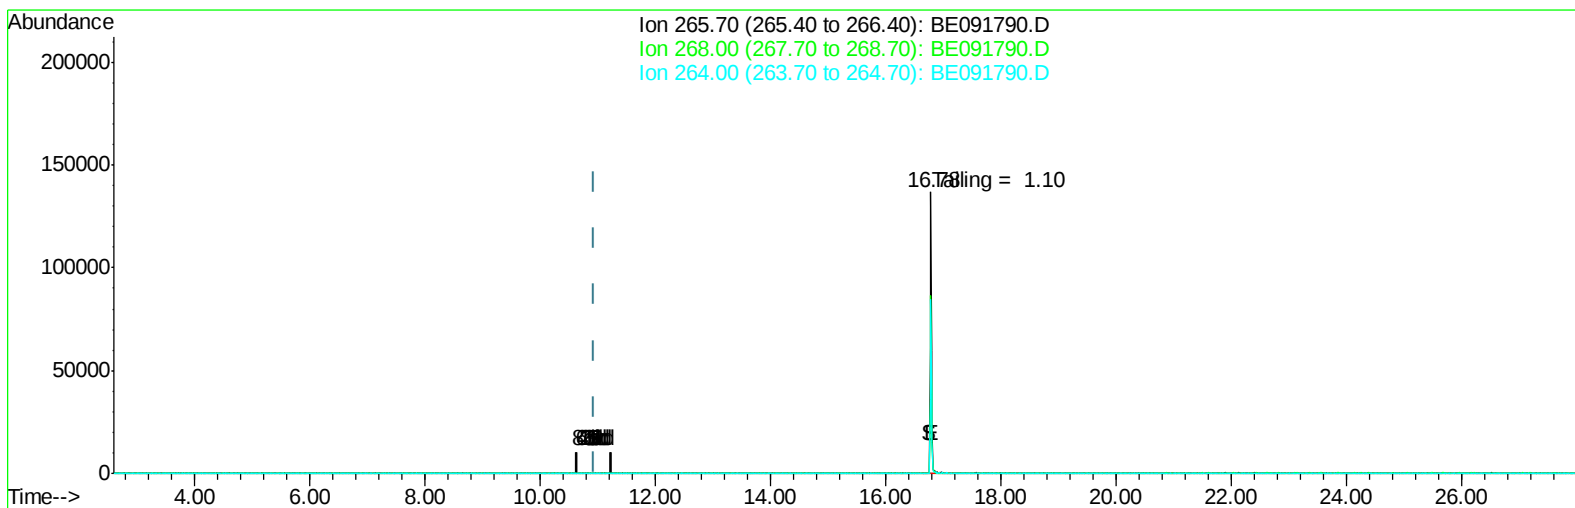

TIC: BE091790.D

(69) Pentachlorophenol (C)
10.930min (-0.018) 539.57ng
response 29

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	14.89#
264.00	66.10	0.00#
0.00	0.00	0.00