


Data Path : Z:\HPCHEM1\BNA E\Data\Be051816\
Data File : BE091790.D
Acq On : 18 May 2016 11:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 26 16:09:46 2016

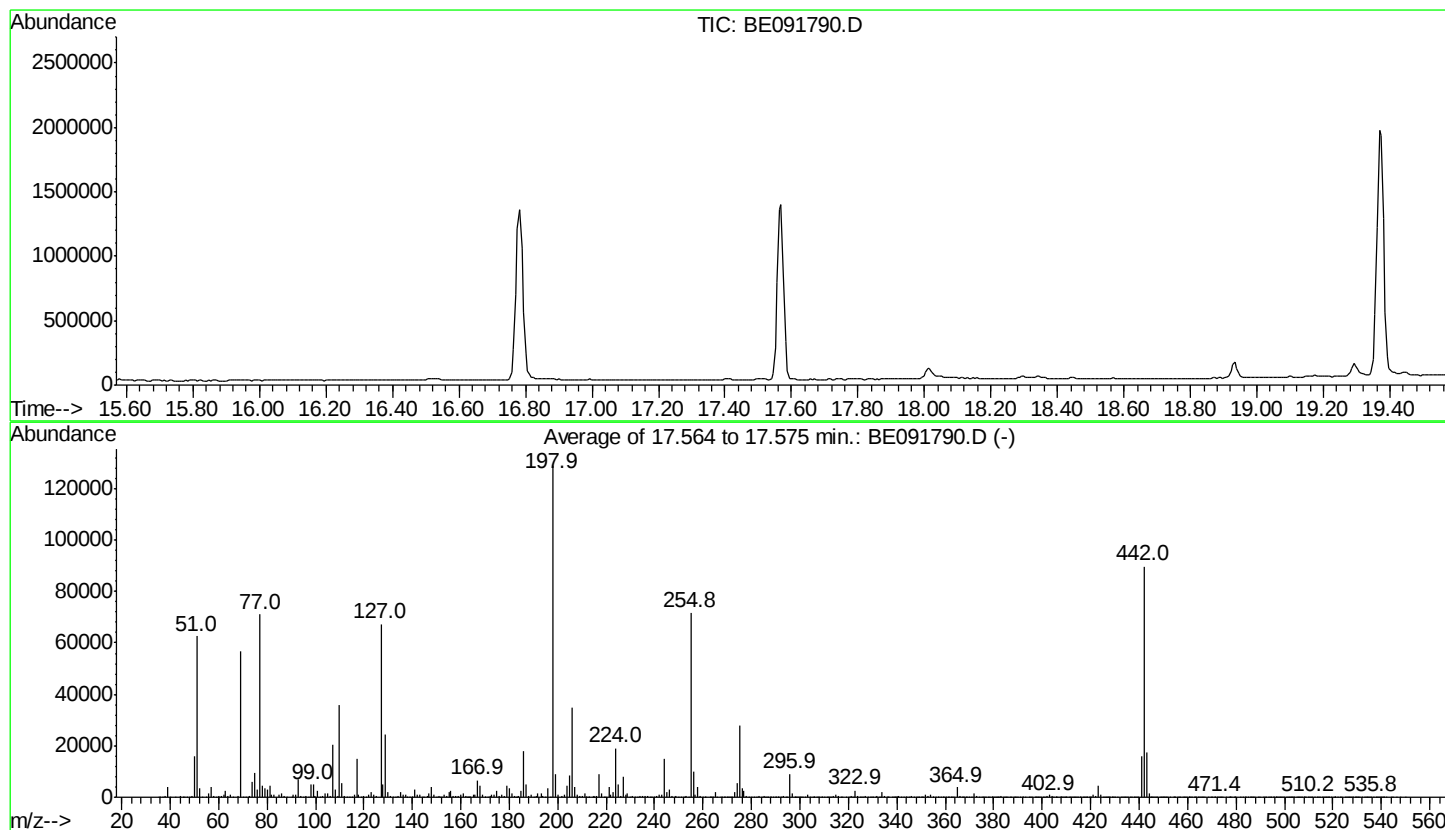

AutoFind: Scans 2549, 2550, 2551; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.6	62590	PASS
68	69	0.00	2	1.3	726	PASS
69	198	0.00	100	44.1	56801	PASS
70	69	0.00	2	0.3	196	PASS
127	198	10	80	52.2	67328	PASS
197	198	0.00	2	0.1	128	PASS
198	198	100	100	100.0	128918	PASS
199	198	5	9	7.1	9183	PASS
275	198	10	60	21.7	28014	PASS
365	198	1	100	3.1	3972	PASS
441	442	0.01	24	17.6	15815	PASS
442	198	50	100	69.6	89664	PASS
443	442	15	24	19.2	17204	PASS