


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051916\
 Data File : BE091799.D
 Acq On : 19 May 2016 8:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 19 15:36:49 2016

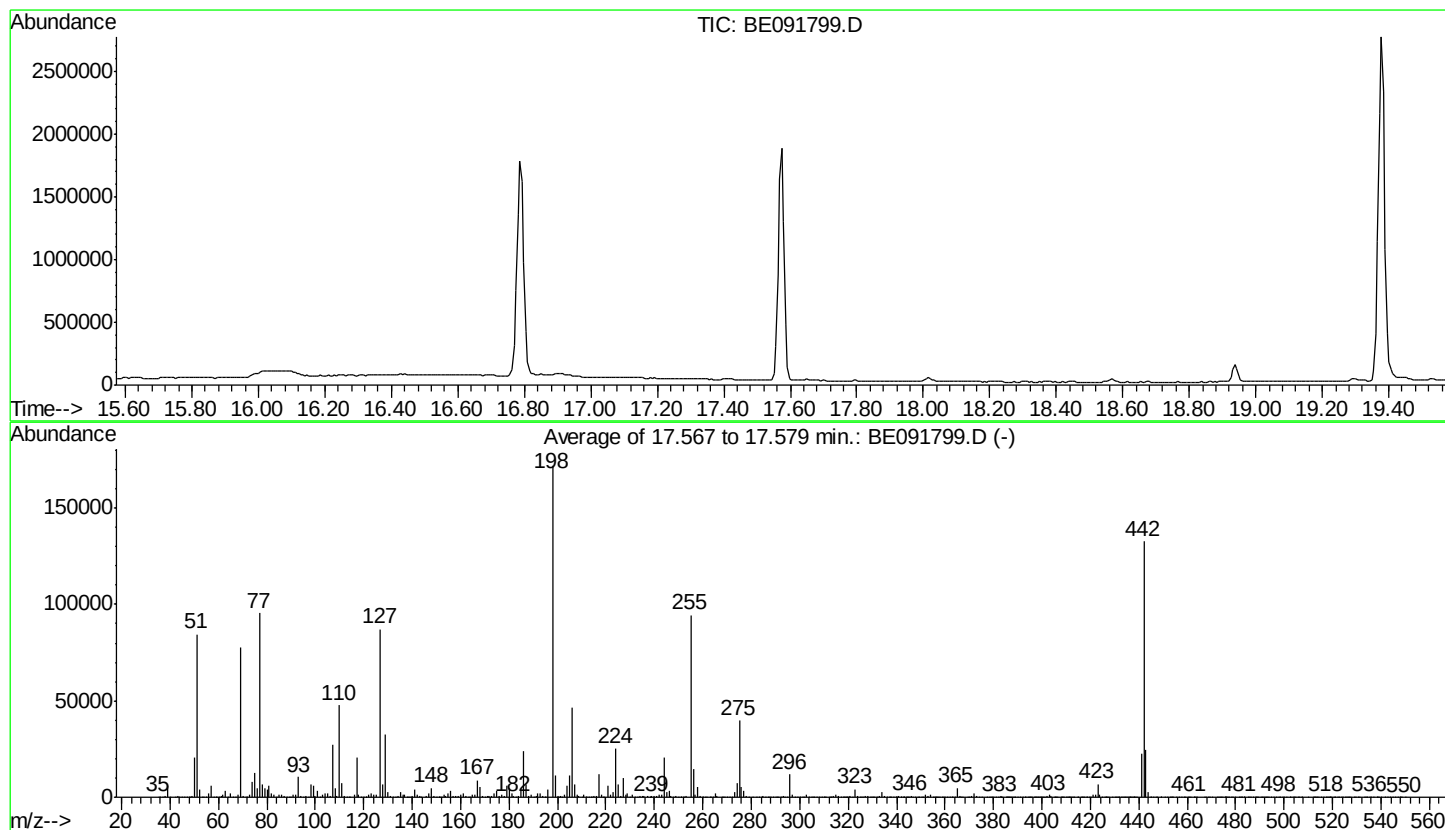

AutoFind: Scans 2549, 2550, 2551; Background Corrected with Scan 2541

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	84521	PASS
68	69	0.00	2	1.7	1285	PASS
69	198	0.00	100	45.1	77505	PASS
70	69	0.00	2	0.5	380	PASS
127	198	10	80	50.6	87002	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	171952	PASS
199	198	5	9	6.7	11602	PASS
275	198	10	60	23.1	39669	PASS
365	198	1	100	2.9	4926	PASS
441	442	0.01	24	17.1	22632	PASS
442	198	50	100	77.1	132570	PASS
443	442	15	24	18.7	24757	PASS