


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051916\
 Data File : BE091816.D
 Acq On : 19 May 2016 18:52
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 19 15:36:49 2016

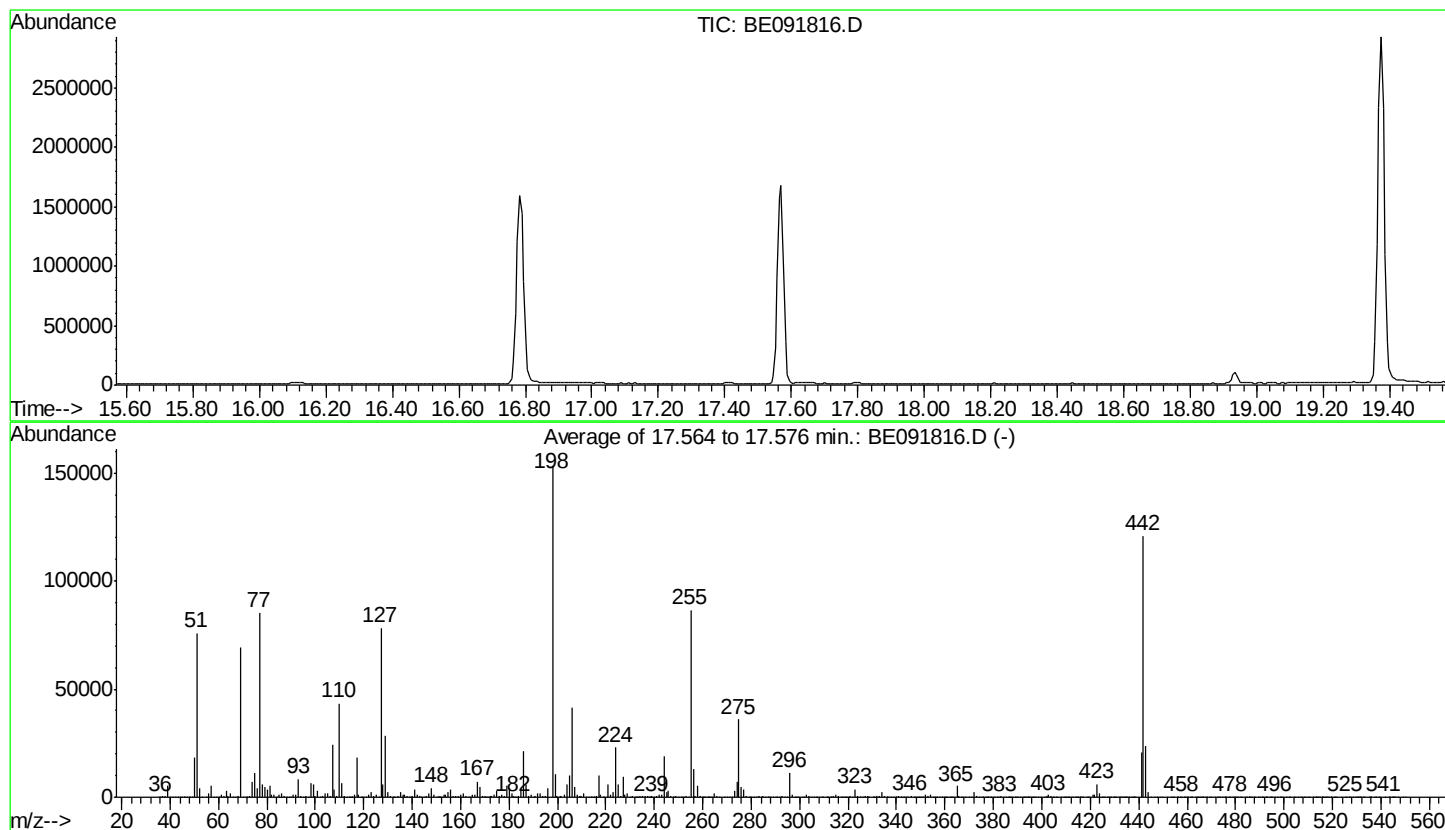

AutoFind: Scans 2549, 2550, 2551; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.6	76026	PASS
68	69	0.00	2	1.1	774	PASS
69	198	0.00	100	45.0	69039	PASS
70	69	0.00	2	0.4	262	PASS
127	198	10	80	51.0	78293	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	153410	PASS
199	198	5	9	7.0	10758	PASS
275	198	10	60	23.4	35951	PASS
365	198	1	100	3.3	5114	PASS
441	442	0.01	24	17.1	20701	PASS
442	198	50	100	78.9	121016	PASS
443	442	15	24	19.5	23648	PASS