


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051916\
 Data File : BE091830.D
 Acq On : 20 May 2016 4:45
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 19 15:36:49 2016

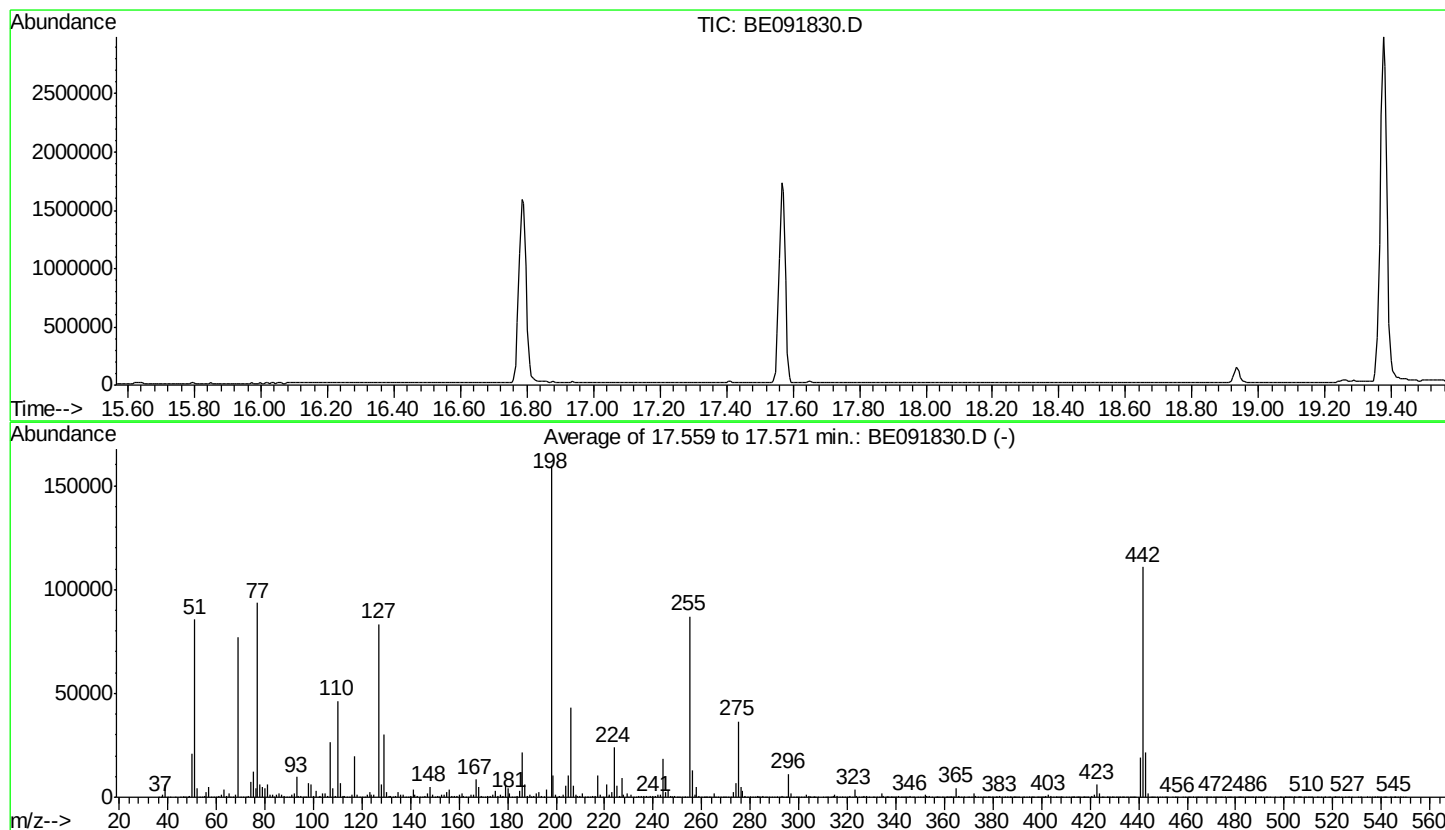

AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	85505	PASS
68	69	0.00	2	1.9	1468	PASS
69	198	0.00	100	48.3	77155	PASS
70	69	0.00	2	0.3	224	PASS
127	198	10	80	52.2	83394	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	159689	PASS
199	198	5	9	6.7	10744	PASS
275	198	10	60	22.9	36532	PASS
365	198	1	100	2.9	4589	PASS
441	442	0.01	24	17.3	19138	PASS
442	198	50	100	69.3	110680	PASS
443	442	15	24	19.6	21651	PASS