


Data Path : Z:\HPCHEM1\BNA E\DATA\BE051917\
 Data File : BE093053.D
 Acq On : 19 May 2017 9:02
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 15 13:35:57 2017

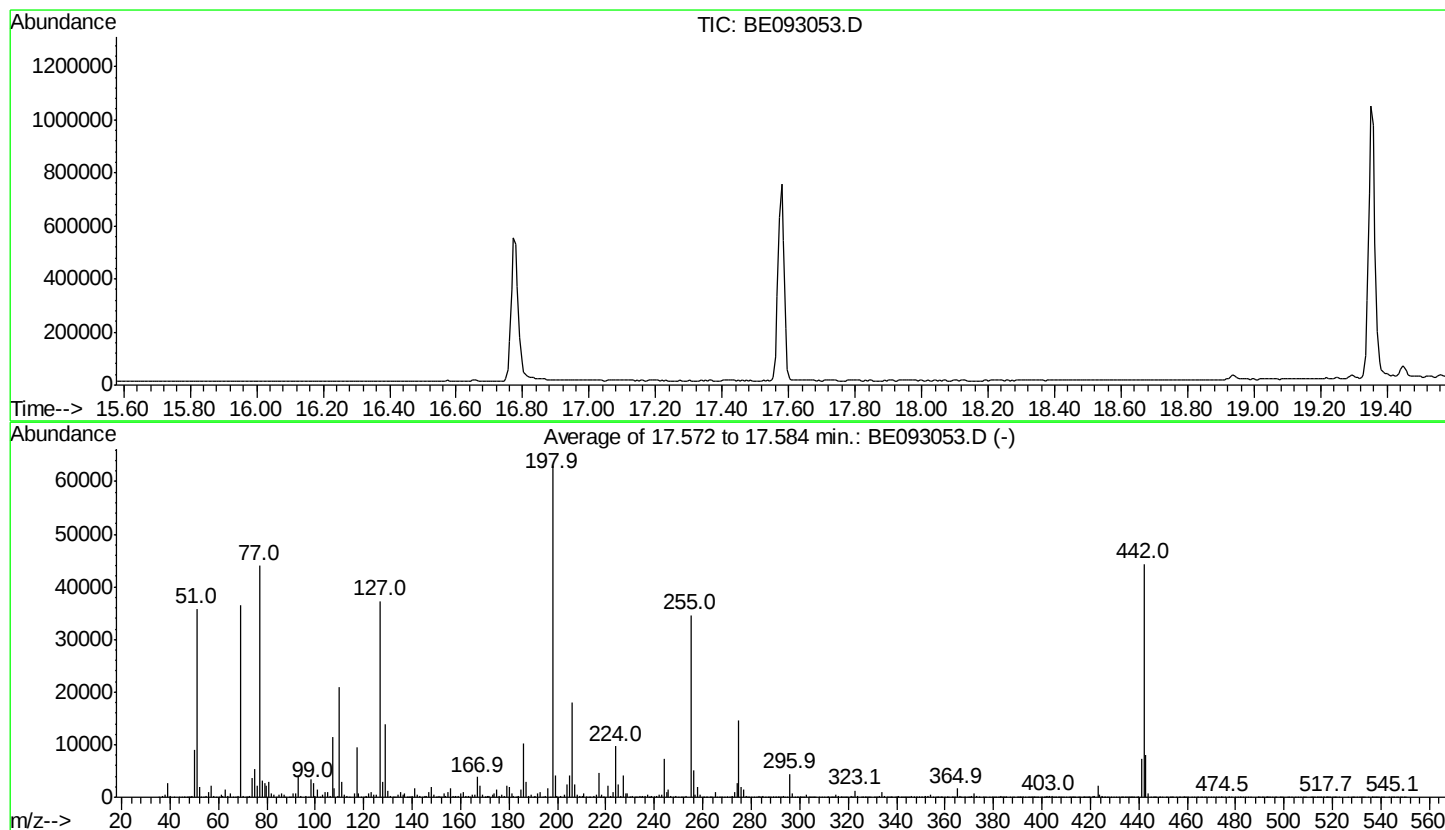

AutoFind: Scans 2550, 2551, 2552; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.8	35827	PASS
68	69	0.00	2	0.5	188	PASS
69	198	0.00	100	58.0	36548	PASS
70	69	0.00	2	0.6	202	PASS
127	198	10	80	59.1	37256	PASS
197	198	0.00	2	0.2	117	PASS
198	198	100	100	100.0	63043	PASS
199	198	5	9	6.5	4128	PASS
275	198	10	60	23.1	14536	PASS
365	198	1	100	2.6	1630	PASS
441	442	0.01	24	16.6	7369	PASS
442	198	50	100	70.3	44320	PASS
443	442	15	24	18.3	8097	PASS