
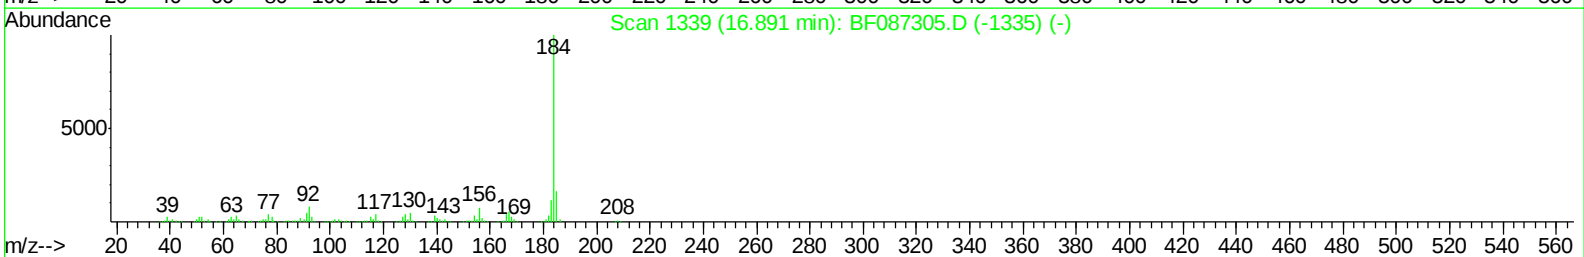
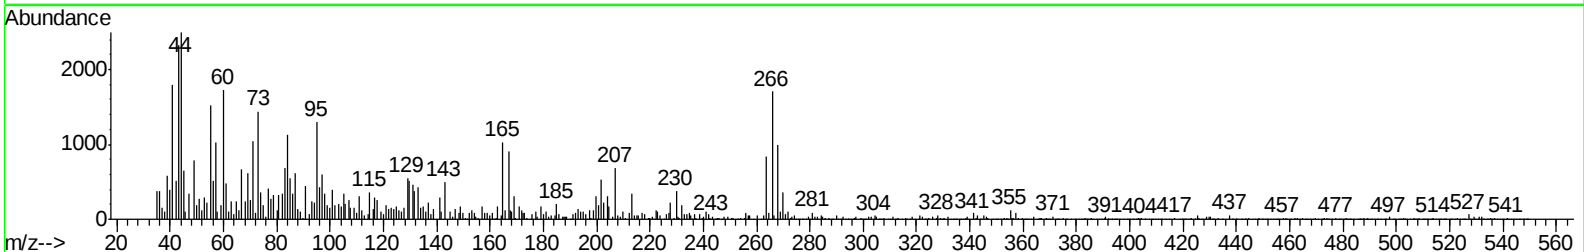


```
Data Path : Z:\HPCHEM1\BNA_E\DATA\BE052316\  
Data File : BE091841.D  
Acq On    : 23 May 2016  11:00  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: May 24 05:44:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 24 01:40:43 2016
Response via : Initial Calibration

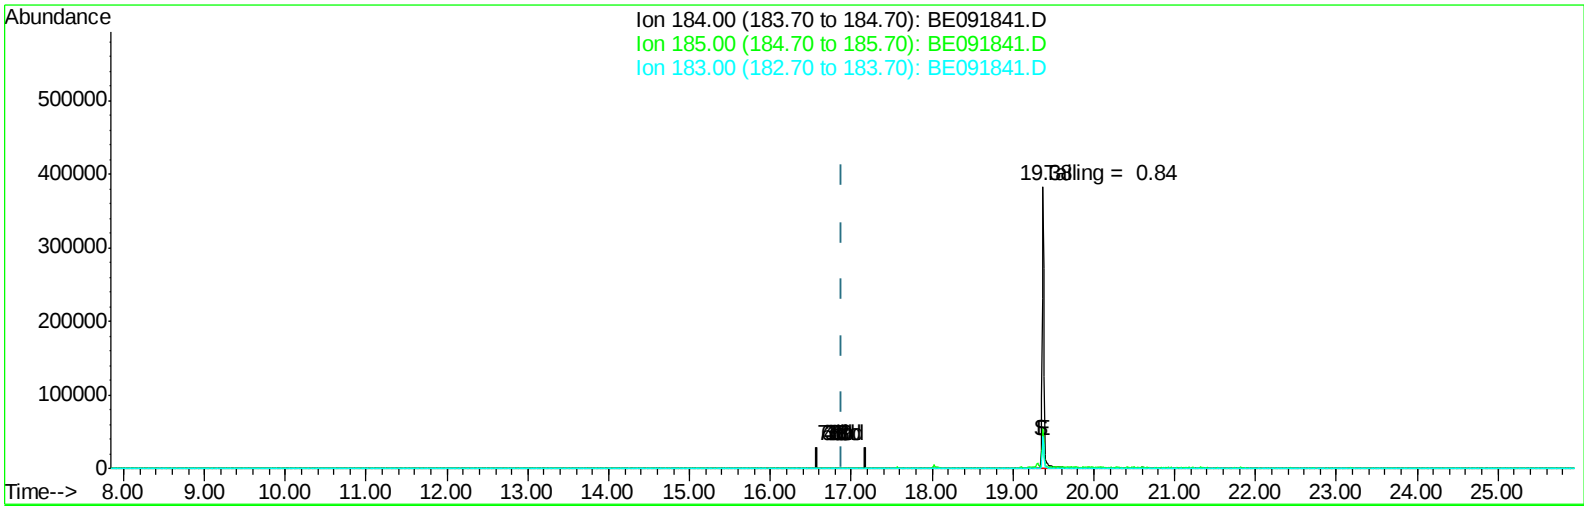

TIC: BE091841.D

(76) Benzidine




16.855min (-0.036) 5.81ng

response 13

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	452.17#
183.00	12.20	119.57#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE052316\
Data File : BE091841.D
Acq On : 23 May 2016 11:00
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 05:44:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 24 01:40:43 2016
Response via : Initial Calibration

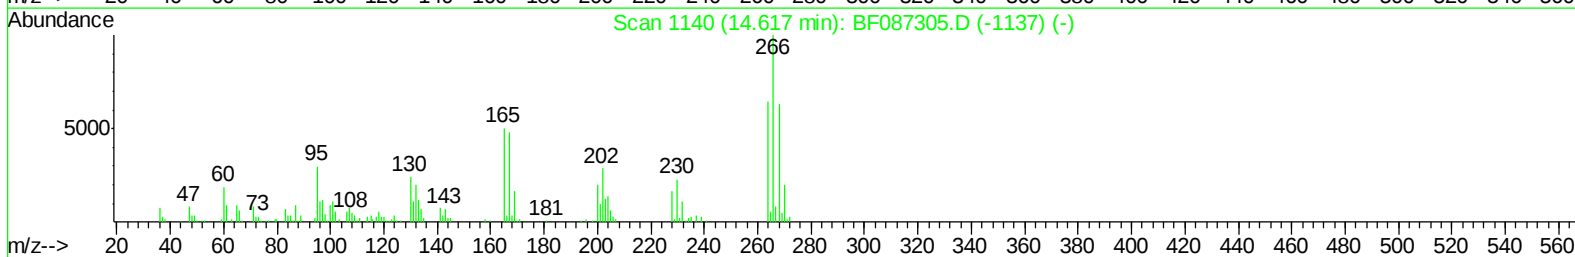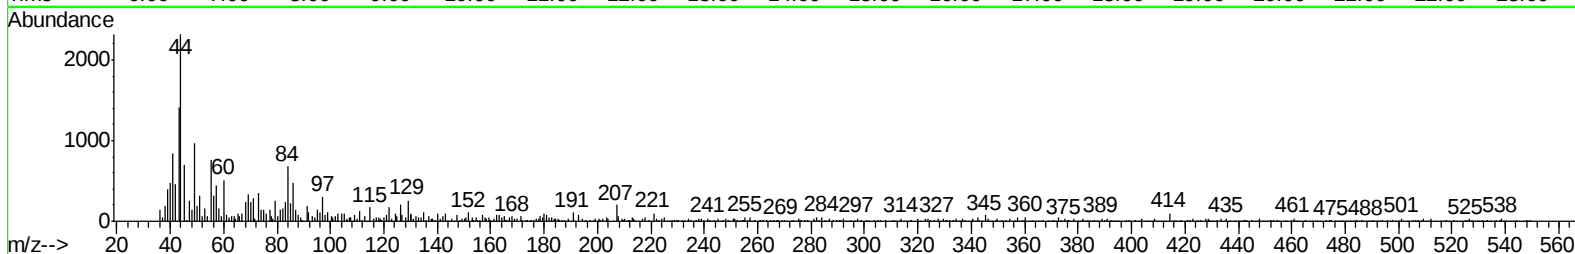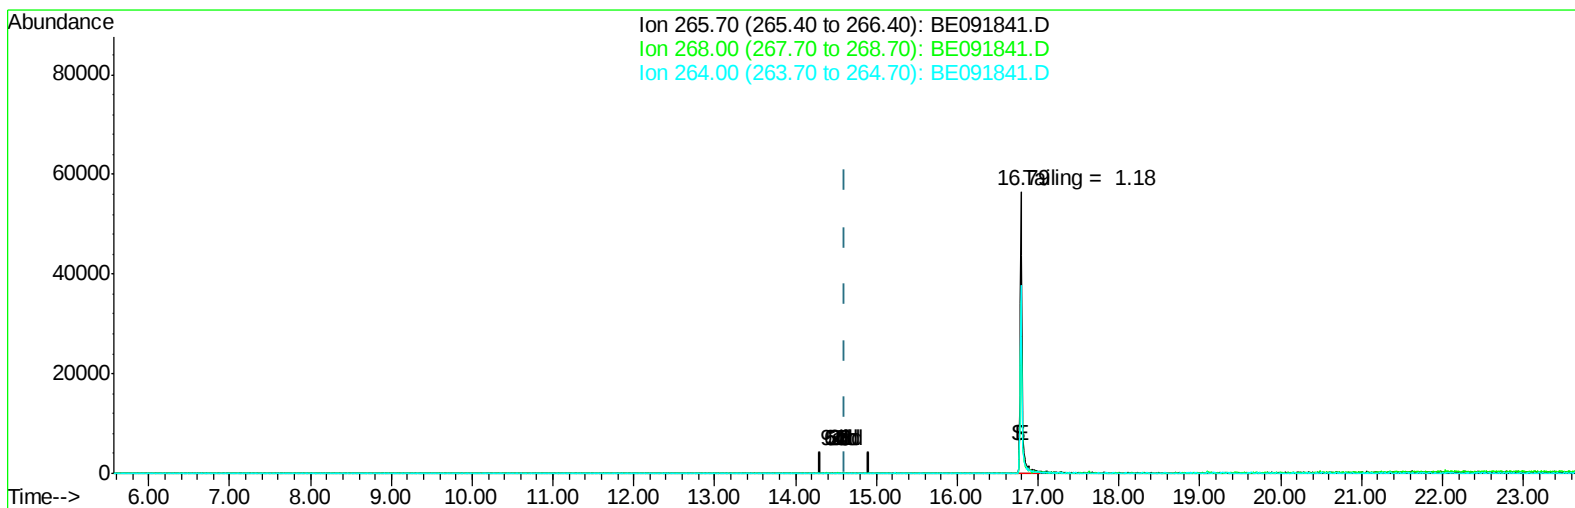

TIC: BE091841.D

(69) Pentachlorophenol (C)

14.593min (-0.023) 94.52ng

response 16

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	44.00#
264.00	66.10	68.00
0.00	0.00	0.00