


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE052316\
Data File : BE091841.D
Acq On : 23 May 2016 11:00
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 19 15:36:49 2016

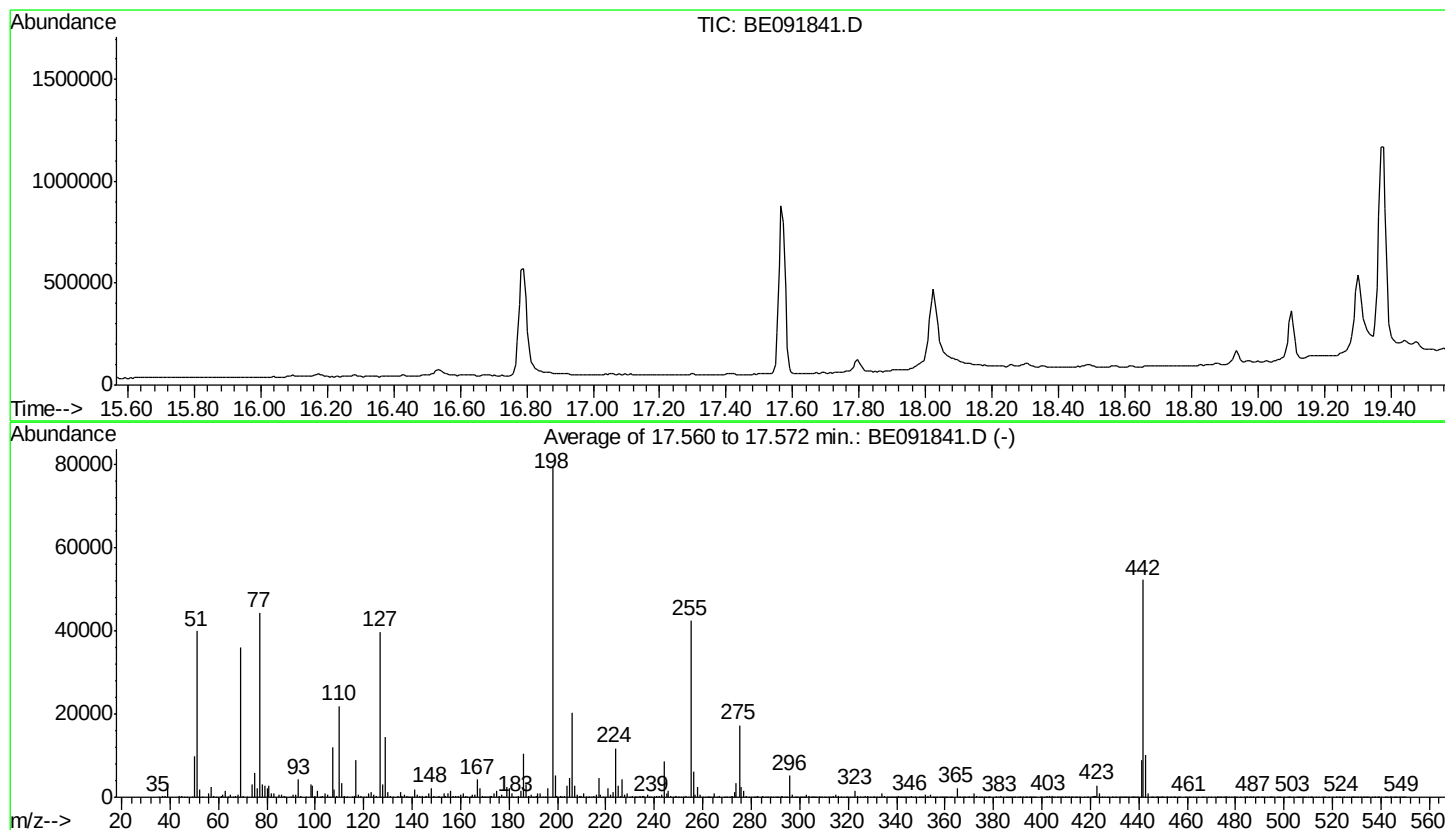

AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	39917	PASS
68	69	0.00	2	1.9	686	PASS
69	198	0.00	100	45.2	36075	PASS
70	69	0.00	2	0.6	223	PASS
127	198	10	80	49.9	39783	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	79747	PASS
199	198	5	9	6.8	5399	PASS
275	198	10	60	21.6	17252	PASS
365	198	1	100	2.7	2173	PASS
441	442	0.01	24	16.8	8789	PASS
442	198	50	100	65.6	52299	PASS
443	442	15	24	19.5	10181	PASS