
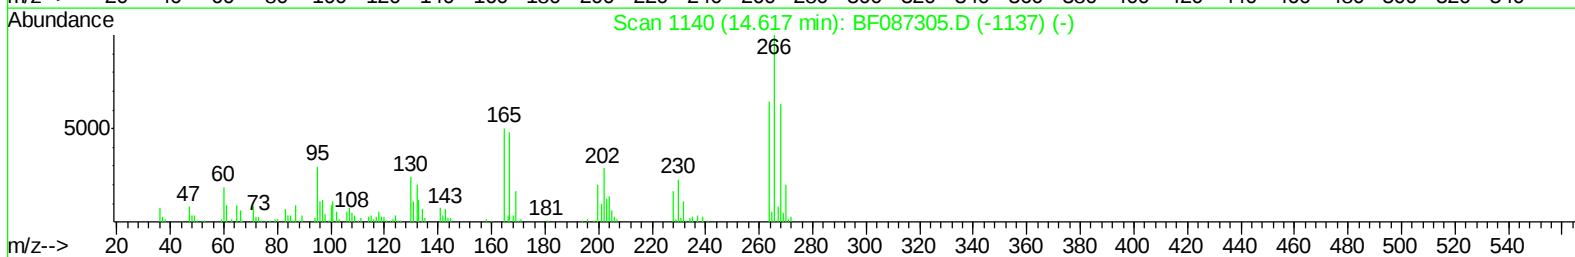
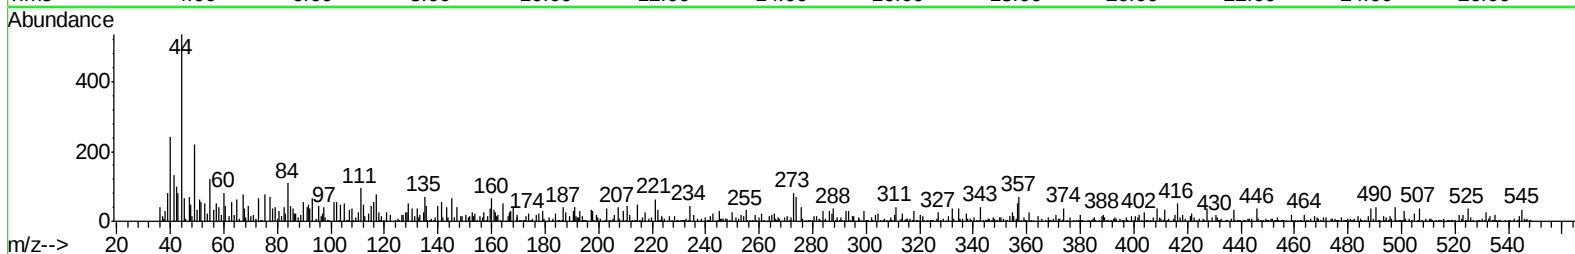


Data Path : Z:\HPCHEM1\BNA_E\Data\BE052516\
Data File : BE091853.D
Acq On : 25 May 2016 9:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 04:03:01 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

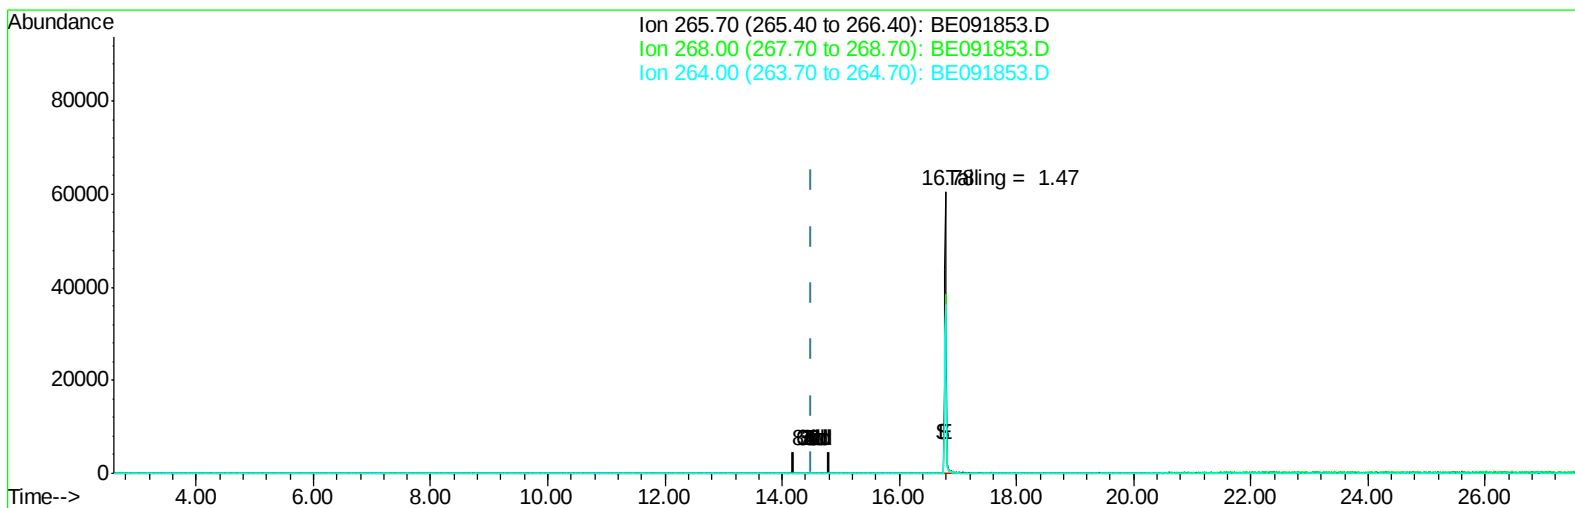

TIC: BE091853.D

(69) Pentachlorophenol (C)

14.515min (+0.001) 125.41ng

response 17

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	34.48#
264.00	66.10	44.83#
0.00	0.00	0.00