
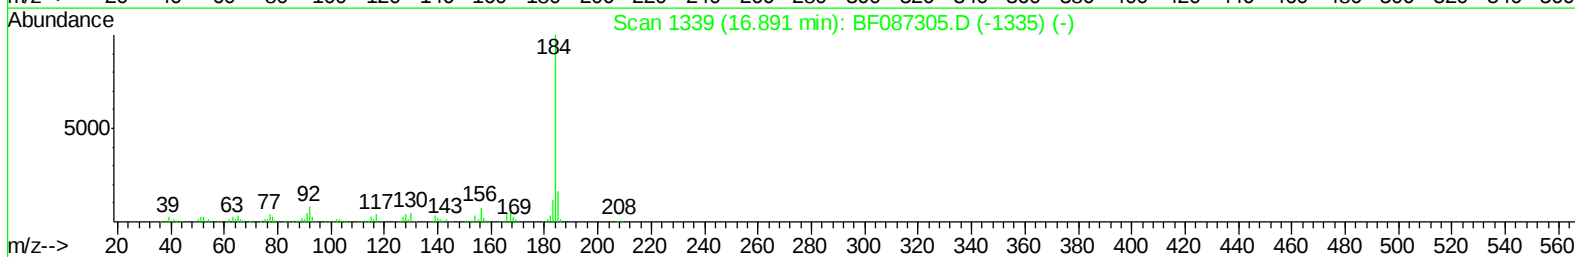
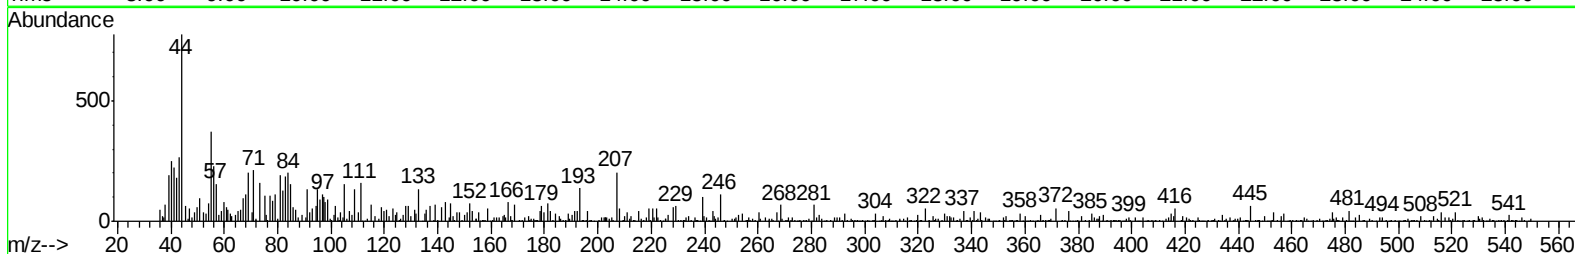


Data Path : Z:\HPCHEM1\BNA_E\Data\BE052516\
Data File : BE091868.D
Acq On : 25 May 2016 21:05
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 04:07:38 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

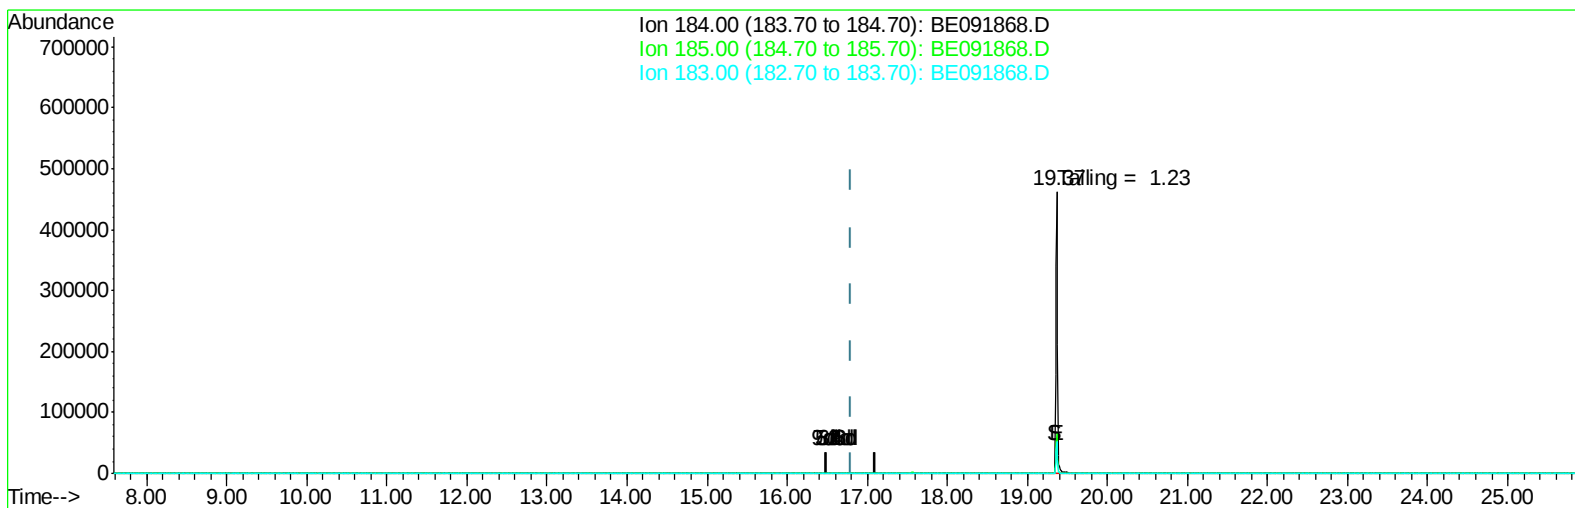

TIC: BE091868.D

(76) Benzidine




16.621min (-0.190) 44.84ng

response 30

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	72.73#
183.00	12.20	21.21#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE052516\
Data File : BE091868.D
Acq On : 25 May 2016 21:05
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 04:07:38 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

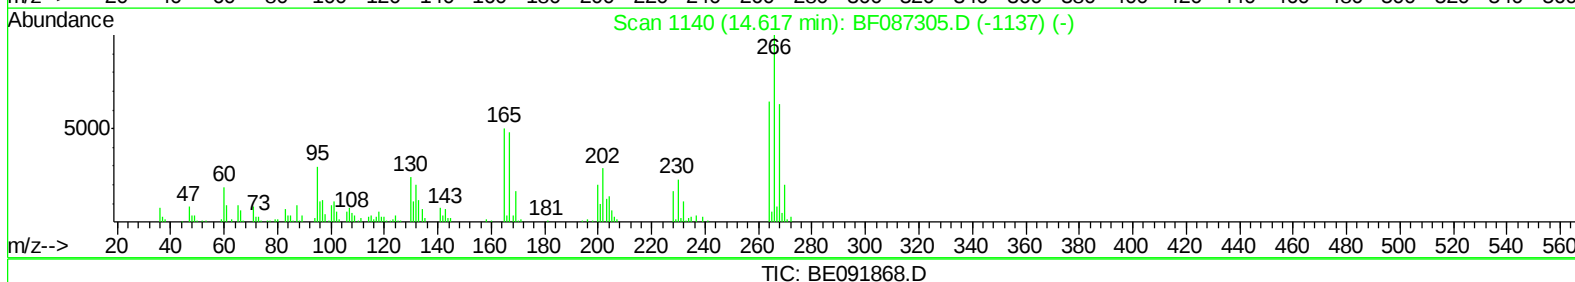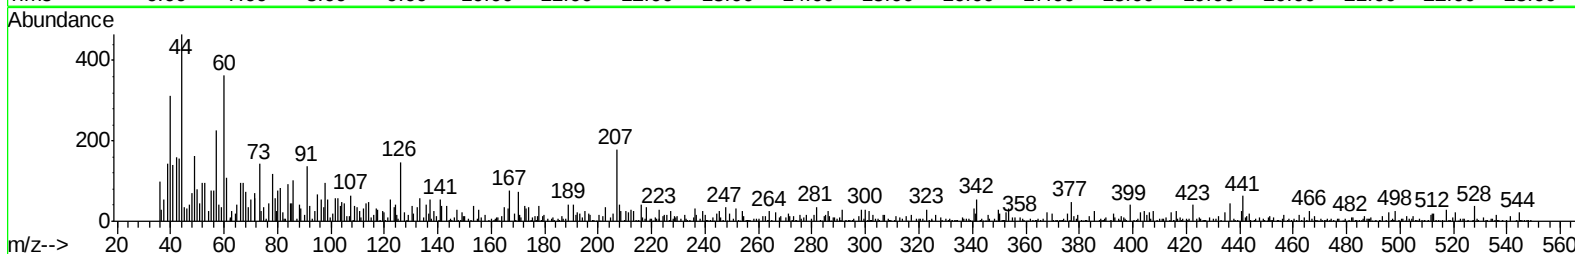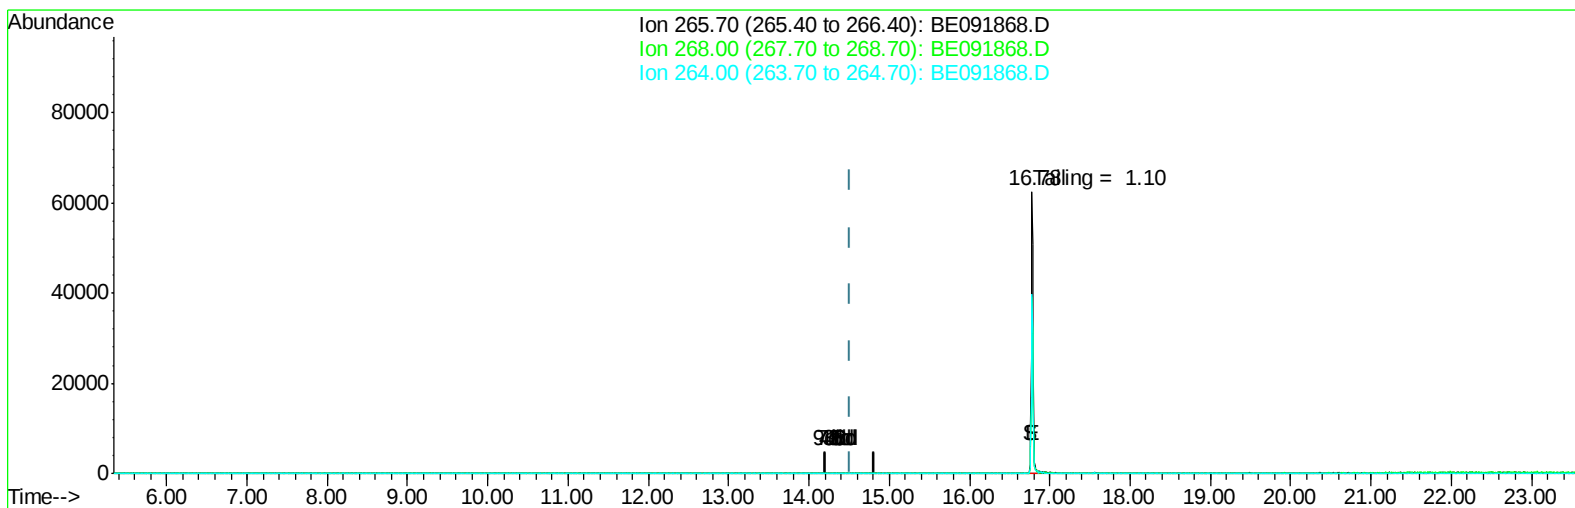

TIC: BE091868.D

(69) Pentachlorophenol (C)
14.348min (-0.166) 590.06ng
response 18

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	52.17
264.00	66.10	104.35#
0.00	0.00	0.00