


Data Path : Z:\HPCHEM1\BNA E\DATA\BE052516\
 Data File : BE091853.D
 Acq On : 25 May 2016 9:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE052516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 19:42:30 2016

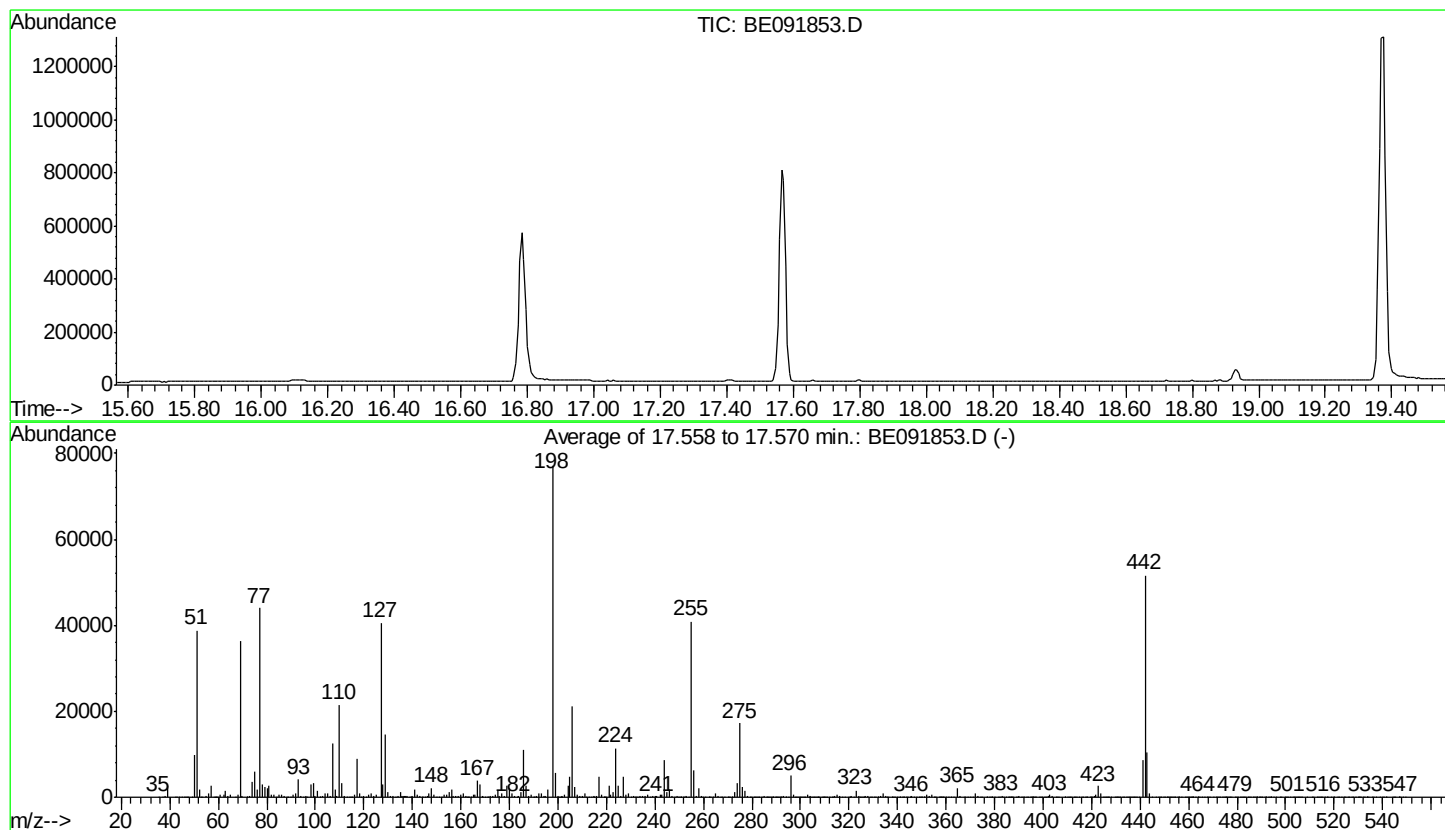

AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	38745	PASS
68	69	0.00	2	1.6	596	PASS
69	198	0.00	100	47.0	36272	PASS
70	69	0.00	2	0.8	306	PASS
127	198	10	80	52.7	40641	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	77141	PASS
199	198	5	9	7.3	5627	PASS
275	198	10	60	22.2	17156	PASS
365	198	1	100	2.9	2205	PASS
441	442	0.01	24	17.0	8795	PASS
442	198	50	100	66.9	51626	PASS
443	442	15	24	20.3	10464	PASS