


Data Path : Z:\HPCHEM1\BNA E\DATA\BE052516\
 Data File : BE091868.D
 Acq On : 25 May 2016 21:05
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE052516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 19:42:30 2016

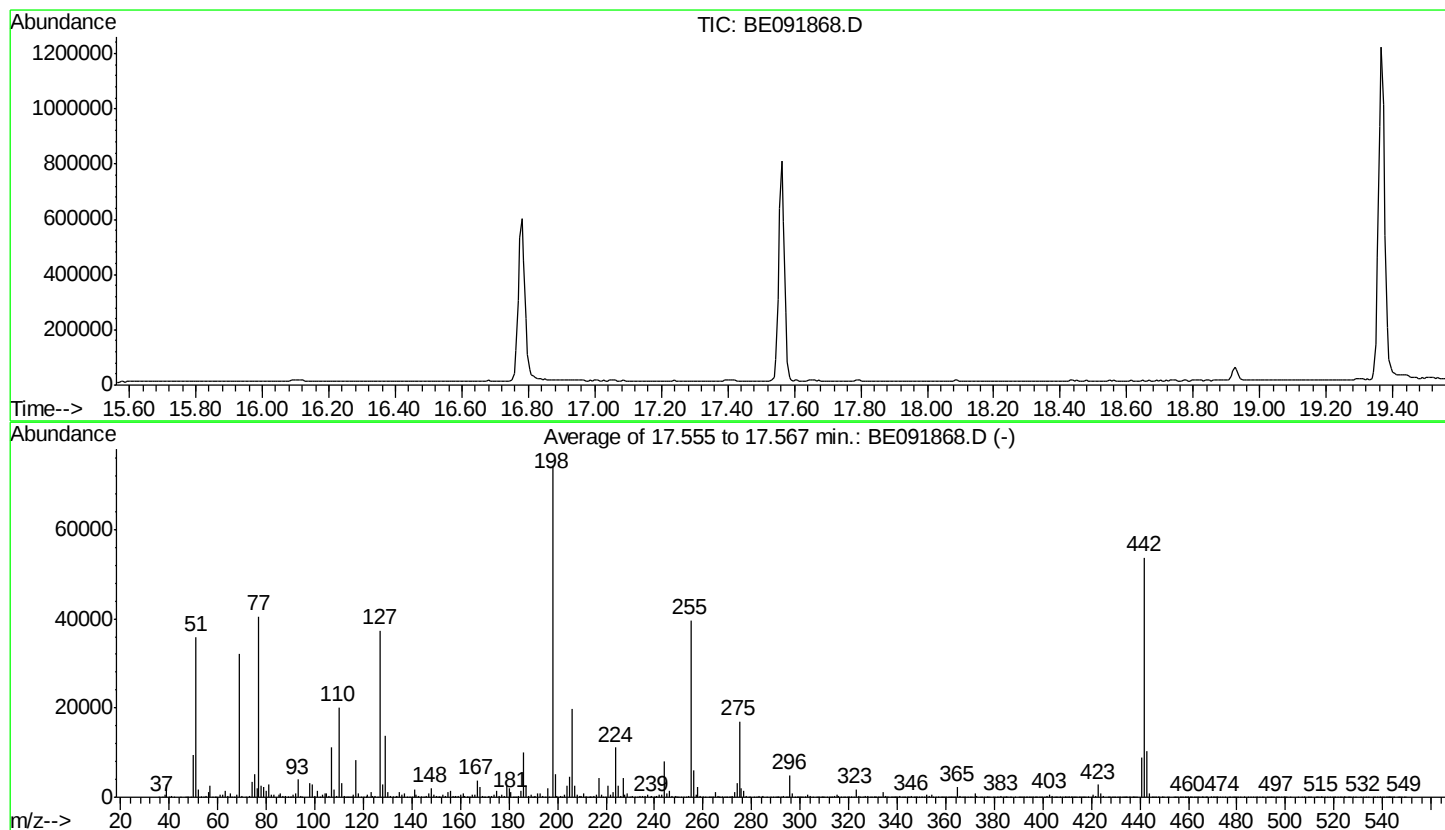

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	35919	PASS
68	69	0.00	2	1.7	551	PASS
69	198	0.00	100	43.3	32172	PASS
70	69	0.00	2	0.5	165	PASS
127	198	10	80	50.4	37434	PASS
197	198	0.00	2	0.2	146	PASS
198	198	100	100	100.0	74320	PASS
199	198	5	9	7.0	5191	PASS
275	198	10	60	22.8	16970	PASS
365	198	1	100	3.2	2406	PASS
441	442	0.01	24	16.6	8903	PASS
442	198	50	100	72.4	53794	PASS
443	442	15	24	19.4	10411	PASS