
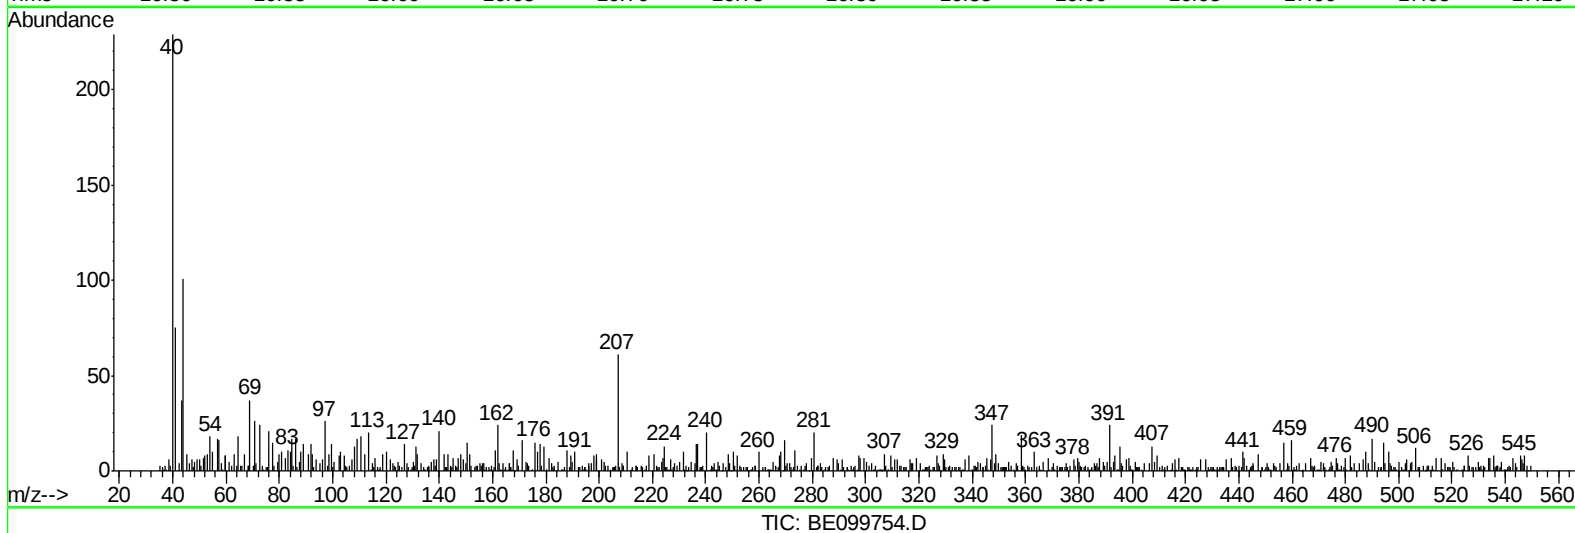


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE052819\
Data File : BE099754.D
Acq On : 28 May 2019 13:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 03:50:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

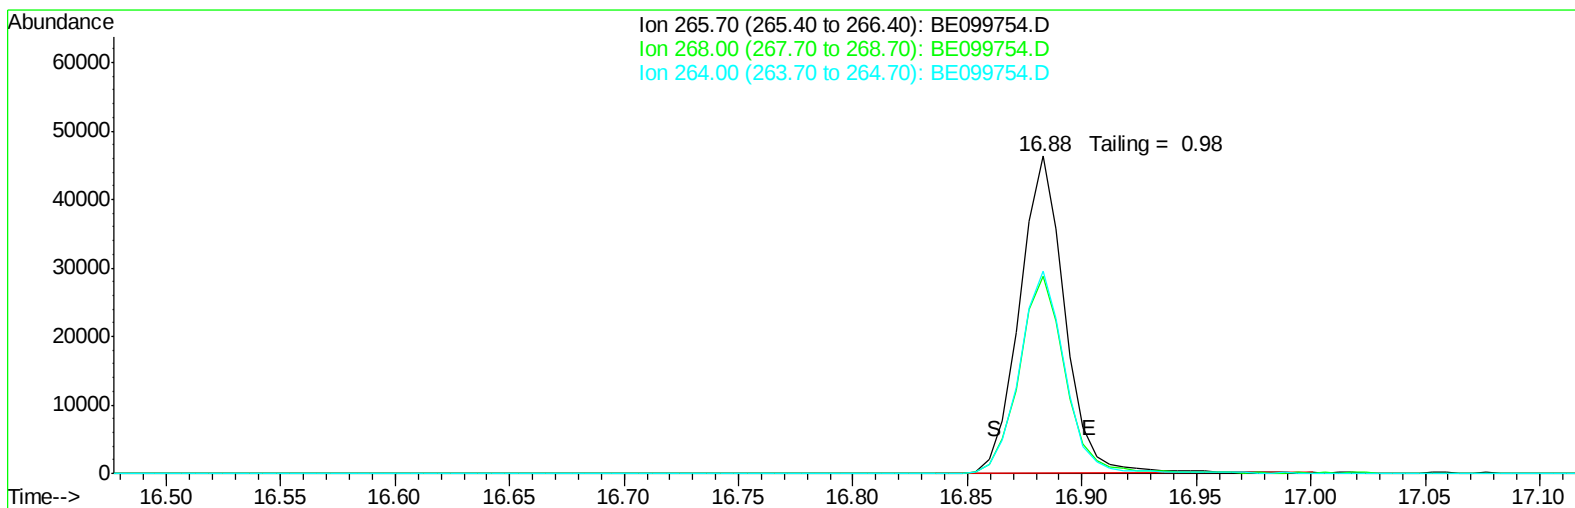

(69) Pentachlorophenol (C)



12.094min (+0.007) 60.12ng

response 7

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	180.00#
264.00	65.00	30.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE052819\
Data File : BE099754.D
Acq On : 28 May 2019 13:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 03:50:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

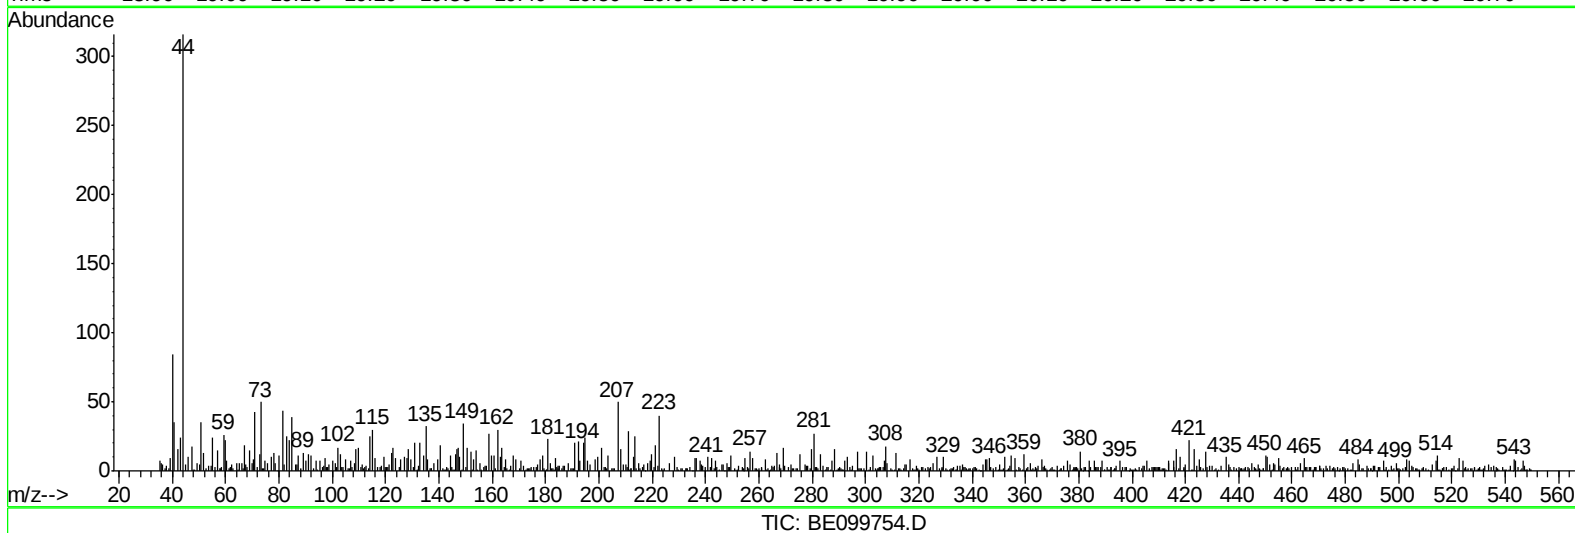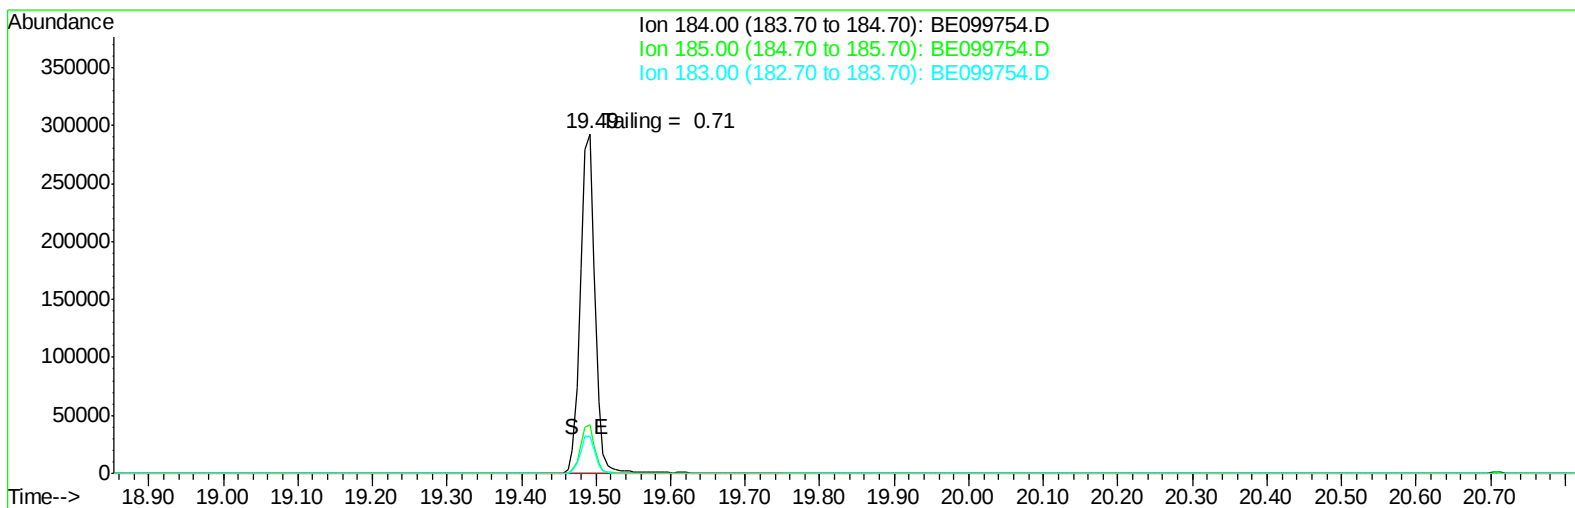

TIC: BE099754.D

(76) Benzidine

14.574min (-0.016) 21.92ng

response 8

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	57.14#
183.00	12.20	85.71#
0.00	0.00	0.00