


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE052819\
 Data File : BE099754.D
 Acq On : 28 May 2019 13:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE052019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 20 19:29:40 2019

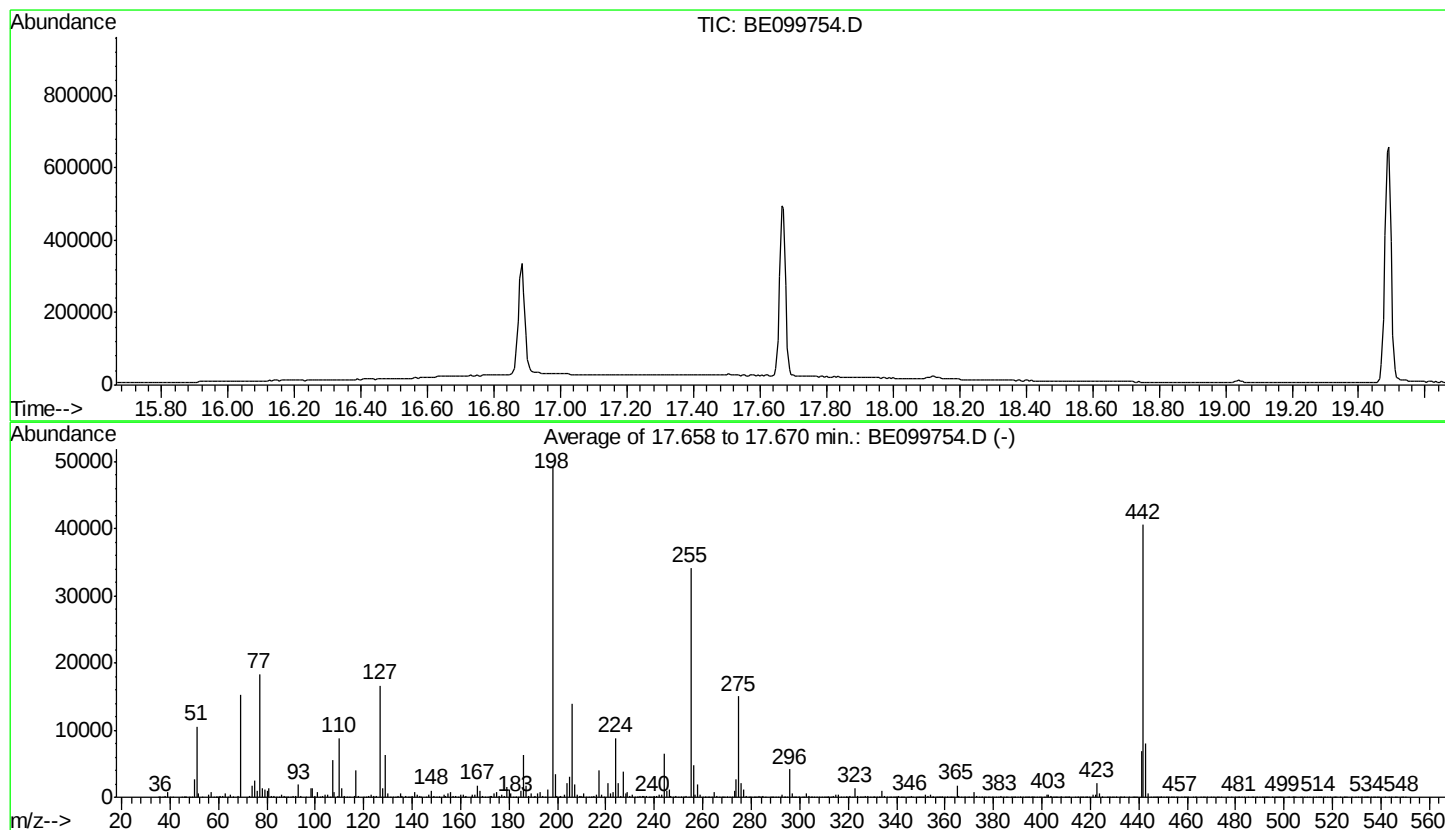

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	10583	PASS
68	69	0.00	2	1.6	244	PASS
69	198	0.00	100	30.7	15178	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.6	16616	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49386	PASS
199	198	5	9	6.8	3347	PASS
275	198	10	60	30.5	15046	PASS
365	198	1	100	3.5	1741	PASS
441	198	0.01	100	14.0	6891	PASS
442	198	50	100	82.2	40592	PASS
443	442	15	24	19.8	8056	PASS